

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017216.D
 Acq On : 18 Sep 2023 21:25
 Operator : MA/JU
 Sample : 04330-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	35	38	46	rVB	37247	56527	1.41%	0.132%
2	3.758	110	114	122	rBV3	50485	82517	2.05%	0.193%
3	3.858	127	131	139	rVB	87807	121404	3.02%	0.283%
4	3.940	139	145	155	rVB	94026	148054	3.69%	0.346%
5	4.058	162	165	173	rVB	18103	24669	0.61%	0.058%
6	4.440	227	230	237	rVB5	14920	24245	0.60%	0.057%
7	4.640	260	264	267	rBV3	13038	17950	0.45%	0.042%
8	4.993	319	324	327	rBV	50171	71161	1.77%	0.166%
9	5.034	327	331	335	rVB	30785	43756	1.09%	0.102%
10	5.111	341	344	349	rBV3	8696	11779	0.29%	0.027%
11	5.452	399	402	407	rBV5	6034	8241	0.21%	0.019%
12	5.575	420	423	430	rVB	11127	14458	0.36%	0.034%
13	6.787	625	629	633	rBV7	5673	8517	0.21%	0.020%
14	6.905	646	649	653	rVB6	4937	7840	0.20%	0.018%
15	7.099	675	682	695	rBV	576886	953764	23.74%	2.227%
16	7.287	708	714	727	rBV	505084	773233	19.25%	1.805%
17	7.463	736	744	753	rBV	612571	973812	24.24%	2.273%
18	7.546	755	758	767	rVV2	8005	16022	0.40%	0.037%
19	7.752	788	793	799	rBV4	7999	14868	0.37%	0.035%
20	7.946	818	826	834	rBV	1135876	1769085	44.04%	4.130%
21	8.652	940	946	962	rBV	334303	579749	14.43%	1.353%
22	8.793	964	970	980	rBV	159416	256324	6.38%	0.598%
23	8.940	991	995	996	rBV4	3466	4714	0.12%	0.011%
24	9.140	1021	1029	1040	rBV	571294	951465	23.69%	2.221%
25	9.222	1040	1043	1045	rVV4	4705	5787	0.14%	0.014%
26	9.257	1047	1049	1054	rVB5	5155	5958	0.15%	0.014%
27	9.352	1059	1065	1068	rBV8	5412	8936	0.22%	0.021%
28	9.675	1116	1120	1124	rVB7	2689	4105	0.10%	0.010%
29	9.857	1142	1151	1159	rBV	454295	748064	18.62%	1.746%
30	9.993	1168	1174	1178	rBV2	16346	30917	0.77%	0.072%
31	10.228	1204	1214	1218	rVB2	11624	25323	0.63%	0.059%
32	10.381	1233	1240	1255	rBV	689763	1150810	28.65%	2.687%
33	10.769	1298	1306	1314	rBV	1559953	2555689	63.62%	5.967%
34	10.934	1326	1334	1350	rBV	455357	828749	20.63%	1.935%
35	11.316	1395	1399	1400	rBV4	4074	5302	0.13%	0.012%
36	11.522	1430	1434	1440	rBV9	7523	10701	0.27%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017216.D
 Acq On : 18 Sep 2023 21:25
 Operator : MA/JU
 Sample : 04330-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	11.593	1443	1446	1447	rBV3	5597	6295	0.16%	0.015%
38	11.804	1476	1482	1488	rBV3	5177	9351	0.23%	0.022%
39	11.904	1494	1499	1507	rVB3	2431	5795	0.14%	0.014%
40	12.175	1541	1545	1550	rVB8	6648	11001	0.27%	0.026%

41	12.351	1568	1575	1585	rVB2	14985	26001	0.65%	0.061%
42	12.569	1607	1612	1614	rBV6	3352	6473	0.16%	0.015%
43	12.922	1669	1672	1676	rBV6	3162	4559	0.11%	0.011%
44	13.057	1692	1695	1699	rBV6	4221	5755	0.14%	0.013%
45	13.175	1713	1715	1720	rVB6	4938	6354	0.16%	0.015%

46	13.363	1742	1747	1750	rBV7	5640	8739	0.22%	0.020%
47	13.445	1755	1761	1770	rVV2	79585	131274	3.27%	0.306%
48	13.787	1814	1819	1823	rBV6	11973	17152	0.43%	0.040%
49	13.928	1837	1843	1846	rBV8	7768	11581	0.29%	0.027%
50	14.016	1852	1858	1867	rBV	1354545	1811766	45.10%	4.230%

51	14.304	1900	1907	1917	rBV	1571479	2214944	55.14%	5.171%
52	14.440	1926	1930	1936	rVB9	5889	8768	0.22%	0.020%
53	14.604	1951	1958	1970	rBV	2308642	3357753	83.59%	7.839%
54	14.828	1991	1996	2012	rBV	170444	357028	8.89%	0.834%
55	15.004	2022	2026	2029	rBV4	15775	21098	0.53%	0.049%

56	15.045	2029	2033	2040	rVB2	36735	58306	1.45%	0.136%
57	15.345	2081	2084	2087	rBV5	4928	7268	0.18%	0.017%
58	15.392	2089	2092	2093	rBV3	5502	4799	0.12%	0.011%
59	15.604	2120	2128	2135	rBV	2041642	2919862	72.69%	6.817%
60	15.734	2145	2150	2156	rBV	186810	252136	6.28%	0.589%

61	15.839	2165	2168	2172	rBV6	10581	12432	0.31%	0.029%
62	16.181	2224	2226	2229	rBV4	5438	6825	0.17%	0.016%
63	16.263	2238	2240	2242	rBV3	7009	7463	0.19%	0.017%
64	16.898	2344	2348	2353	rBV2	32555	48418	1.21%	0.113%
65	17.375	2423	2429	2440	rBV	2837550	4016898	100.00%	9.378%

66	17.475	2440	2446	2454	rVV2	2042012	2943188	73.27%	6.871%
67	17.563	2458	2461	2467	rVB6	30676	47960	1.19%	0.112%
68	17.998	2532	2535	2539	rBV	34576	44227	1.10%	0.103%
69	18.216	2569	2572	2578	rBV3	93767	149664	3.73%	0.349%
70	19.716	2822	2827	2838	rBV	2682918	3483679	86.73%	8.133%

71	21.480	3123	3127	3132	rVB	2418523	2997739	74.63%	6.999%
72	23.833	3523	3527	3541	rVB2	1237477	2610773	64.99%	6.095%
73	24.004	3551	3556	3564	rVB	1455053	2886082	71.85%	6.738%




Sum of corrected areas: 42833901

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017216.D
Acq On : 18 Sep 2023 21:25
Operator : MA/JU
Sample : 04330-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

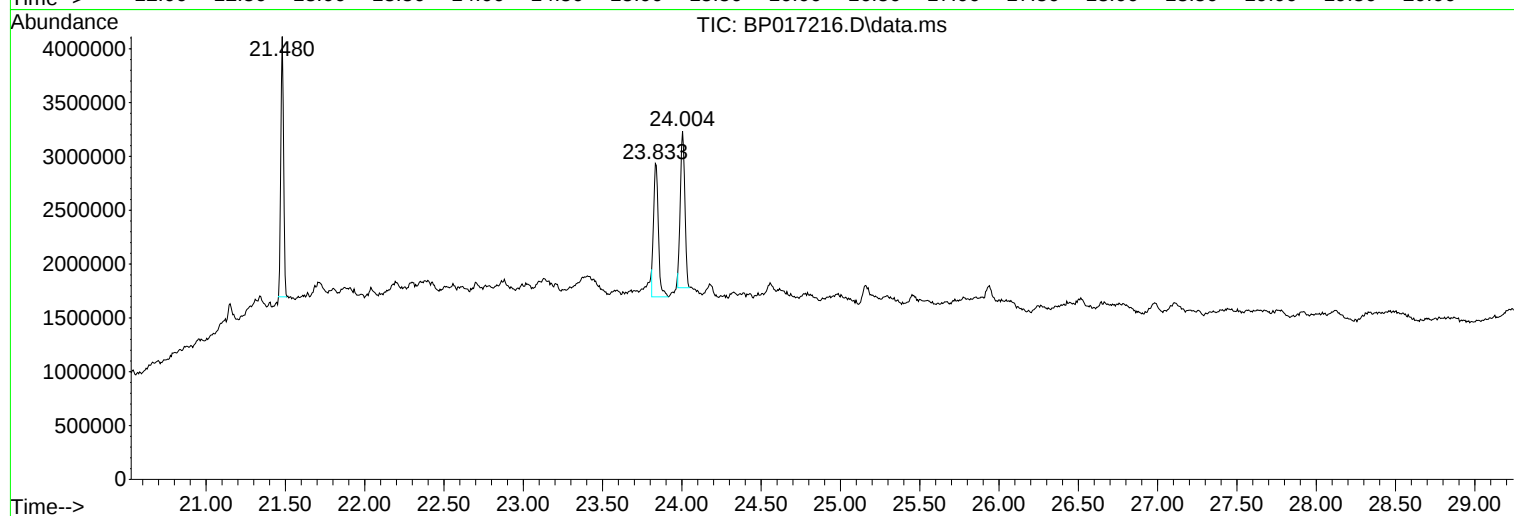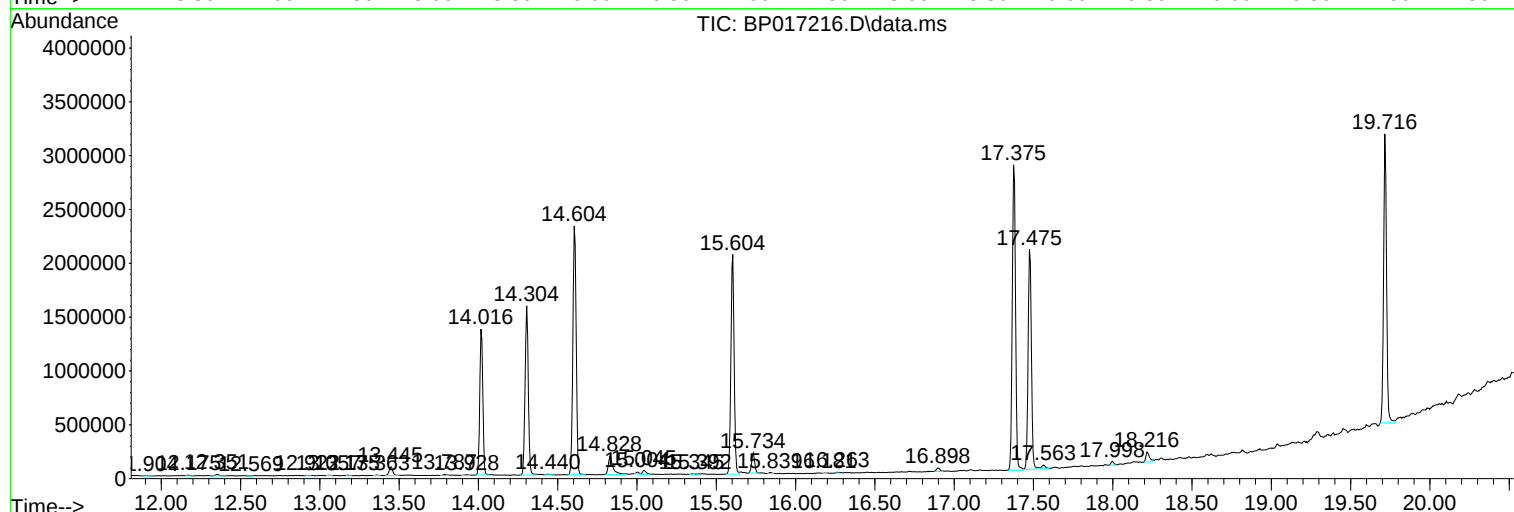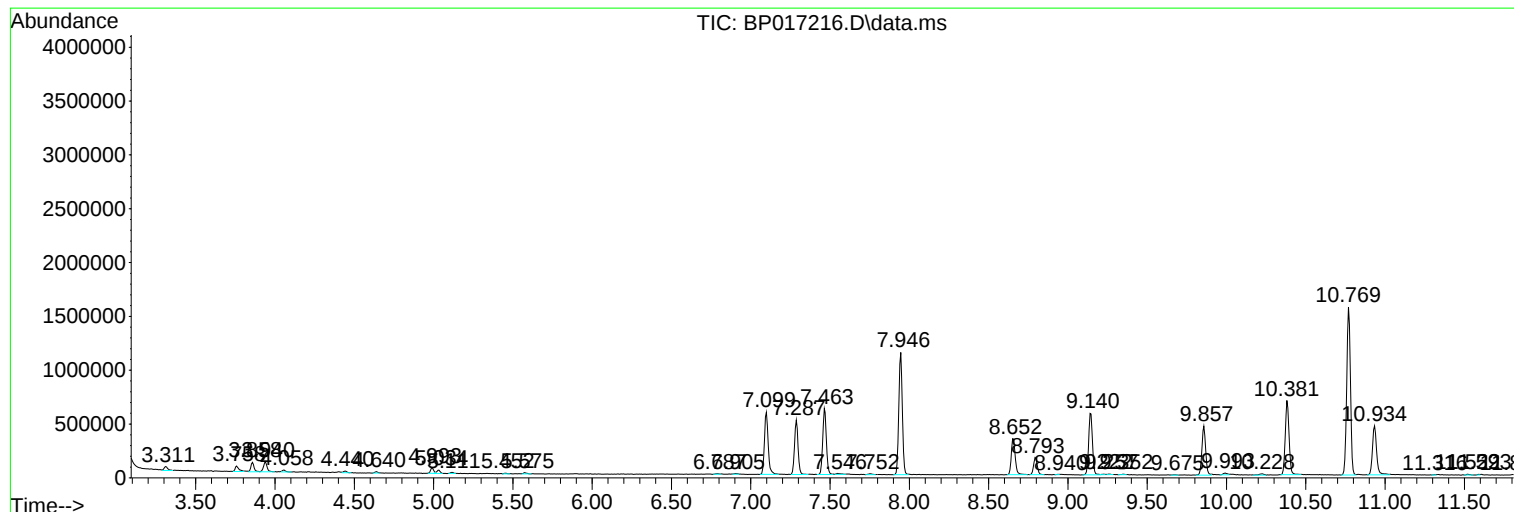

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017216.D
Acq On : 18 Sep 2023 21:25
Operator : MA/JU
Sample : 04330-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017216.D
Acq On : 18 Sep 2023 21:25
Operator : MA/JU
Sample : 04330-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc