

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017218.D
 Acq On : 18 Sep 2023 22:33
 Operator : MA/JU
 Sample : 04330-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	35	38	43	rVB	37045	42314	1.61%	0.116%
2	3.758	110	114	125	rVV2	51346	86143	3.27%	0.236%
3	3.858	127	131	136	rVV	79208	97687	3.71%	0.268%
4	3.940	140	145	152	rVB	92394	137916	5.24%	0.378%
5	4.058	161	165	168	rVB	21473	28620	1.09%	0.078%
6	4.440	228	230	239	rVB4	17337	24395	0.93%	0.067%
7	4.640	261	264	269	rVB2	15087	19233	0.73%	0.053%
8	4.993	319	324	329	rBV	54105	79843	3.03%	0.219%
9	5.117	342	345	350	rVB5	9582	13287	0.50%	0.036%
10	5.399	389	393	398	rVV7	7001	11469	0.44%	0.031%
11	5.452	399	402	408	rVB6	6481	10350	0.39%	0.028%
12	5.534	411	416	418	rVV2	13666	20388	0.77%	0.056%
13	5.575	421	423	428	rVV2	12470	15670	0.60%	0.043%
14	5.899	473	478	486	rVB4	13963	27986	1.06%	0.077%
15	6.511	576	582	586	rBV9	4994	11316	0.43%	0.031%
16	6.558	586	590	597	rVB3	20332	34417	1.31%	0.094%
17	6.905	643	649	655	rVB8	8071	18395	0.70%	0.050%
18	7.099	675	682	694	rVB	538493	946397	35.96%	2.594%
19	7.287	707	714	724	rBV	482503	741816	28.19%	2.033%
20	7.463	738	744	753	rBV	560033	909750	34.57%	2.493%
21	7.546	753	758	765	rBV2	26639	64160	2.44%	0.176%
22	7.752	787	793	797	rBV5	6463	14458	0.55%	0.040%
23	7.946	816	826	835	rBV	1018370	1582346	60.13%	4.337%
24	8.040	835	842	844	rBV6	6468	12605	0.48%	0.035%
25	8.387	898	901	906	rBV6	7564	11182	0.42%	0.031%
26	8.657	939	947	953	rBV	370022	621260	23.61%	1.703%
27	8.722	953	958	965	rVV2	53686	109660	4.17%	0.301%
28	8.793	965	970	980	rVV	219943	350473	13.32%	0.961%
29	9.022	1006	1009	1013	rVB6	6176	9852	0.37%	0.027%
30	9.146	1017	1030	1037	rBV	520928	906677	34.45%	2.485%
31	9.257	1046	1049	1054	rVB7	6459	9740	0.37%	0.027%
32	9.352	1058	1065	1071	rBV7	8339	17120	0.65%	0.047%
33	9.622	1109	1111	1118	rVB8	6511	10434	0.40%	0.029%
34	9.722	1124	1128	1131	rBV5	5853	8579	0.33%	0.024%
35	9.857	1141	1151	1159	rBV	376285	635935	24.16%	1.743%
36	9.963	1166	1169	1171	rBV4	7683	10881	0.41%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017218.D
 Acq On : 18 Sep 2023 22:33
 Operator : MA/JU
 Sample : 04330-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	9.993	1171	1174	1180	rVV2	19809	34245	1.30%	0.094%
38	10.199	1201	1209	1214	rBV2	71623	170174	6.47%	0.466%
39	10.381	1234	1240	1251	rBV	590701	983968	37.39%	2.697%
40	10.663	1280	1288	1295	rVV3	117310	214294	8.14%	0.587%
41	10.769	1298	1306	1312	rVV	1319669	2170499	82.47%	5.949%
42	10.822	1312	1315	1323	rVB2	33537	70448	2.68%	0.193%
43	10.934	1326	1334	1348	rBV	417646	751775	28.57%	2.060%
44	11.028	1348	1350	1355	rVB6	6200	8566	0.33%	0.023%
45	11.110	1358	1364	1372	rBV	76312	124072	4.71%	0.340%
46	11.340	1393	1403	1405	rBV	8445	22722	0.86%	0.062%
47	11.410	1411	1415	1418	rVB6	6980	9904	0.38%	0.027%
48	11.528	1430	1435	1439	rBV7	10010	18955	0.72%	0.052%
49	11.593	1440	1446	1455	rVV4	32659	68346	2.60%	0.187%
50	11.704	1460	1465	1469	rVV	22345	30934	1.18%	0.085%
51	11.763	1471	1475	1479	rVV7	5088	10733	0.41%	0.029%
52	11.804	1479	1482	1486	rVV5	8617	13237	0.50%	0.036%
53	12.057	1519	1525	1527	rBV7	5429	9342	0.35%	0.026%
54	12.104	1527	1533	1541	rBV3	80750	154973	5.89%	0.425%
55	12.304	1563	1567	1569	rVV5	8649	13608	0.52%	0.037%
56	12.351	1572	1575	1581	rVB3	16892	27332	1.04%	0.075%
57	12.428	1581	1588	1593	rBV	26463	38969	1.48%	0.107%
58	12.646	1621	1625	1631	rVB2	18486	29554	1.12%	0.081%
59	12.746	1638	1642	1645	rBV5	9679	14748	0.56%	0.040%
60	12.816	1649	1654	1658	rVV6	6935	13046	0.50%	0.036%
61	12.851	1658	1660	1665	rVB6	8411	11471	0.44%	0.031%
62	12.922	1669	1672	1677	rBV6	10641	16457	0.63%	0.045%
63	13.010	1684	1687	1691	rVB6	7500	9701	0.37%	0.027%
64	13.057	1691	1695	1701	rVB4	20813	30733	1.17%	0.084%
65	13.357	1740	1746	1751	rBV	80149	107652	4.09%	0.295%
66	13.410	1751	1755	1757	rVV3	12402	17202	0.65%	0.047%
67	13.445	1757	1761	1770	rVB	72967	121222	4.61%	0.332%
68	13.757	1809	1814	1815	rBV5	12591	18656	0.71%	0.051%
69	13.787	1815	1819	1822	rVV4	33133	51330	1.95%	0.141%
70	13.822	1822	1825	1832	rVV3	20967	37284	1.42%	0.102%
71	13.922	1836	1842	1846	rVV7	24541	49411	1.88%	0.135%
72	13.975	1847	1851	1853	rVV3	19052	32203	1.22%	0.088%
73	14.016	1853	1858	1875	rVB	1060002	1544797	58.70%	4.234%
74	14.222	1890	1893	1898	rVB7	5666	8916	0.34%	0.024%
75	14.304	1900	1907	1918	rBV	1224398	1791409	68.07%	4.910%
76	14.434	1924	1929	1936	rVB	70685	91421	3.47%	0.251%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017218.D
 Acq On : 18 Sep 2023 22:33
 Operator : MA/JU
 Sample : 04330-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

77	14.604	1952	1958	1967	rBV	1771616	2492329	94.70%	6.831%
78	14.669	1967	1969	1979	rVB9	12737	20985	0.80%	0.058%
79	14.834	1991	1997	2011	rBV	93673	209370	7.96%	0.574%
80	14.987	2018	2023	2029	rBV6	20297	44951	1.71%	0.123%
81	15.045	2030	2033	2042	rVB6	33625	65759	2.50%	0.180%
82	15.204	2056	2060	2067	rVB6	13728	25868	0.98%	0.071%
83	15.263	2067	2070	2079	rVB10	14603	30710	1.17%	0.084%
84	15.351	2081	2085	2086	rBV4	11519	13809	0.52%	0.038%
85	15.387	2088	2091	2098	rVV2	41013	56282	2.14%	0.154%
86	15.604	2121	2128	2135	rBV	1457913	2160596	82.10%	5.922%
87	15.734	2145	2150	2155	rBV	69605	96317	3.66%	0.264%
88	15.781	2155	2158	2165	rVB5	25692	47386	1.80%	0.130%
89	16.263	2235	2240	2247	rBV2	65045	124664	4.74%	0.342%
90	17.057	2372	2375	2379	rBV	33705	41019	1.56%	0.112%
91	17.104	2379	2383	2388	rVB3	33998	49759	1.89%	0.136%
92	17.375	2423	2429	2434	rBV	1776077	2447109	92.98%	6.707%
93	17.475	2441	2446	2454	rBV	1405410	1990726	75.64%	5.456%
94	17.563	2459	2461	2465	rVB5	32955	34829	1.32%	0.095%
95	17.804	2499	2502	2507	rVB3	55765	74021	2.81%	0.203%
96	18.216	2569	2572	2580	rBV6	56207	135935	5.17%	0.373%
97	19.716	2822	2827	2835	rBV	1760044	2523178	95.87%	6.915%
98	21.480	3123	3127	3131	rVB	1761784	2240292	85.13%	6.140%
99	23.833	3523	3527	3534	rVB2	1227389	2332011	88.61%	6.391%
100	24.004	3551	3556	3563	rVB	1323867	2631739	100.00%	7.213%



Sum of corrected areas: 36486707

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017218.D
Acq On : 18 Sep 2023 22:33
Operator : MA/JU
Sample : 04330-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

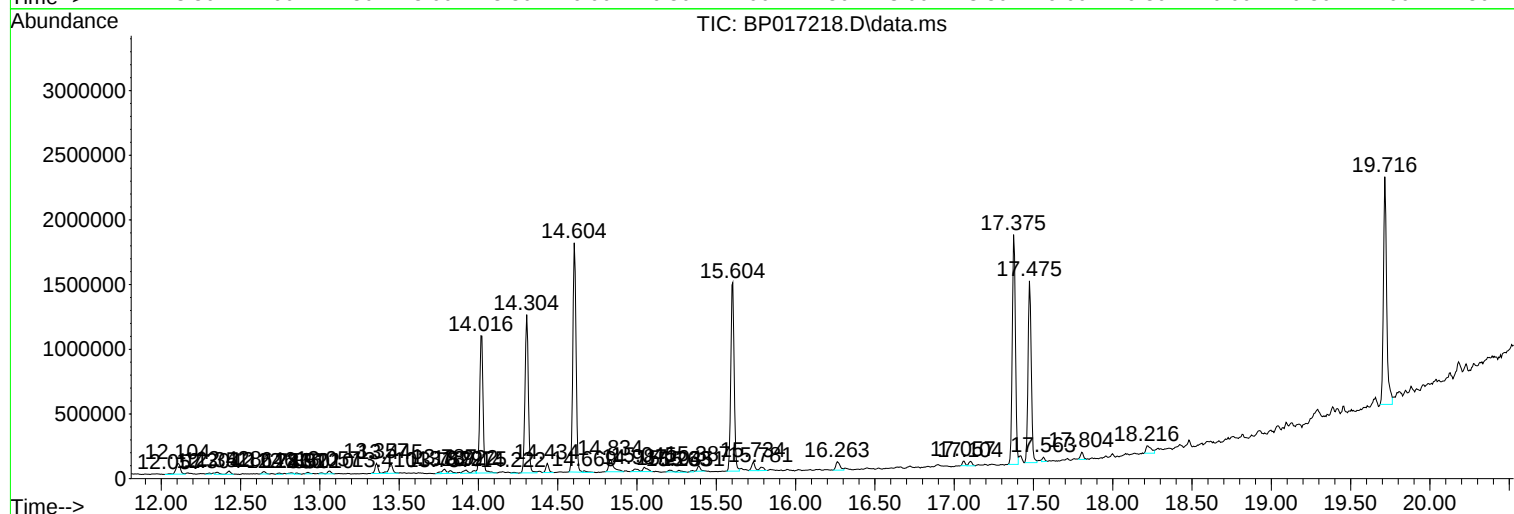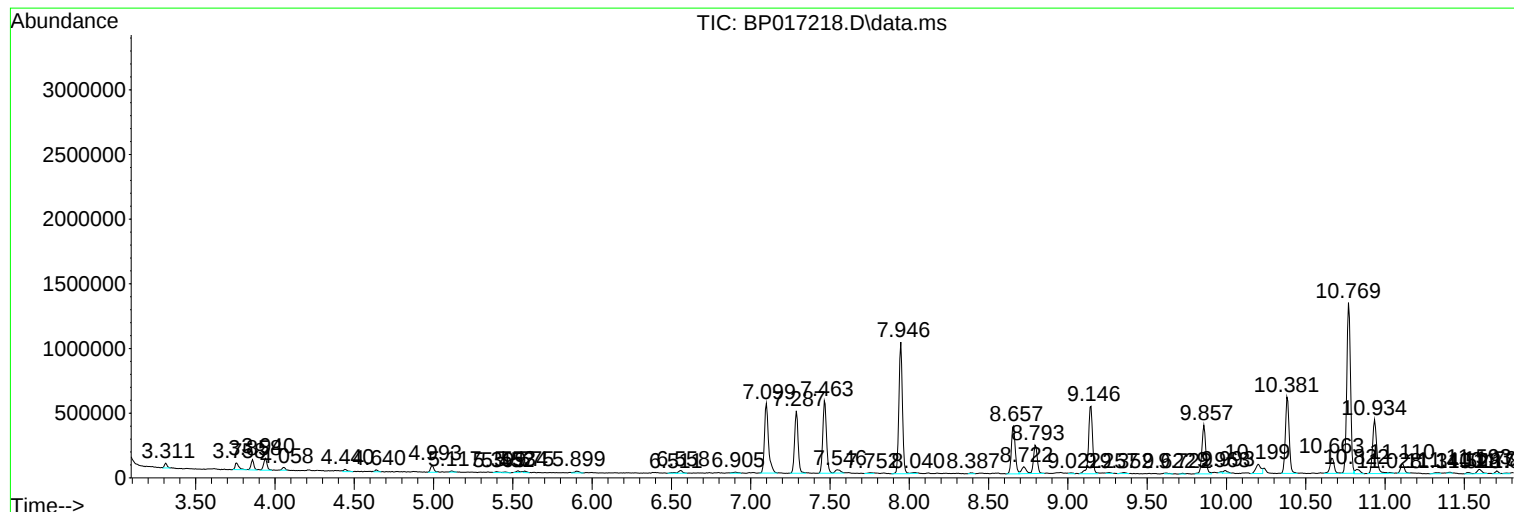

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017218.D
Acq On : 18 Sep 2023 22:33
Operator : MA/JU
Sample : 04330-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017218.D
Acq On : 18 Sep 2023 22:33
Operator : MA/JU
Sample : 04330-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------