

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017220.D
 Acq On : 18 Sep 2023 23:42
 Operator : MA/JU
 Sample : 04330-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	35	38	43	rVB	39713	49341	1.41%	0.119%
2	3.758	110	114	125	rVB2	31414	55741	1.59%	0.135%
3	3.858	127	131	136	rVB	67851	84919	2.43%	0.205%
4	3.940	139	145	151	rVB	91366	129683	3.71%	0.313%
5	4.058	161	165	171	rVB	17344	25881	0.74%	0.063%
6	4.446	227	231	235	rVB3	16642	26952	0.77%	0.065%
7	4.640	260	264	269	rBV2	18026	23116	0.66%	0.056%
8	4.987	319	323	328	rBV	49166	72829	2.08%	0.176%
9	5.034	328	331	337	rVB	13490	19288	0.55%	0.047%
10	5.117	341	345	350	rBV3	9122	15783	0.45%	0.038%
11	5.452	400	402	406	rVB5	7028	6769	0.19%	0.016%
12	5.581	418	424	429	rBV	10206	18828	0.54%	0.045%
13	5.899	476	478	483	rVB4	6535	7602	0.22%	0.018%
14	6.905	646	649	656	rVB9	8039	13376	0.38%	0.032%
15	7.099	674	682	697	rBV	627532	1047231	29.95%	2.529%
16	7.287	707	714	723	rBV	550929	829122	23.71%	2.002%
17	7.463	737	744	755	rBV	657597	1059998	30.32%	2.560%
18	7.558	755	760	764	rVV5	8321	17501	0.50%	0.042%
19	7.616	767	770	776	rVB8	6221	8482	0.24%	0.020%
20	7.752	786	793	796	rBV3	6124	11612	0.33%	0.028%
21	7.946	819	826	834	rBV	1156725	1798206	51.43%	4.343%
22	8.122	851	856	858	rBV5	5790	6715	0.19%	0.016%
23	8.399	896	903	906	rBV8	3516	6780	0.19%	0.016%
24	8.657	939	947	958	rBV	447169	766209	21.91%	1.850%
25	8.793	964	970	979	rVV	170863	281564	8.05%	0.680%
26	8.940	992	995	998	rBV4	4250	7132	0.20%	0.017%
27	9.146	1018	1030	1038	rBV	609247	1017875	29.11%	2.458%
28	9.252	1047	1048	1056	rVB8	9444	13011	0.37%	0.031%
29	9.352	1058	1065	1071	rVB8	7705	19501	0.56%	0.047%
30	9.634	1105	1113	1119	rBV8	8500	21996	0.63%	0.053%
31	9.857	1140	1151	1160	rBV	482045	814401	23.29%	1.967%
32	9.993	1170	1174	1179	rBV5	15038	33199	0.95%	0.080%
33	10.228	1207	1214	1220	rVV5	12770	28990	0.83%	0.070%
34	10.381	1234	1240	1256	rVV	683446	1169670	33.45%	2.825%
35	10.657	1280	1287	1294	rBV4	28774	49642	1.42%	0.120%
36	10.769	1299	1306	1313	rVV	1472414	2392016	68.41%	5.777%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017220.D
 Acq On : 18 Sep 2023 23:42
 Operator : MA/JU
 Sample : 04330-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

37	10.840	1313	1318	1323	rVB5	21975	40332	1.15%	0.097%
38	10.934	1326	1334	1351	rBV	389657	761954	21.79%	1.840%
39	11.328	1394	1401	1410	rBV	8868	23695	0.68%	0.057%
40	11.404	1410	1414	1419	rBV7	11201	22654	0.65%	0.055%
41	11.528	1427	1435	1439	rBV7	8710	17190	0.49%	0.042%
42	11.593	1441	1446	1447	rVV5	9641	12956	0.37%	0.031%
43	11.610	1447	1449	1455	rVB7	10870	13254	0.38%	0.032%
44	11.704	1461	1465	1470	rVB2	20001	29620	0.85%	0.072%
45	11.757	1470	1474	1476	rBV5	5557	8568	0.25%	0.021%
46	11.804	1479	1482	1485	rVV5	6366	9636	0.28%	0.023%
47	11.846	1486	1489	1493	rVB6	4591	7903	0.23%	0.019%
48	11.946	1502	1506	1509	rBV5	8627	9879	0.28%	0.024%
49	12.110	1528	1534	1539	rBV2	36802	60999	1.74%	0.147%
50	12.175	1542	1545	1550	rVV7	8080	14225	0.41%	0.034%
51	12.240	1554	1556	1560	rVV4	5549	8230	0.24%	0.020%
52	12.298	1563	1566	1570	rVV6	9468	17742	0.51%	0.043%
53	12.351	1573	1575	1580	rVV3	14930	19530	0.56%	0.047%
54	12.428	1583	1588	1591	rVV6	7769	10268	0.29%	0.025%
55	12.657	1622	1627	1632	rBV9	14528	27036	0.77%	0.065%
56	12.746	1637	1642	1646	rBV8	9720	16018	0.46%	0.039%
57	12.851	1658	1660	1666	rVB6	6959	8537	0.24%	0.021%
58	12.922	1666	1672	1676	rBV6	15771	29865	0.85%	0.072%
59	13.010	1683	1687	1691	rVB7	8179	10083	0.29%	0.024%
60	13.057	1691	1695	1701	rVB3	17888	27905	0.80%	0.067%
61	13.181	1711	1716	1720	rVB4	9718	13844	0.40%	0.033%
62	13.357	1737	1746	1751	rBV3	41044	67539	1.93%	0.163%
63	13.445	1754	1761	1768	rBV	68839	120267	3.44%	0.290%
64	13.757	1808	1814	1815	rVV5	9198	15451	0.44%	0.037%
65	13.787	1815	1819	1824	rVB7	11333	21326	0.61%	0.052%
66	13.922	1837	1842	1846	rBV6	15023	24065	0.69%	0.058%
67	14.016	1852	1858	1867	rVV	1208854	1666232	47.66%	4.024%
68	14.140	1875	1879	1880	rBV4	7696	7571	0.22%	0.018%
69	14.304	1900	1907	1916	rBV2	1308940	1896293	54.24%	4.579%
70	14.434	1925	1929	1935	rVB	39465	51557	1.47%	0.125%
71	14.604	1952	1958	1968	rBV	1841445	2640070	75.51%	6.376%
72	14.834	1991	1997	2011	rBV	183270	366042	10.47%	0.884%
73	14.934	2011	2014	2018	rVV6	8883	16030	0.46%	0.039%
74	14.998	2020	2025	2029	rVV7	20313	45079	1.29%	0.109%
75	15.045	2029	2033	2041	rVV5	47244	90462	2.59%	0.218%
76	15.122	2044	2046	2049	rVB3	7928	7881	0.23%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
 Data File : BP017220.D
 Acq On : 18 Sep 2023 23:42
 Operator : MA/JU
 Sample : 04330-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Title : SVOA CALIBRATION

77	15.204	2054	2060	2066	rBV3	11190	28369	0.81%	0.069%
78	15.263	2067	2070	2074	rBV6	7936	11188	0.32%	0.027%
79	15.351	2079	2085	2088	rBV5	11940	20774	0.59%	0.050%
80	15.392	2088	2092	2095	rBV	34766	44611	1.28%	0.108%
81	15.545	2114	2118	2121	rBV6	5261	7426	0.21%	0.018%
82	15.604	2121	2128	2135	rBV	1697691	2432119	69.56%	5.873%
83	15.734	2145	2150	2155	rBV	134119	182296	5.21%	0.440%
84	15.787	2155	2159	2165	rVV6	22800	39176	1.12%	0.095%
85	15.839	2165	2168	2174	rVB7	10898	16865	0.48%	0.041%
86	15.945	2184	2186	2192	rVB7	8200	10668	0.31%	0.026%
87	16.263	2236	2240	2246	rBV	49195	77478	2.22%	0.187%
88	16.722	2313	2318	2323	rBV9	14071	31596	0.90%	0.076%
89	17.063	2372	2376	2379	rVB	30951	36280	1.04%	0.088%
90	17.104	2379	2383	2388	rVB4	17856	23861	0.68%	0.058%
91	17.375	2423	2429	2434	rBV	1918029	2697487	77.15%	6.514%
92	17.416	2434	2436	2441	rVV	60489	84783	2.42%	0.205%
93	17.475	2441	2446	2456	rVV	1692653	2415693	69.09%	5.834%
94	17.804	2499	2502	2507	rVB3	38860	47119	1.35%	0.114%
95	18.216	2568	2572	2580	rBV4	97471	184371	5.27%	0.445%
96	18.480	2615	2617	2620	rVB2	42218	39562	1.13%	0.096%
97	19.716	2822	2827	2836	rBV	2253706	3090054	88.38%	7.462%
98	21.480	3123	3127	3132	rVB	2216598	2793221	79.89%	6.745%
99	23.839	3523	3528	3542	rVB2	1642631	3496357	100.00%	8.443%
100	24.004	3551	3556	3566	rVB	1666081	3389269	96.94%	8.185%



Sum of corrected areas: 41409372

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017220.D
Acq On : 18 Sep 2023 23:42
Operator : MA/JU
Sample : 04330-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

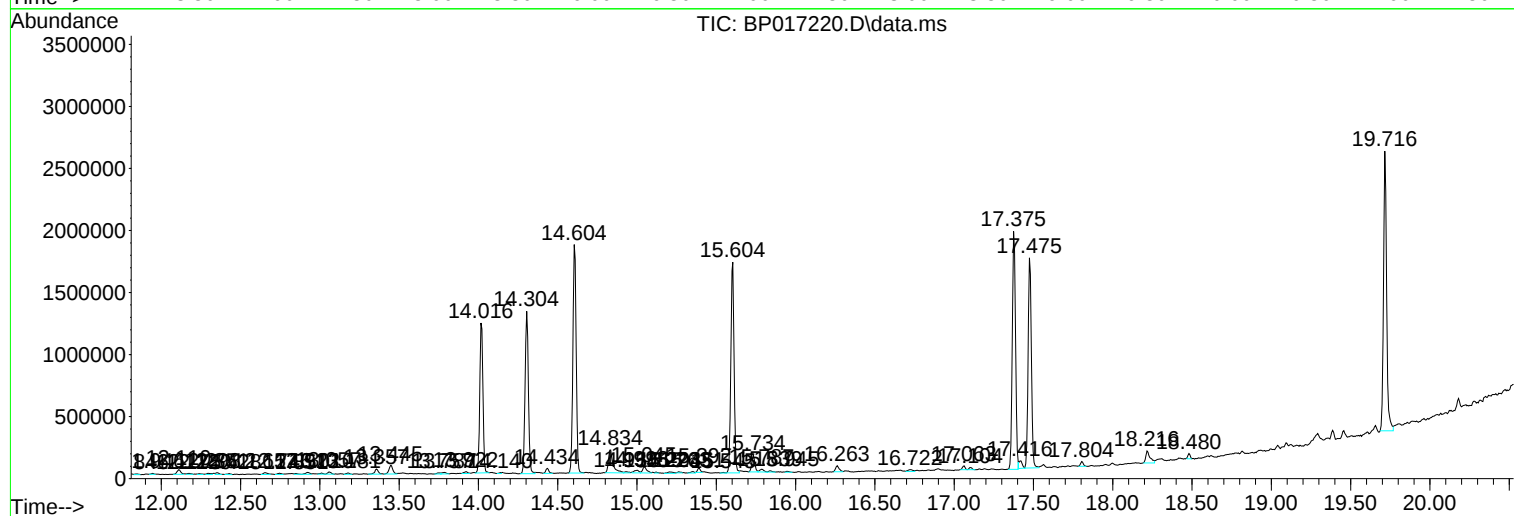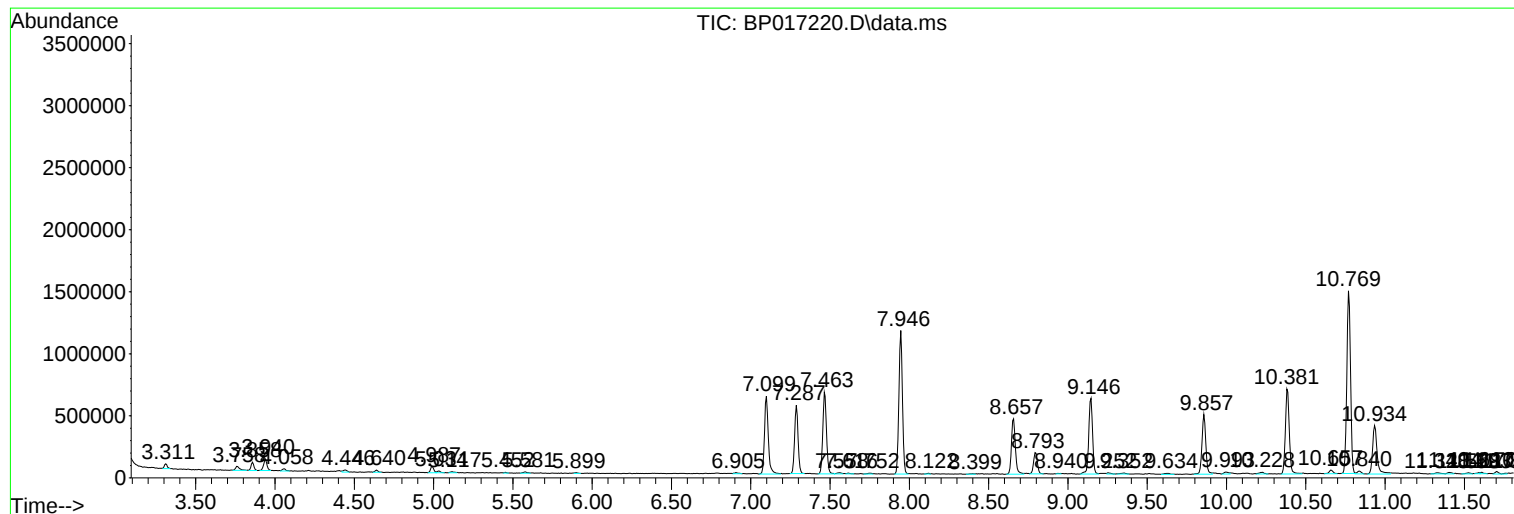

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017220.D
Acq On : 18 Sep 2023 23:42
Operator : MA/JU
Sample : 04330-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091823\
Data File : BP017220.D
Acq On : 18 Sep 2023 23:42
Operator : MA/JU
Sample : 04330-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZYF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc