

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091919\
 Data File : BP000320.D
 Acq On : 19 Sep 2019 11:12
 Operator : HP/JU
 Sample : PB123205BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123205BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.858	293	301	308	rVB	251535	336477	3.35%	0.563%
2	5.416	561	566	569	rBV	5023155	4852567	48.37%	8.126%
3	6.428	733	738	741	rBV	4892067	4953418	49.37%	8.295%
4	6.563	757	761	764	rBV	6106378	5339248	53.22%	8.941%
5	6.793	796	800	803	rBV	1917729	1457818	14.53%	2.441%
6	6.952	823	827	830	rBV	5409476	4691068	46.76%	7.855%
7	7.352	890	895	898	rBV	3810128	3296964	32.86%	5.521%
8	8.075	1014	1018	1021	rBV	2316902	1861718	18.56%	3.117%
9	9.152	1197	1201	1205	rBV	7735639	7338985	73.15%	12.289%
10	9.834	1313	1317	1321	rBV	2854523	2306409	22.99%	3.862%
11	10.628	1448	1452	1471	rBV	5414198	5054897	50.38%	8.464%
12	11.328	1567	1571	1575	rBV	2992253	2567087	25.59%	4.299%
13	12.934	1839	1844	1847	rBV	9833901	10032828	100.00%	16.800%
14	13.992	2020	2024	2028	rBV	2987578	2829765	28.21%	4.738%
15	15.481	2271	2277	2282	rVB	2258876	2800003	27.91%	4.689%


Sum of corrected areas: 59719252

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091919\
Data File : BP000320.D
Acq On : 19 Sep 2019 11:12
Operator : HP/JU
Sample : PB123205BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123205BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

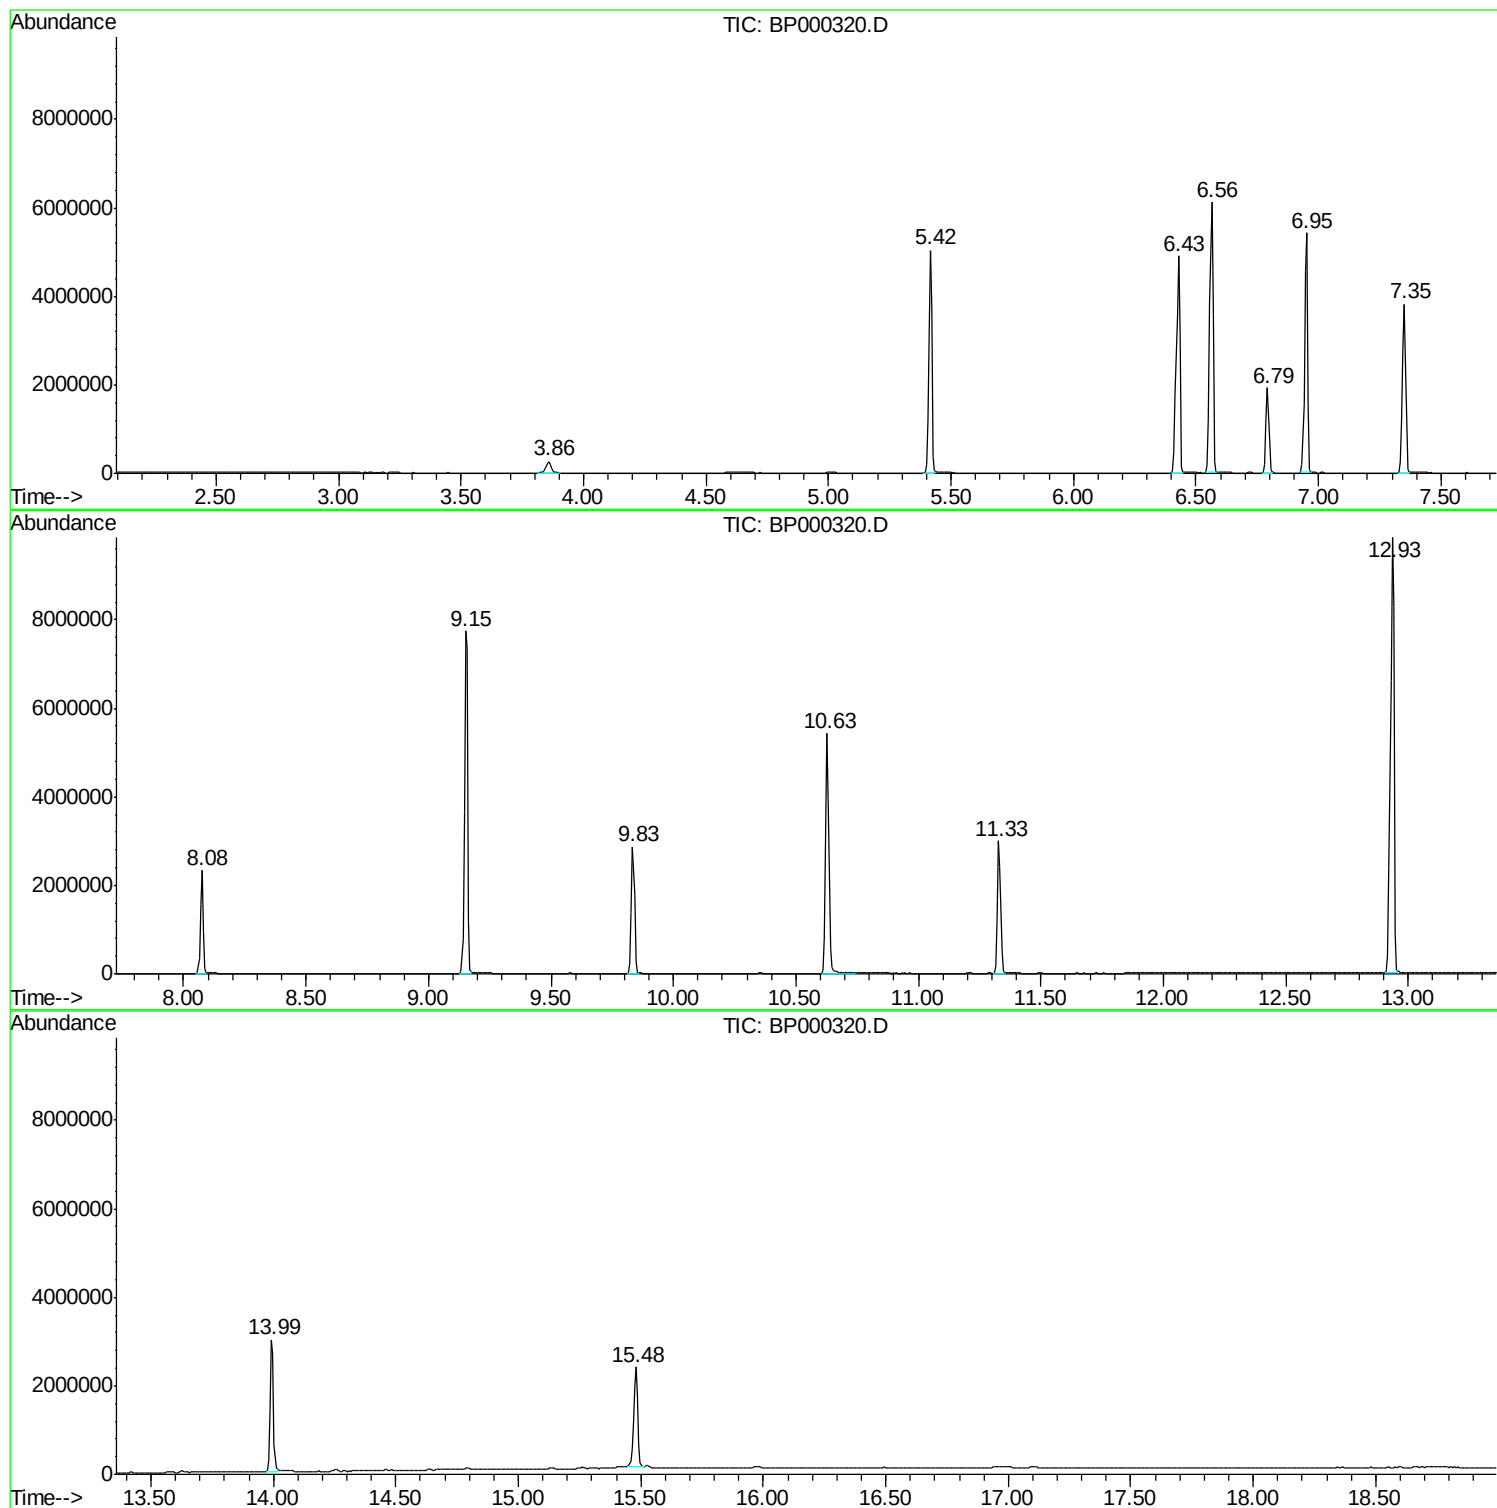

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091919\
Data File : BP000320.D
Acq On : 19 Sep 2019 11:12
Operator : HP/JU
Sample : PB123205BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123205BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	73.25 ng	5339250	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
4		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

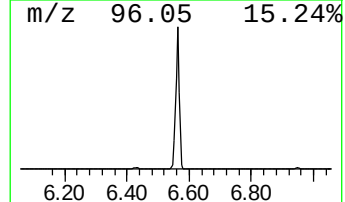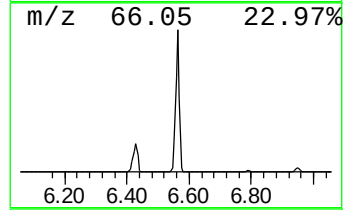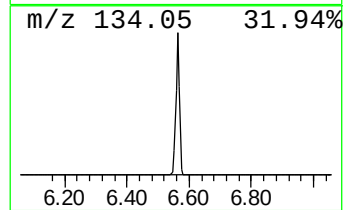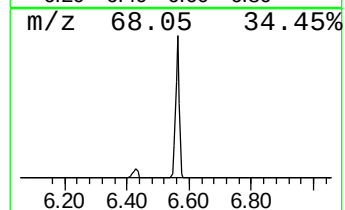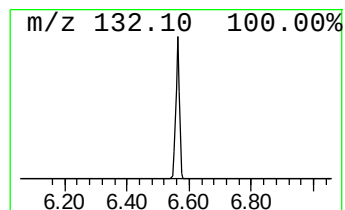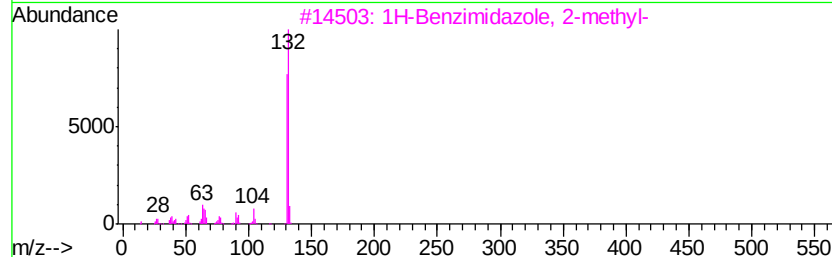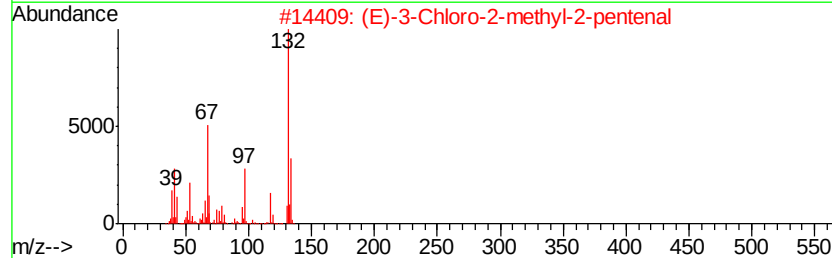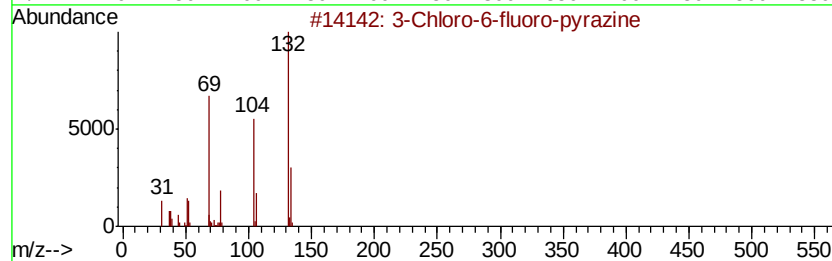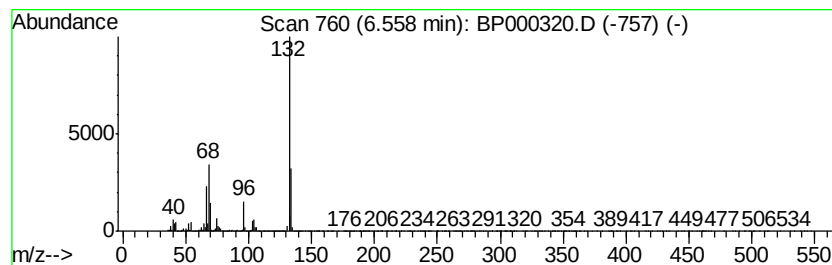

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091919\
Data File : BP000320.D
Acq On : 19 Sep 2019 11:12
Operator : HP/JU
Sample : PB123205BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123205BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	73.3	ng	5339250	1	6.79	1457820	20.0