

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091919\
 Data File : BP000322.D
 Acq On : 19 Sep 2019 12:00
 Operator : HP/JU
 Sample : PB123199BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123199BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	561	567	570	rBV	5313623	5589416	53.97%	8.458%
2	6.428	733	738	741	rBV	5315489	5719085	55.23%	8.655%
3	6.564	756	761	764	rBV	6539103	6083646	58.75%	9.206%
4	6.793	796	800	803	rBV	1847603	1533108	14.80%	2.320%
5	6.952	822	827	830	rBV	5843689	5427878	52.41%	8.214%
6	7.352	889	895	898	rBV	4171413	3792907	36.63%	5.740%
7	8.069	1014	1017	1021	rBV	2197449	2048839	19.78%	3.100%
8	9.152	1196	1201	1204	rBV	10039840	8808536	85.06%	13.330%
9	9.834	1313	1317	1320	rBV	3020841	2621253	25.31%	3.967%
10	10.628	1447	1452	1455	rBV	6326936	5794612	55.95%	8.769%
11	11.328	1567	1571	1574	rBV	3220685	2790045	26.94%	4.222%
12	12.934	1839	1844	1847	rBV	10189335	10355901	100.00%	15.671%
13	13.993	2020	2024	2027	rBV	3077951	2755590	26.61%	4.170%
14	15.475	2270	2276	2281	rBV	2265001	2760788	26.66%	4.178%


Sum of corrected areas: 66081604

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091919\
Data File : BP000322.D
Acq On : 19 Sep 2019 12:00
Operator : HP/JU
Sample : PB123199BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123199BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

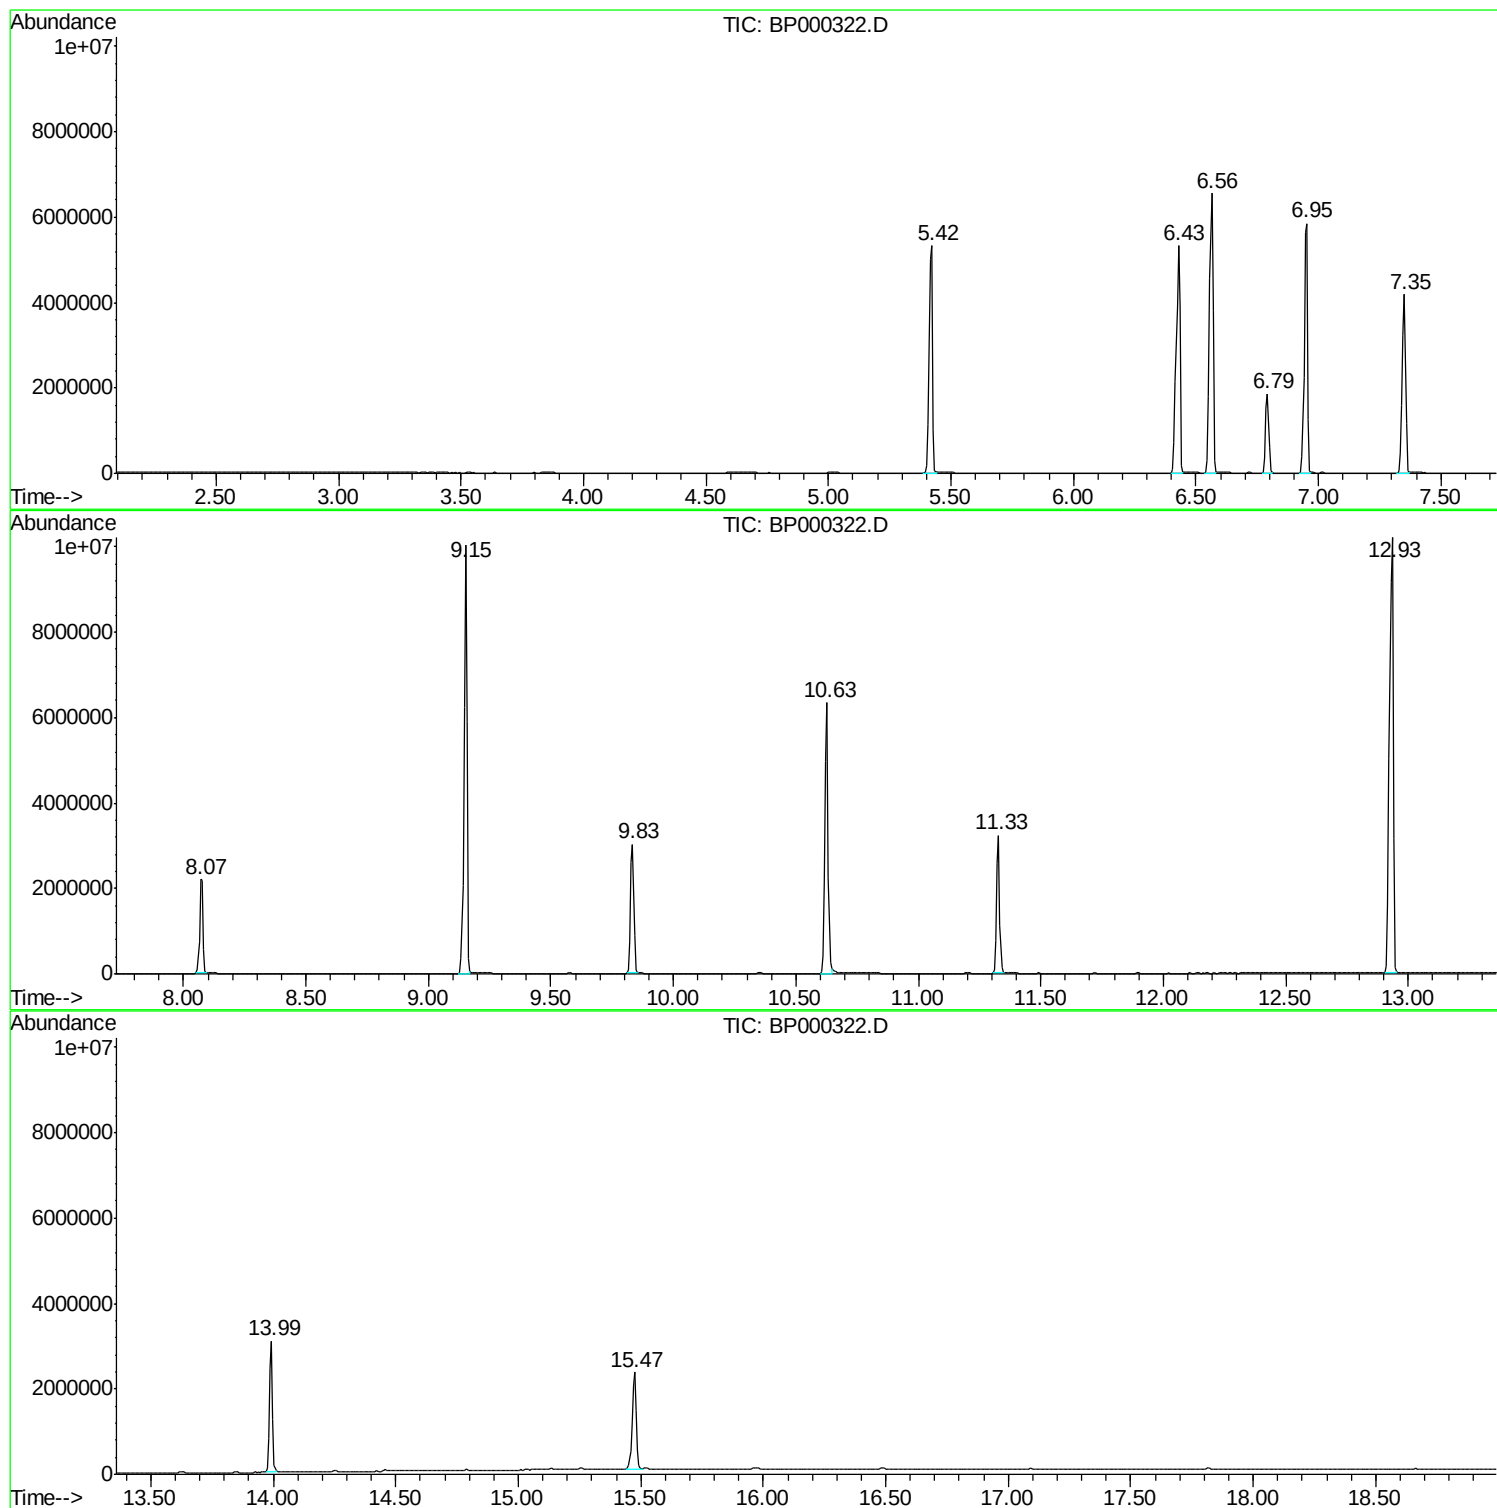

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091919\
Data File : BP000322.D
Acq On : 19 Sep 2019 12:00
Operator : HP/JU
Sample : PB123199BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123199BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	79.36 ng	6083650	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
5		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	12

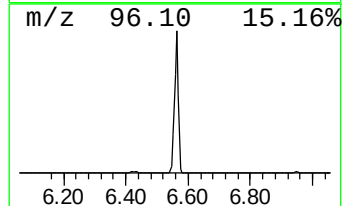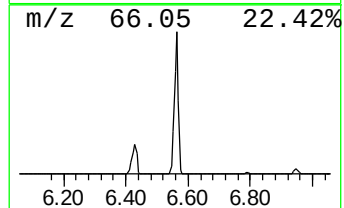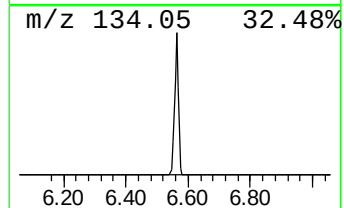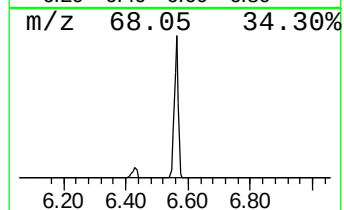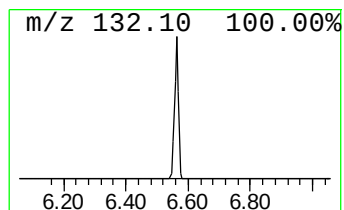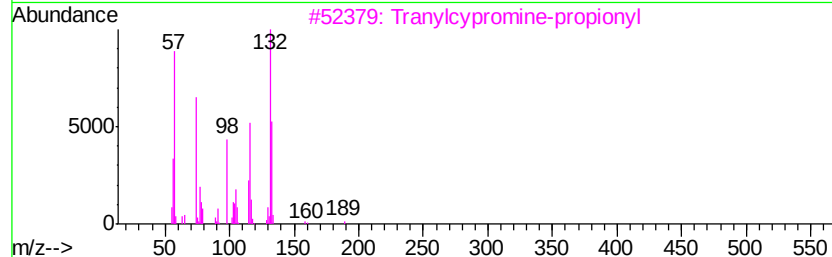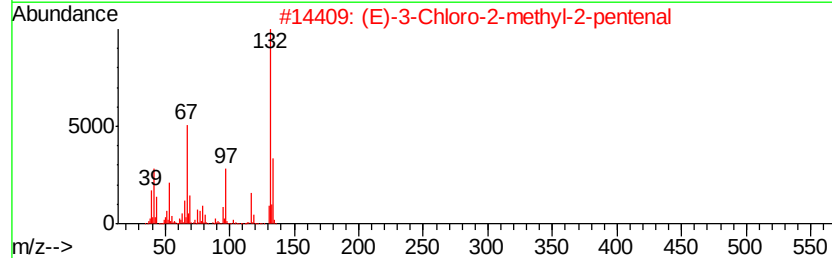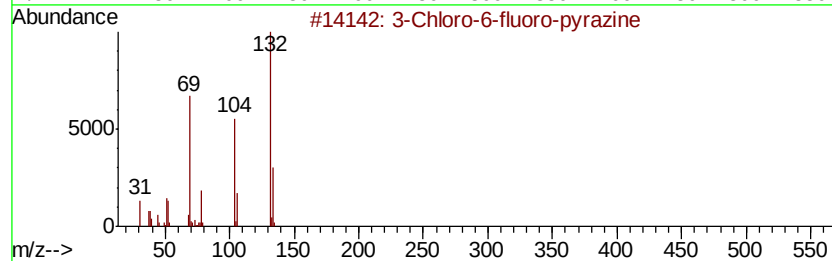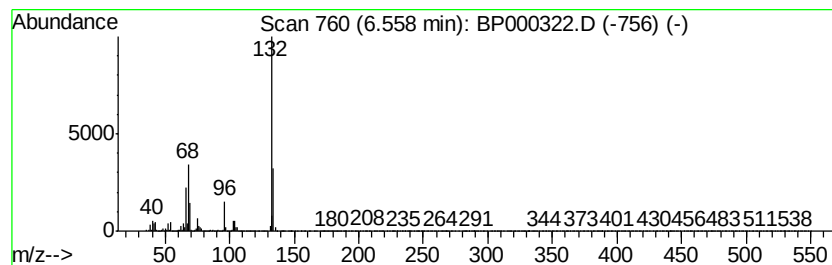

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091919\
Data File : BP000322.D
Acq On : 19 Sep 2019 12:00
Operator : HP/JU
Sample : PB123199BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123199BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.56	6.56	79.4	ng	6083650	1	6.79	1533110	20.0