


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091919\
 Data File : BP000316.D
 Acq On : 19 Sep 2019 08:58
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

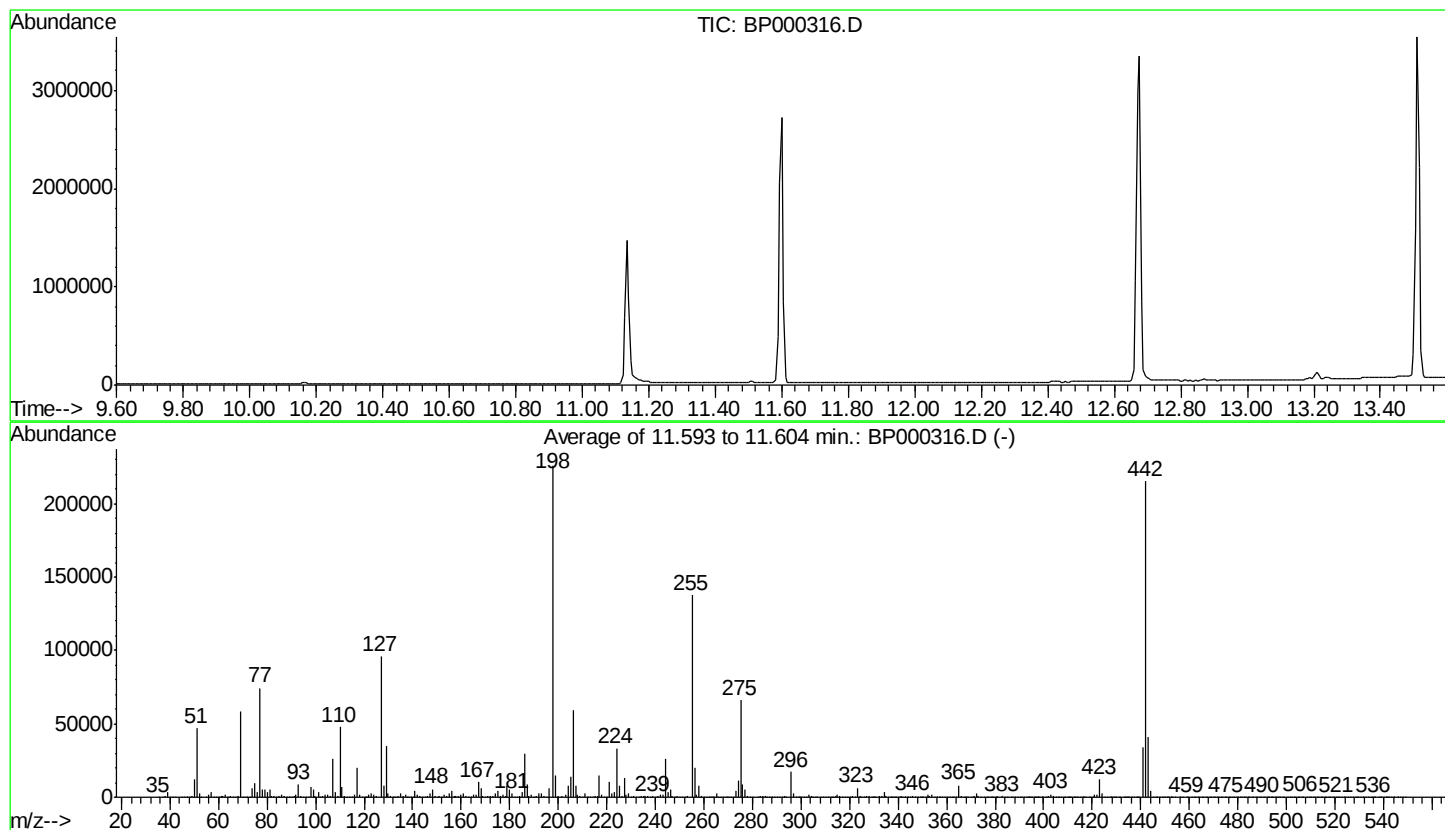

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	46722	PASS
68	69	0.00	2	1.2	726	PASS
69	198	0.00	100	25.9	58488	PASS
70	69	0.00	2	0.5	305	PASS
127	198	10	80	42.3	95607	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	225959	PASS
199	198	5	9	6.7	15128	PASS
275	198	10	60	29.2	66065	PASS
365	198	1	100	3.6	8215	PASS
441	198	0.01	100	15.1	34043	PASS
442	198	50	100	95.3	215402	PASS
443	442	15	24	19.2	41458	PASS