

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092023\
 Data File : BP017244.D
 Acq On : 20 Sep 2023 18:00
 Operator : MA/JU
 Sample : PB155669BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	42	rVB	51072	60936	1.65%	0.146%
2	3.740	107	111	123	rBV	324584	464898	12.57%	1.112%
3	4.052	160	164	169	rVB3	11237	16384	0.44%	0.039%
4	6.916	645	651	654	rVB6	3257	6647	0.18%	0.016%
5	7.093	674	681	694	rBV	708491	1128549	30.52%	2.700%
6	7.281	706	713	727	rBV	634427	969238	26.21%	2.319%
7	7.458	736	743	757	rBV	764376	1189371	32.16%	2.846%
8	7.940	818	825	833	rBV	735464	1126011	30.45%	2.694%
9	8.646	938	945	962	rBV	866059	1448927	39.18%	3.467%
10	9.140	1022	1029	1044	rBV	676133	1128887	30.52%	2.701%
11	9.852	1142	1150	1161	rBV	563318	922677	24.95%	2.208%
12	10.375	1230	1239	1254	rBV	853771	1436013	38.83%	3.436%
13	10.763	1297	1305	1313	rBV	1029328	1676129	45.32%	4.010%
14	10.928	1326	1333	1345	rBV	278195	485653	13.13%	1.162%
15	11.463	1419	1424	1429	rVB9	2017	4286	0.12%	0.010%
16	12.351	1569	1575	1582	rVB	16517	27197	0.74%	0.065%
17	12.569	1605	1612	1615	rBV8	1726	3996	0.11%	0.010%
18	13.440	1755	1760	1765	rBV2	14634	23231	0.63%	0.056%
19	14.016	1851	1858	1871	rBV	1488451	2075777	56.13%	4.967%
20	14.298	1899	1906	1919	rBV	1863803	2595681	70.19%	6.210%
21	14.387	1919	1921	1924	rVB4	3966	4270	0.12%	0.010%
22	14.598	1951	1957	1968	rBV	1504386	2153761	58.24%	5.153%
23	14.822	1988	1995	2011	rBV	473447	881403	23.83%	2.109%
24	15.598	2120	2127	2137	rBV	2222656	3146473	85.08%	7.528%
25	15.728	2143	2149	2162	rVV	596082	810705	21.92%	1.940%
26	15.834	2164	2167	2174	rVB4	11380	16448	0.44%	0.039%
27	17.034	2368	2371	2374	rBV5	4069	4886	0.13%	0.012%
28	17.163	2390	2393	2399	rVB6	4556	6429	0.17%	0.015%
29	17.369	2420	2428	2438	rBV	1705280	2396074	64.79%	5.733%
30	17.469	2439	2445	2459	rVV2	2238538	3245929	87.77%	7.766%
31	17.769	2492	2496	2497	rBV4	4538	5508	0.15%	0.013%
32	18.004	2531	2536	2541	rBV9	5329	10266	0.28%	0.025%
33	18.216	2569	2572	2578	rBV7	7224	10877	0.29%	0.026%
34	19.286	2750	2754	2759	rVB2	26814	33369	0.90%	0.080%
35	19.351	2762	2765	2770	rVV2	24153	31032	0.84%	0.074%
36	19.716	2821	2827	2833	rBV	2783241	3581828	96.85%	8.570%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092023\
Data File : BP017244.D
Acq On : 20 Sep 2023 18:00
Operator : MA/JU
Sample : PB155669BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK669

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	21.474	3121	3126	3135	rBV	1856266	2393649	64.72%	5.727%
38	23.827	3519	3526	3539	rVB2	1770925	3698288	100.00%	8.849%
39	23.998	3548	3555	3568	rVB	1222711	2573676	69.59%	6.158%




Sum of corrected areas: 41795359

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092023\
Data File : BP017244.D
Acq On : 20 Sep 2023 18:00
Operator : MA/JU
Sample : PB155669BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

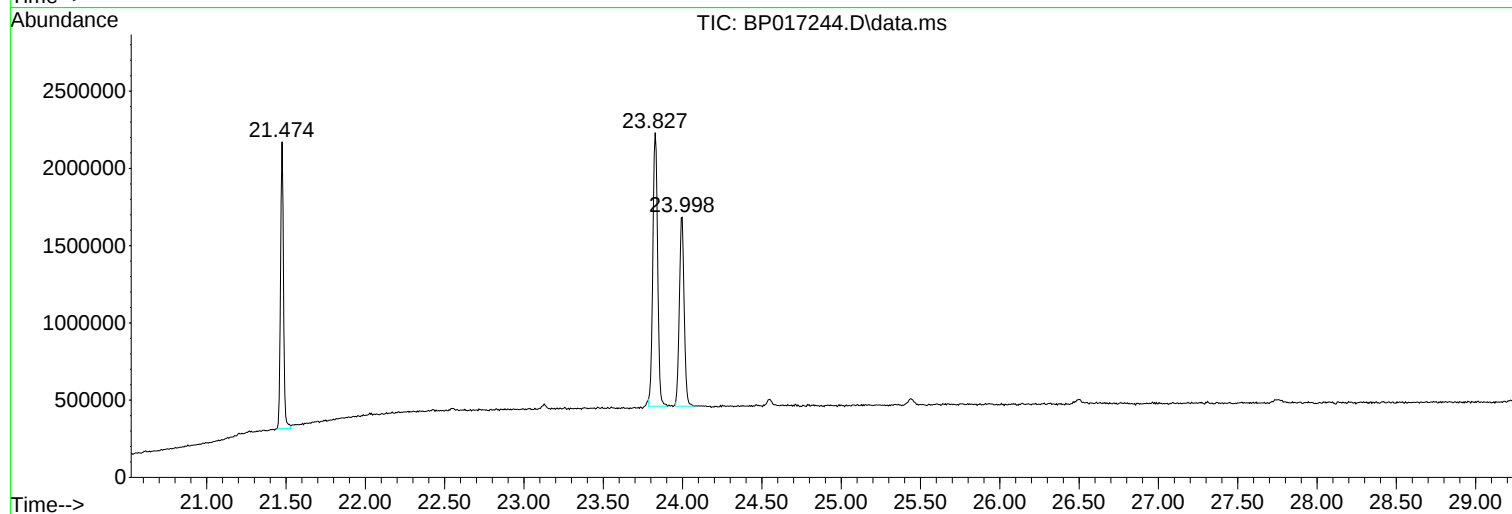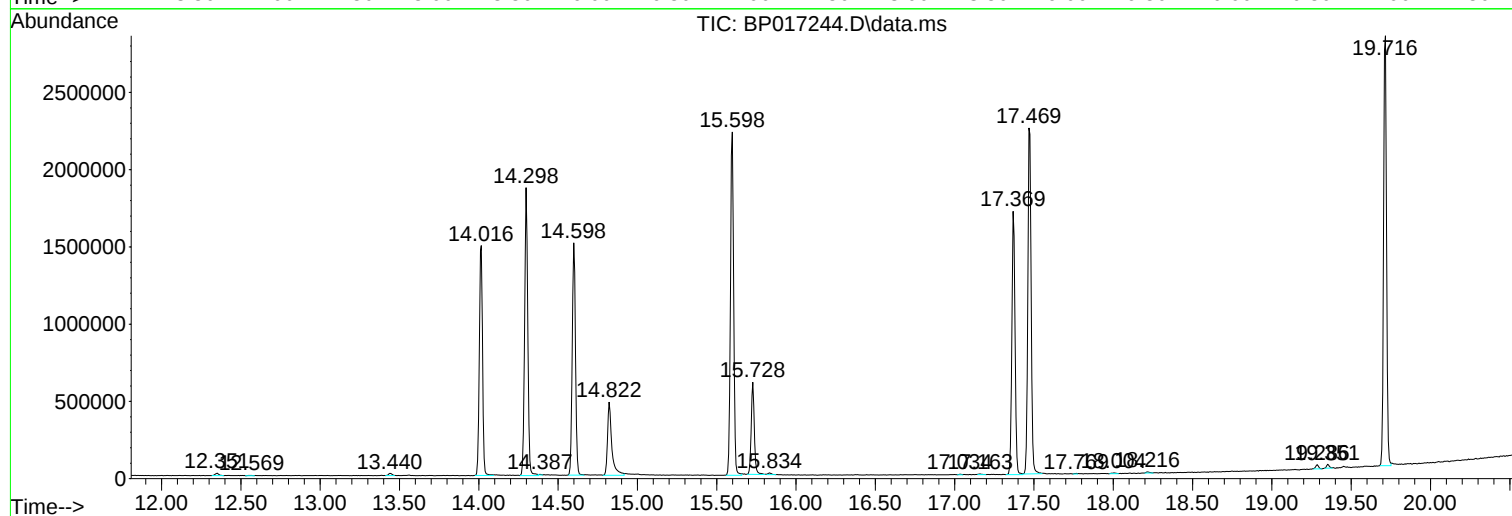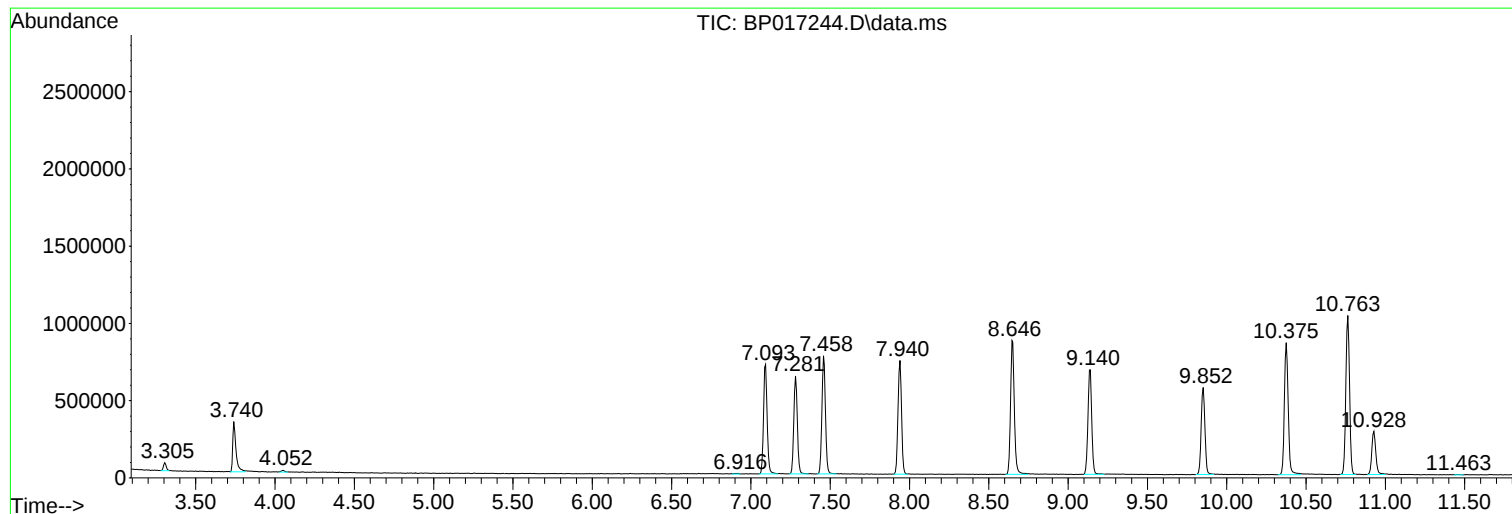

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092023\
Data File : BP017244.D
Acq On : 20 Sep 2023 18:00
Operator : MA/JU
Sample : PB155669BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092023\
Data File : BP017244.D
Acq On : 20 Sep 2023 18:00
Operator : MA/JU
Sample : PB155669BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------