



2-Nitrophenol

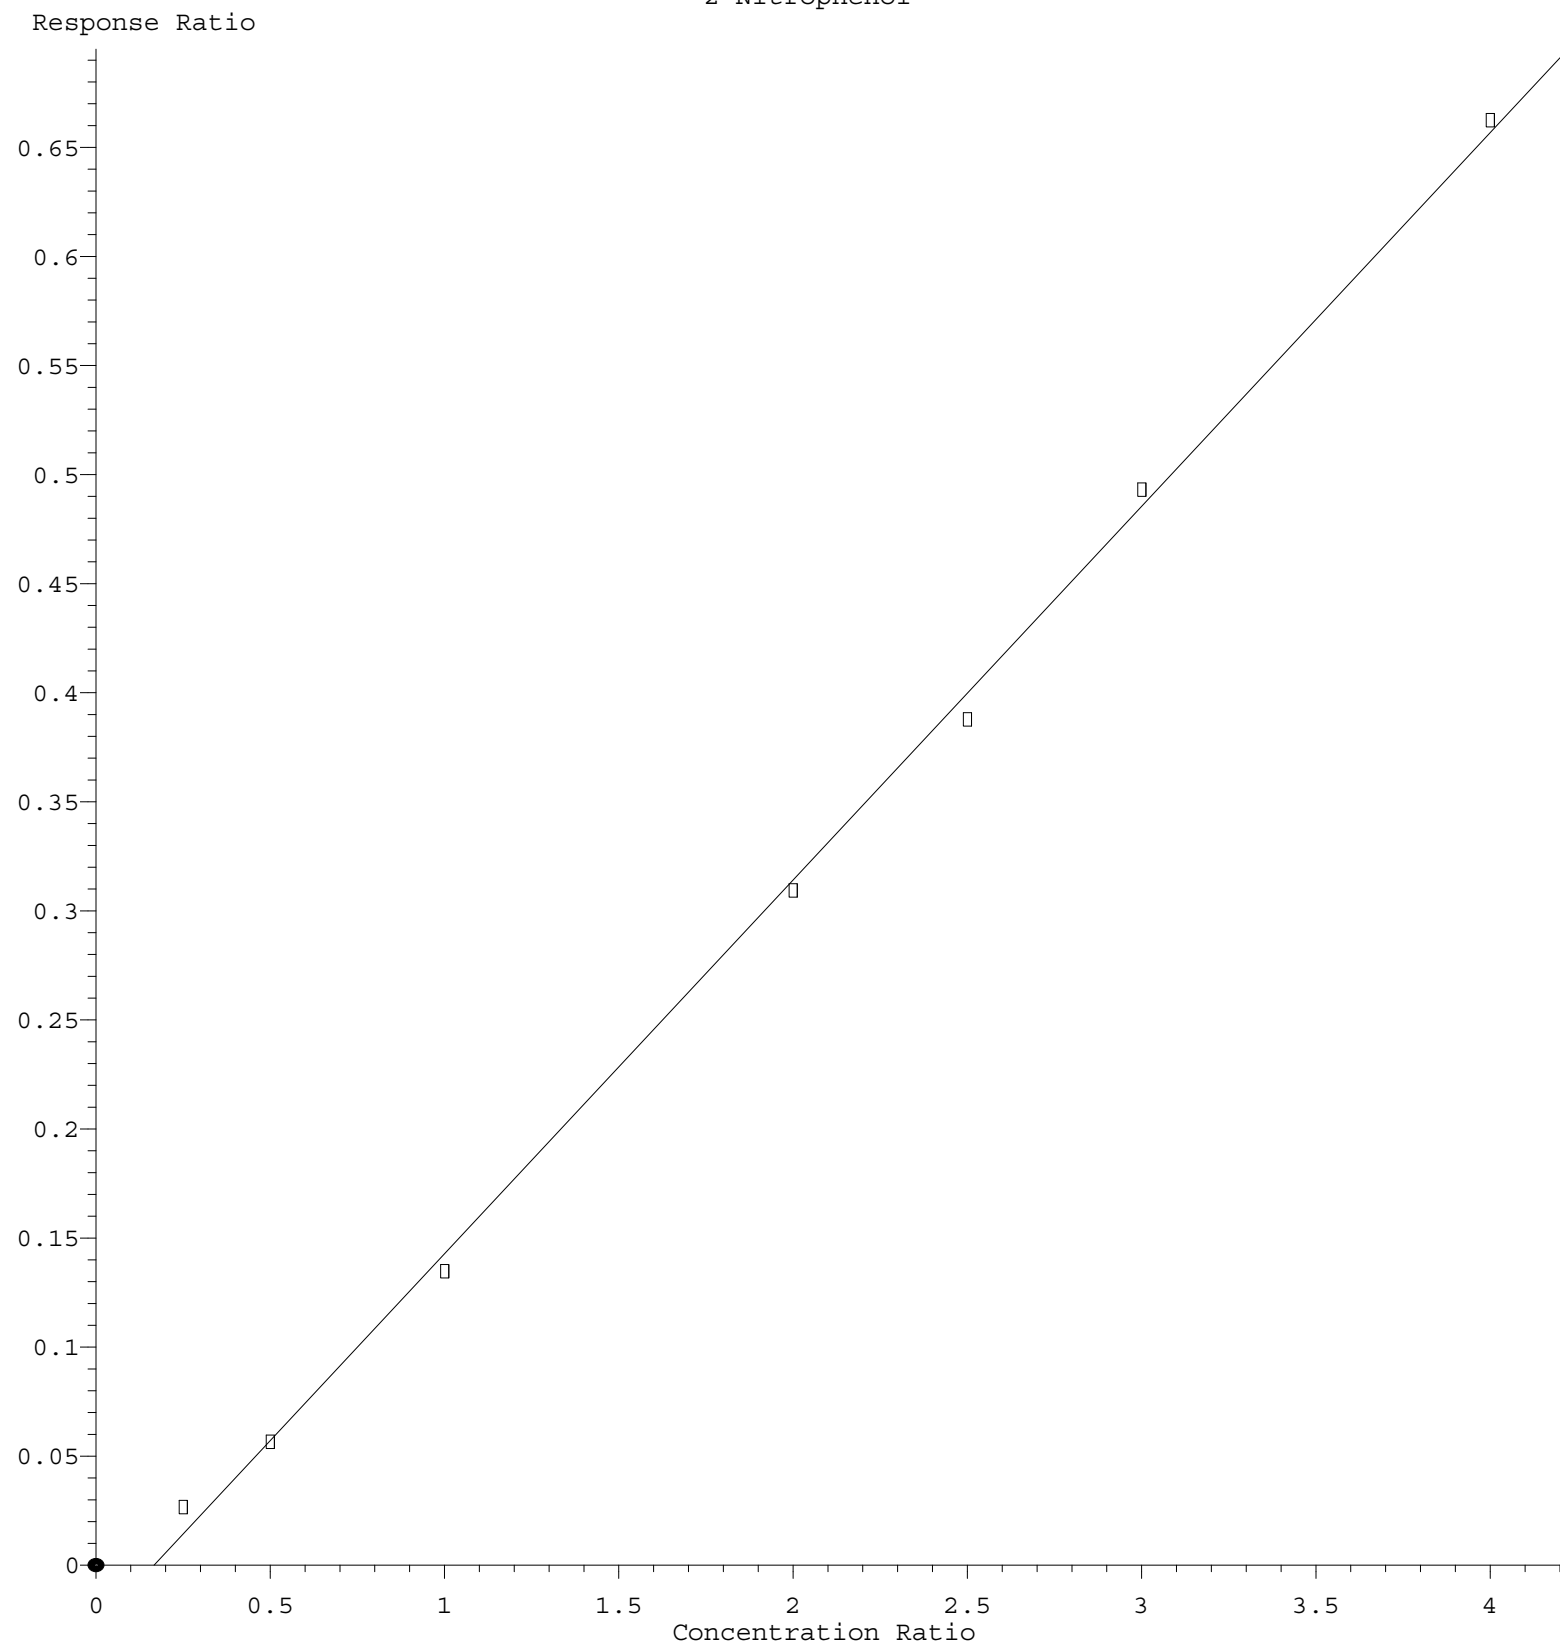

Response = $1.713 \times 10^{-1} \times \text{Amt} - 2.854 \times 10^{-2}$
 Coef of Det (r^2) = 0.998589 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M
 Calibration Table Last Updated: Thu Sep 22 02:45:14 2022


2,4-Dinitrophenol

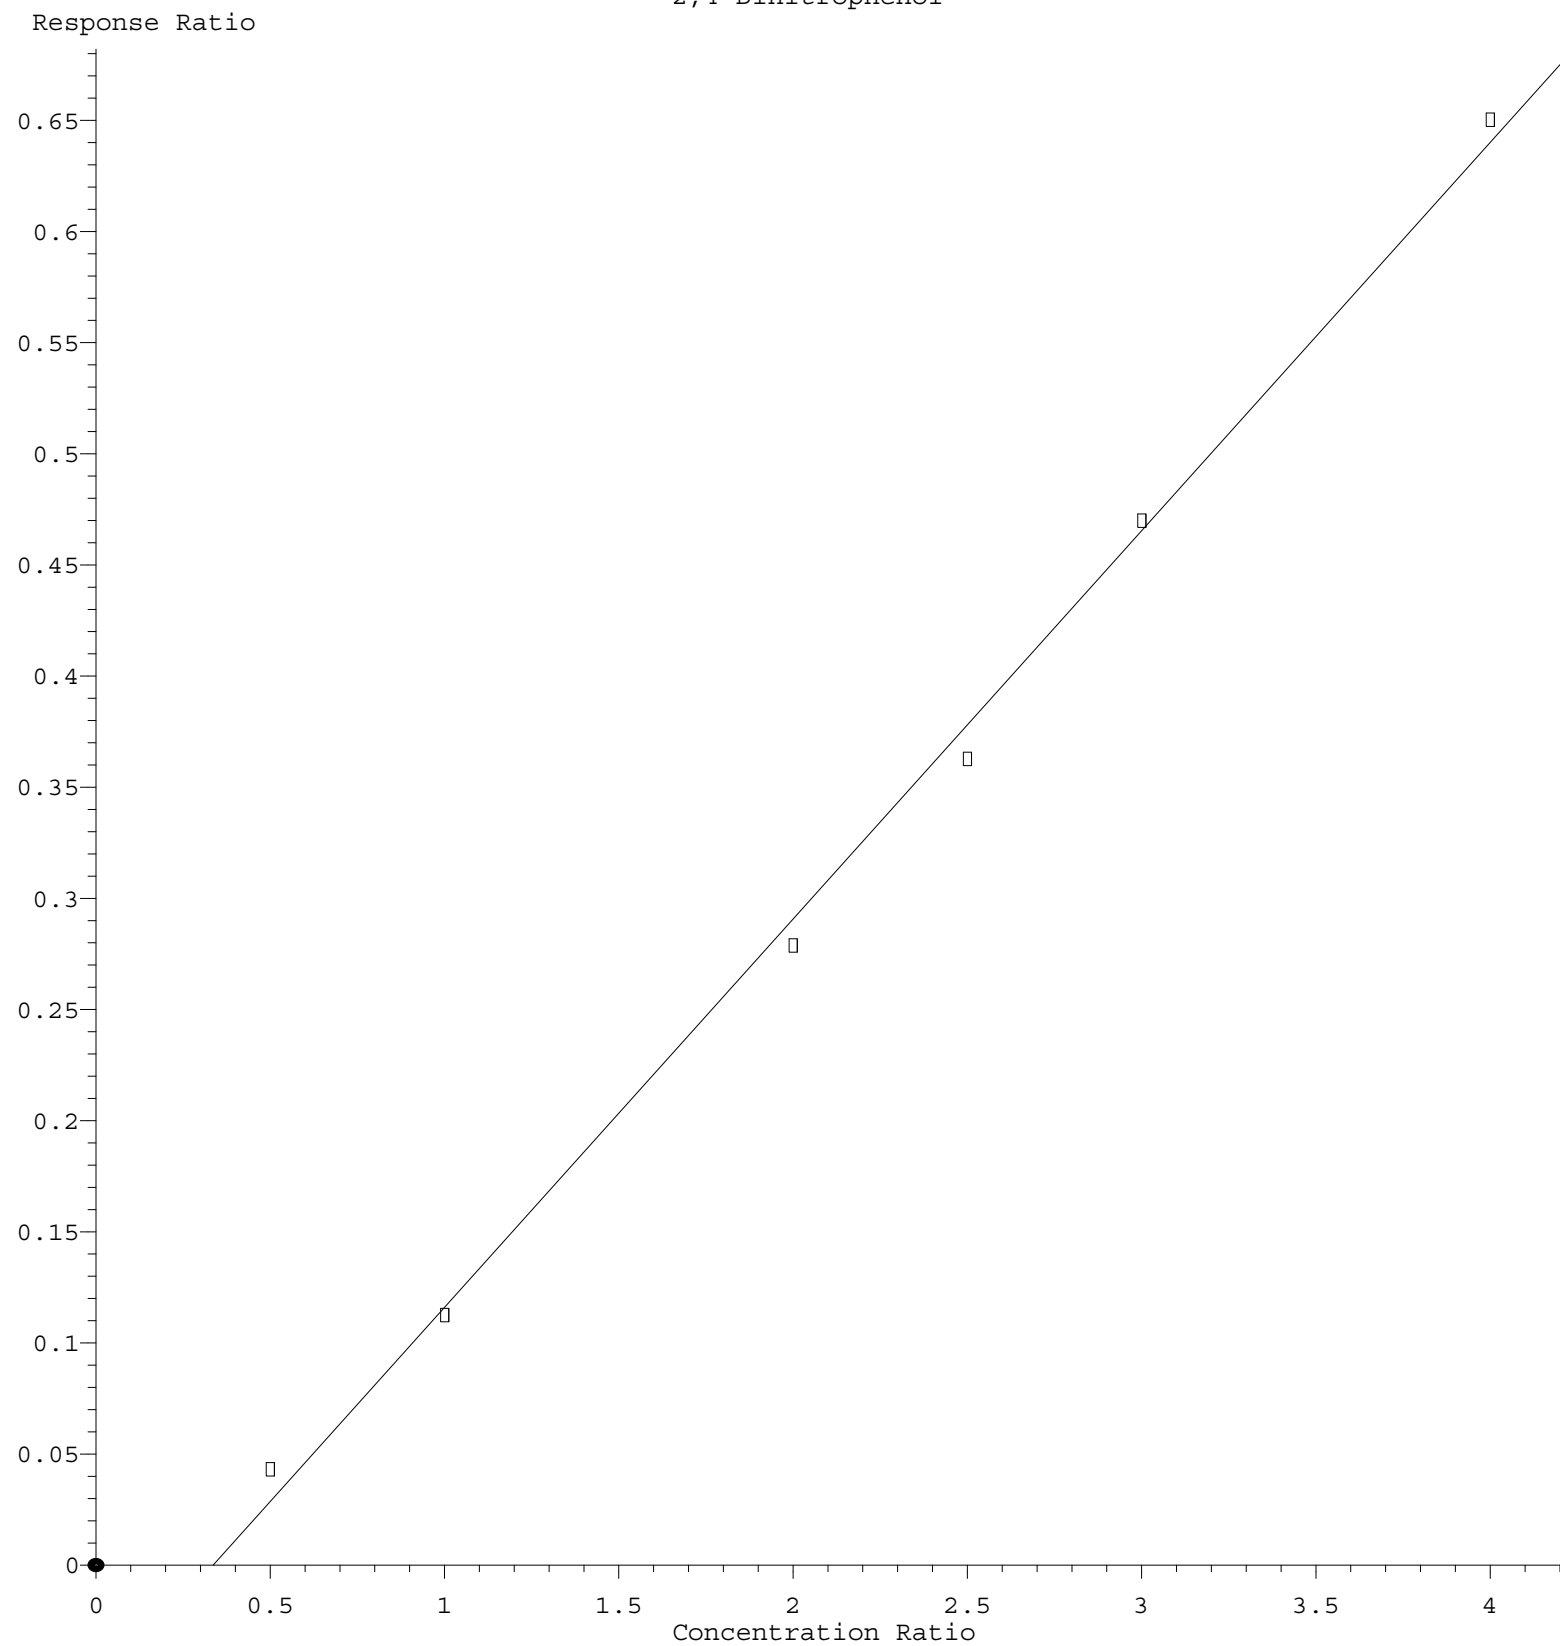

Response = $1.746 \times 10^{-1} \times \text{Amt} - 5.871 \times 10^{-2}$
 Coef of Det (r^2) = 0.997174 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M
 Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

Benzoic acid

Response Ratio

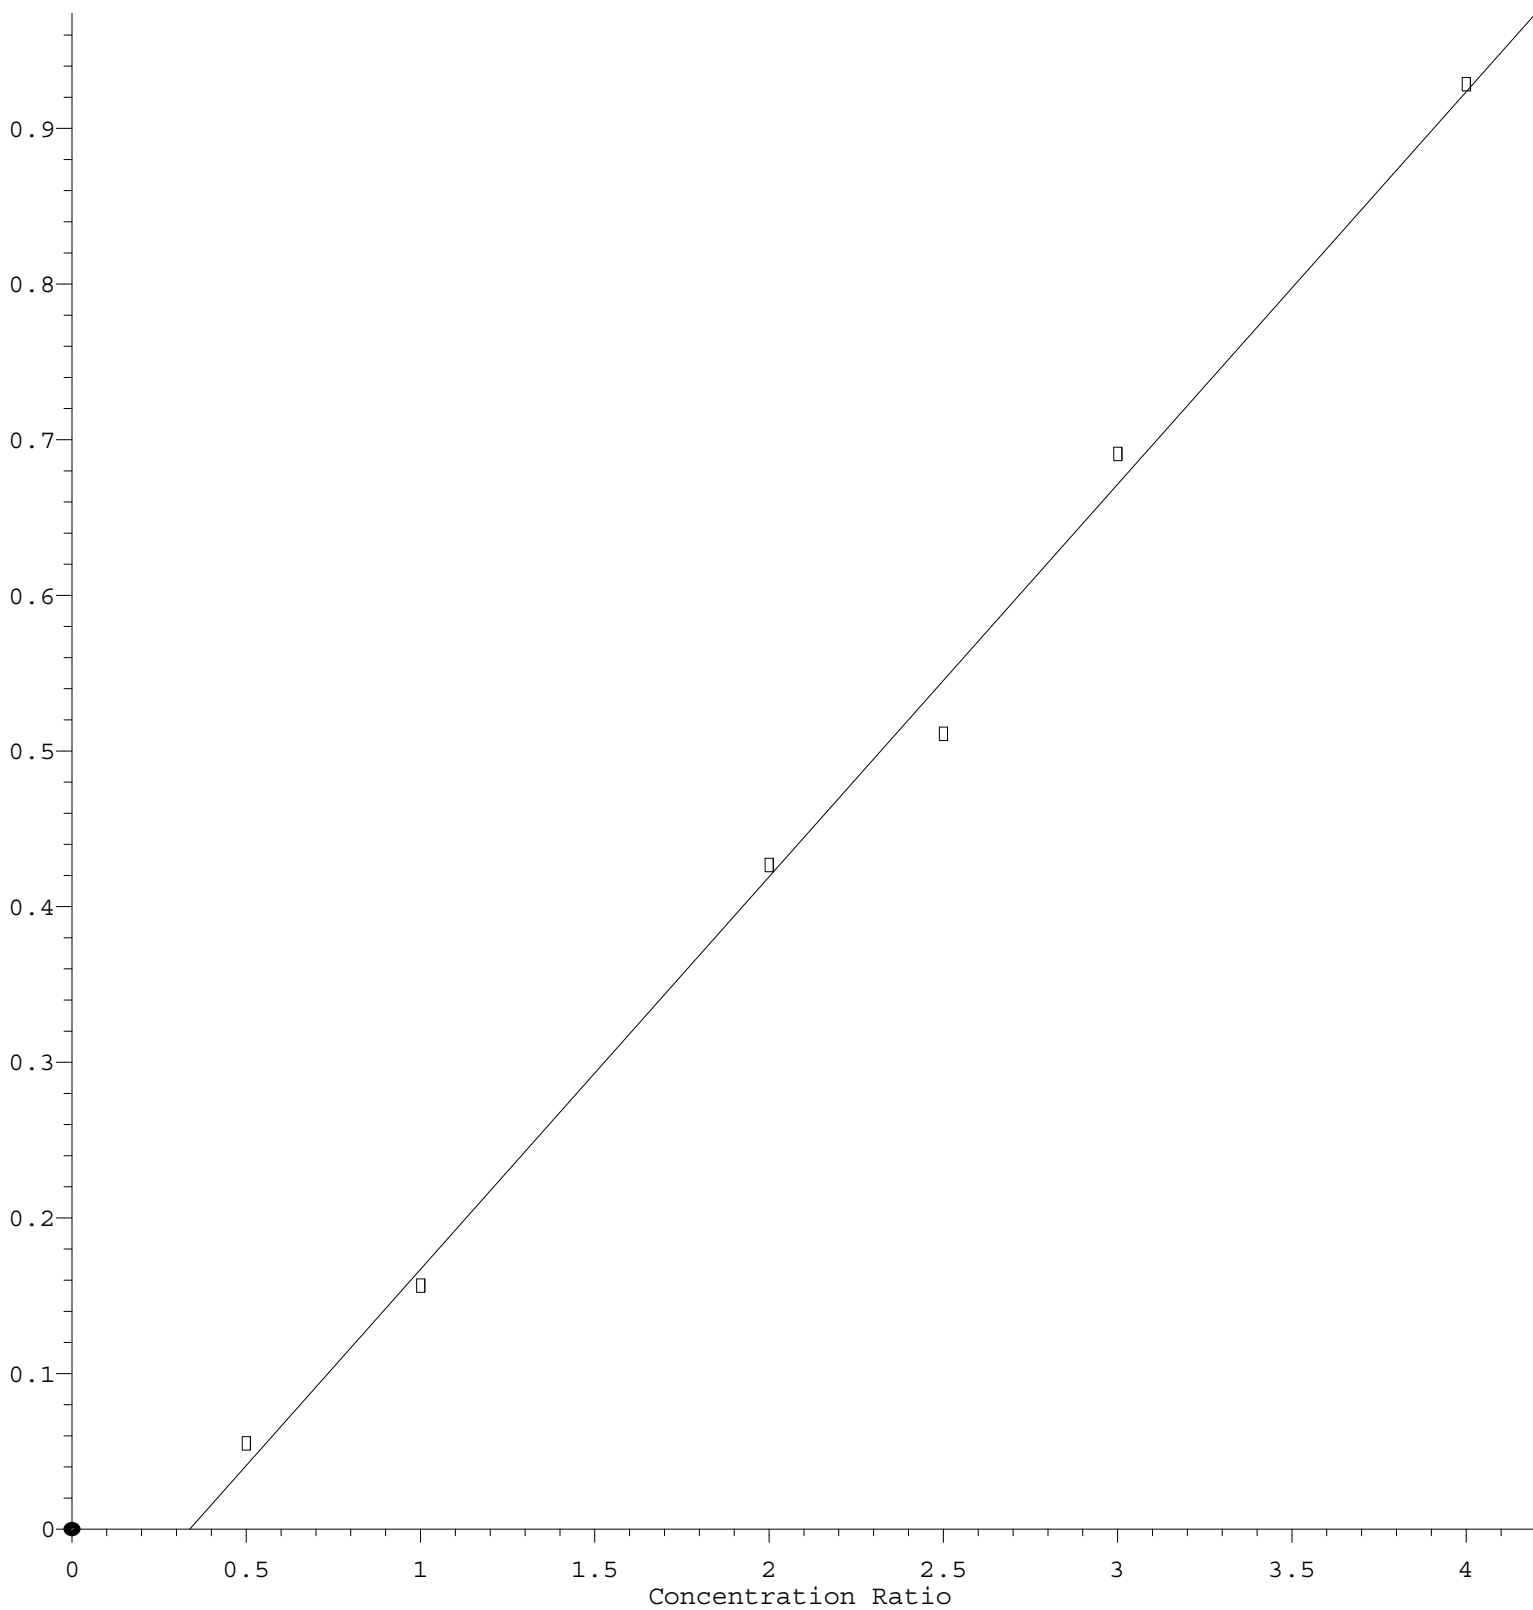

$$\text{Response} = 2.523\text{e-}001 * \text{Amt} - 8.525\text{e-}002$$


Coef of Det (r^2) = 0.996353 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M

Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

4-Nitroaniline

Response Ratio

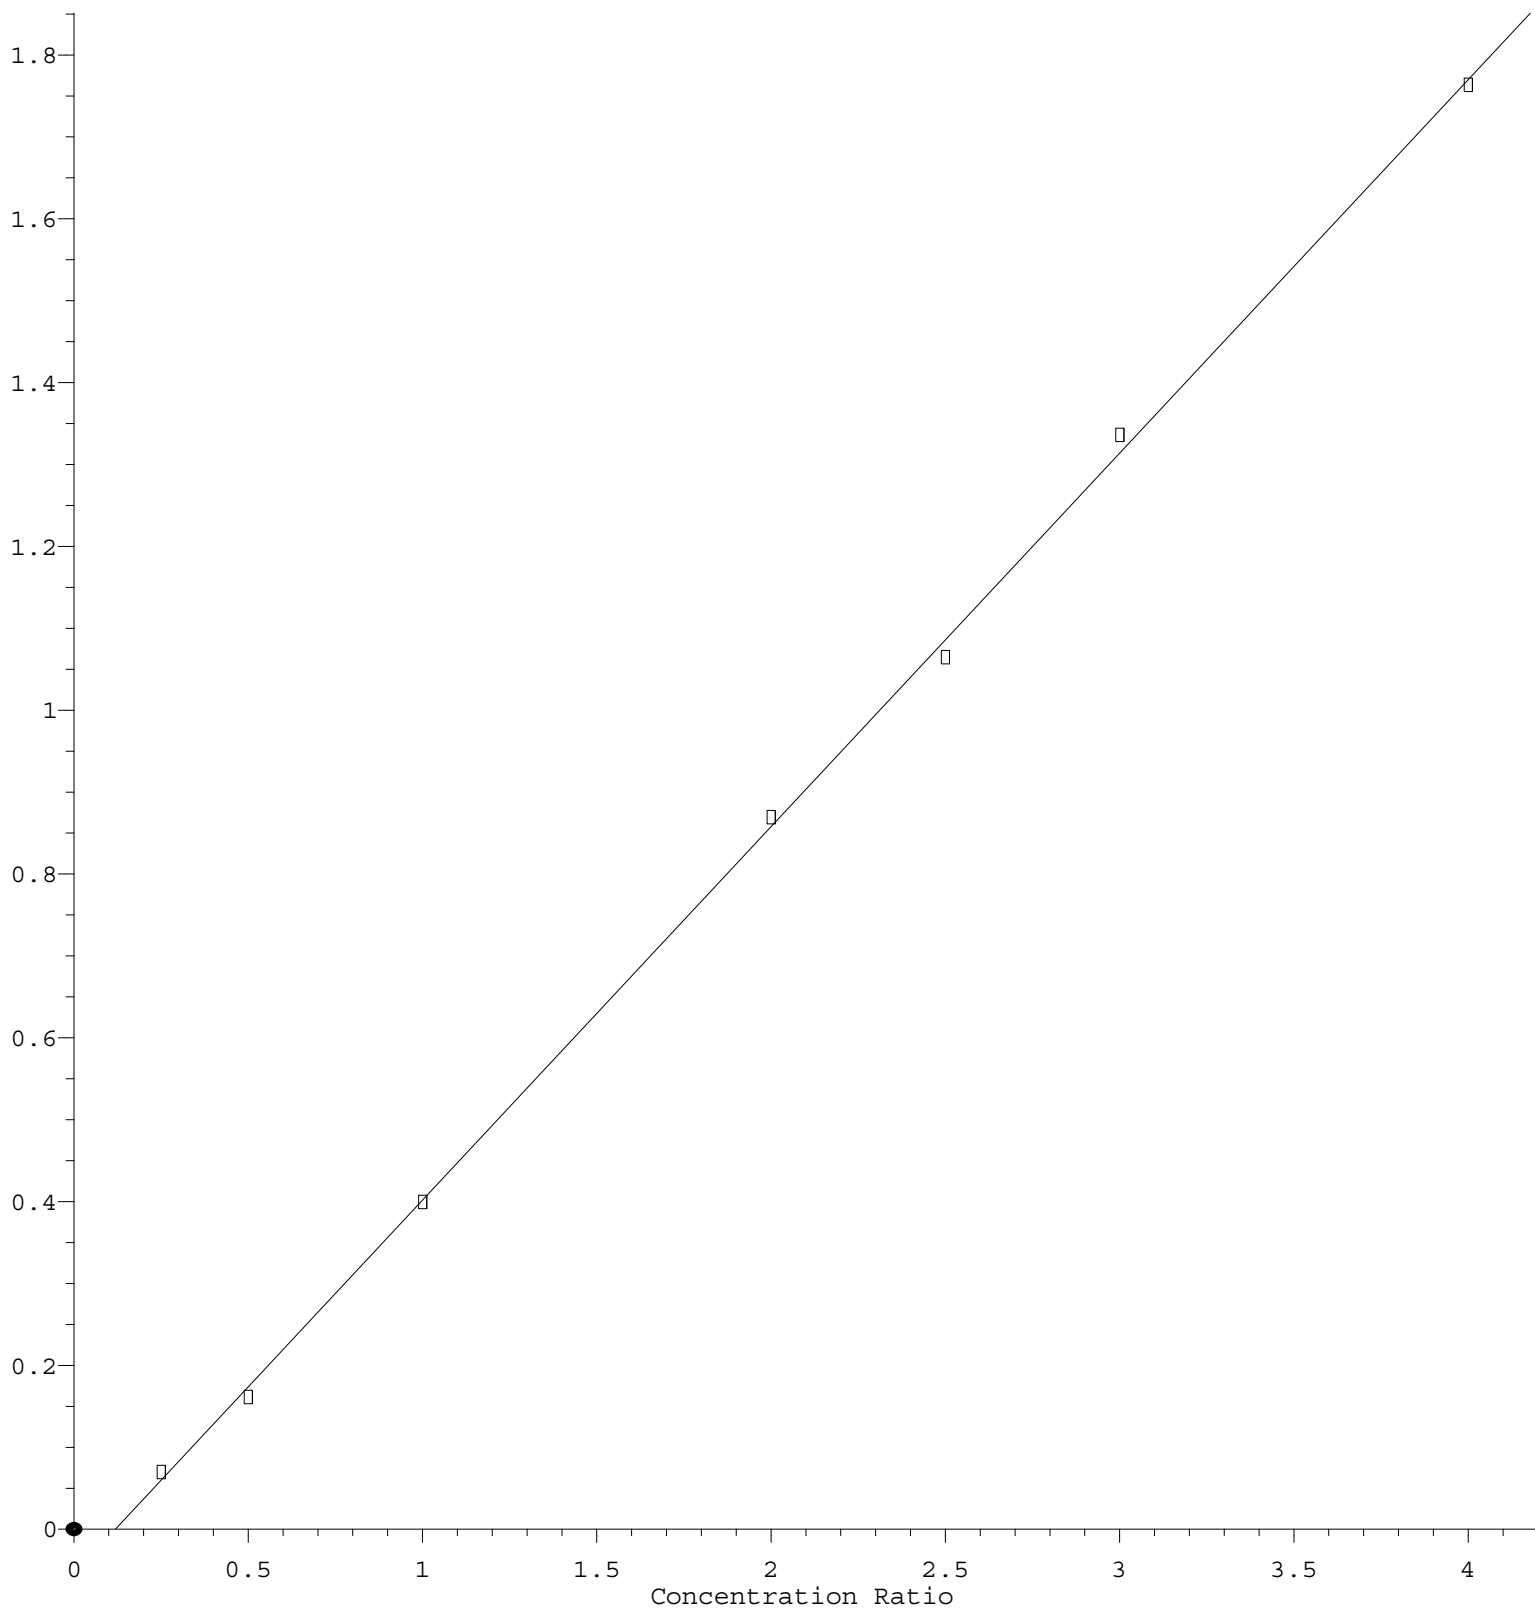

$$\text{Response} = 4.562\text{e-}001 * \text{Amt} - 5.442\text{e-}002$$


Coef of Det (r^2) = 0.999424 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M

Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

2,4-Dinitrotoluene

Response Ratio

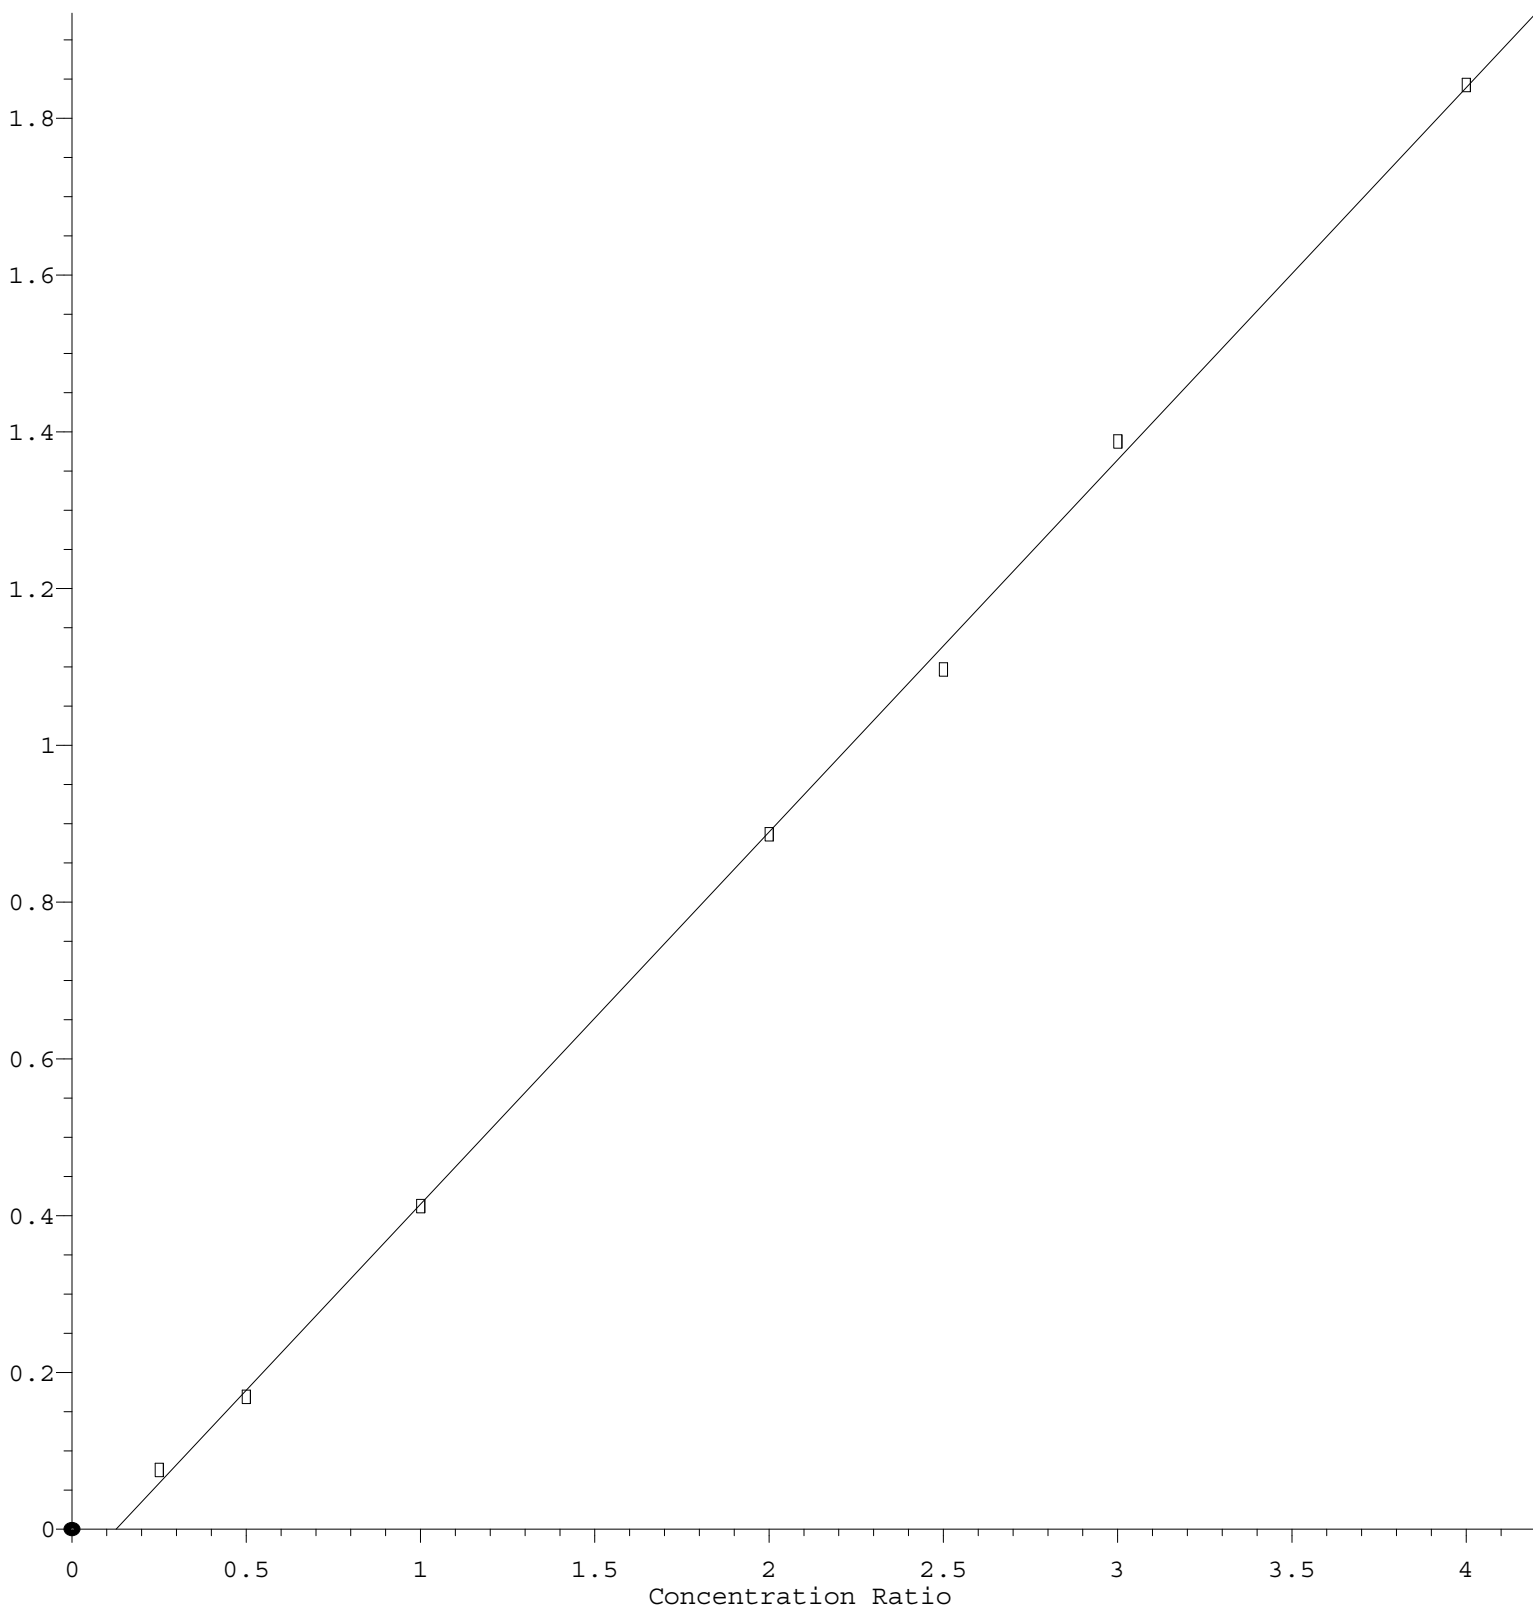


$$\text{Response} = 4.748\text{e-}001 * \text{Amt} - 6.028\text{e-}002$$

Coef of Det (r^2) = 0.999289 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M


Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

4,6-Dinitro-2-methylphenol

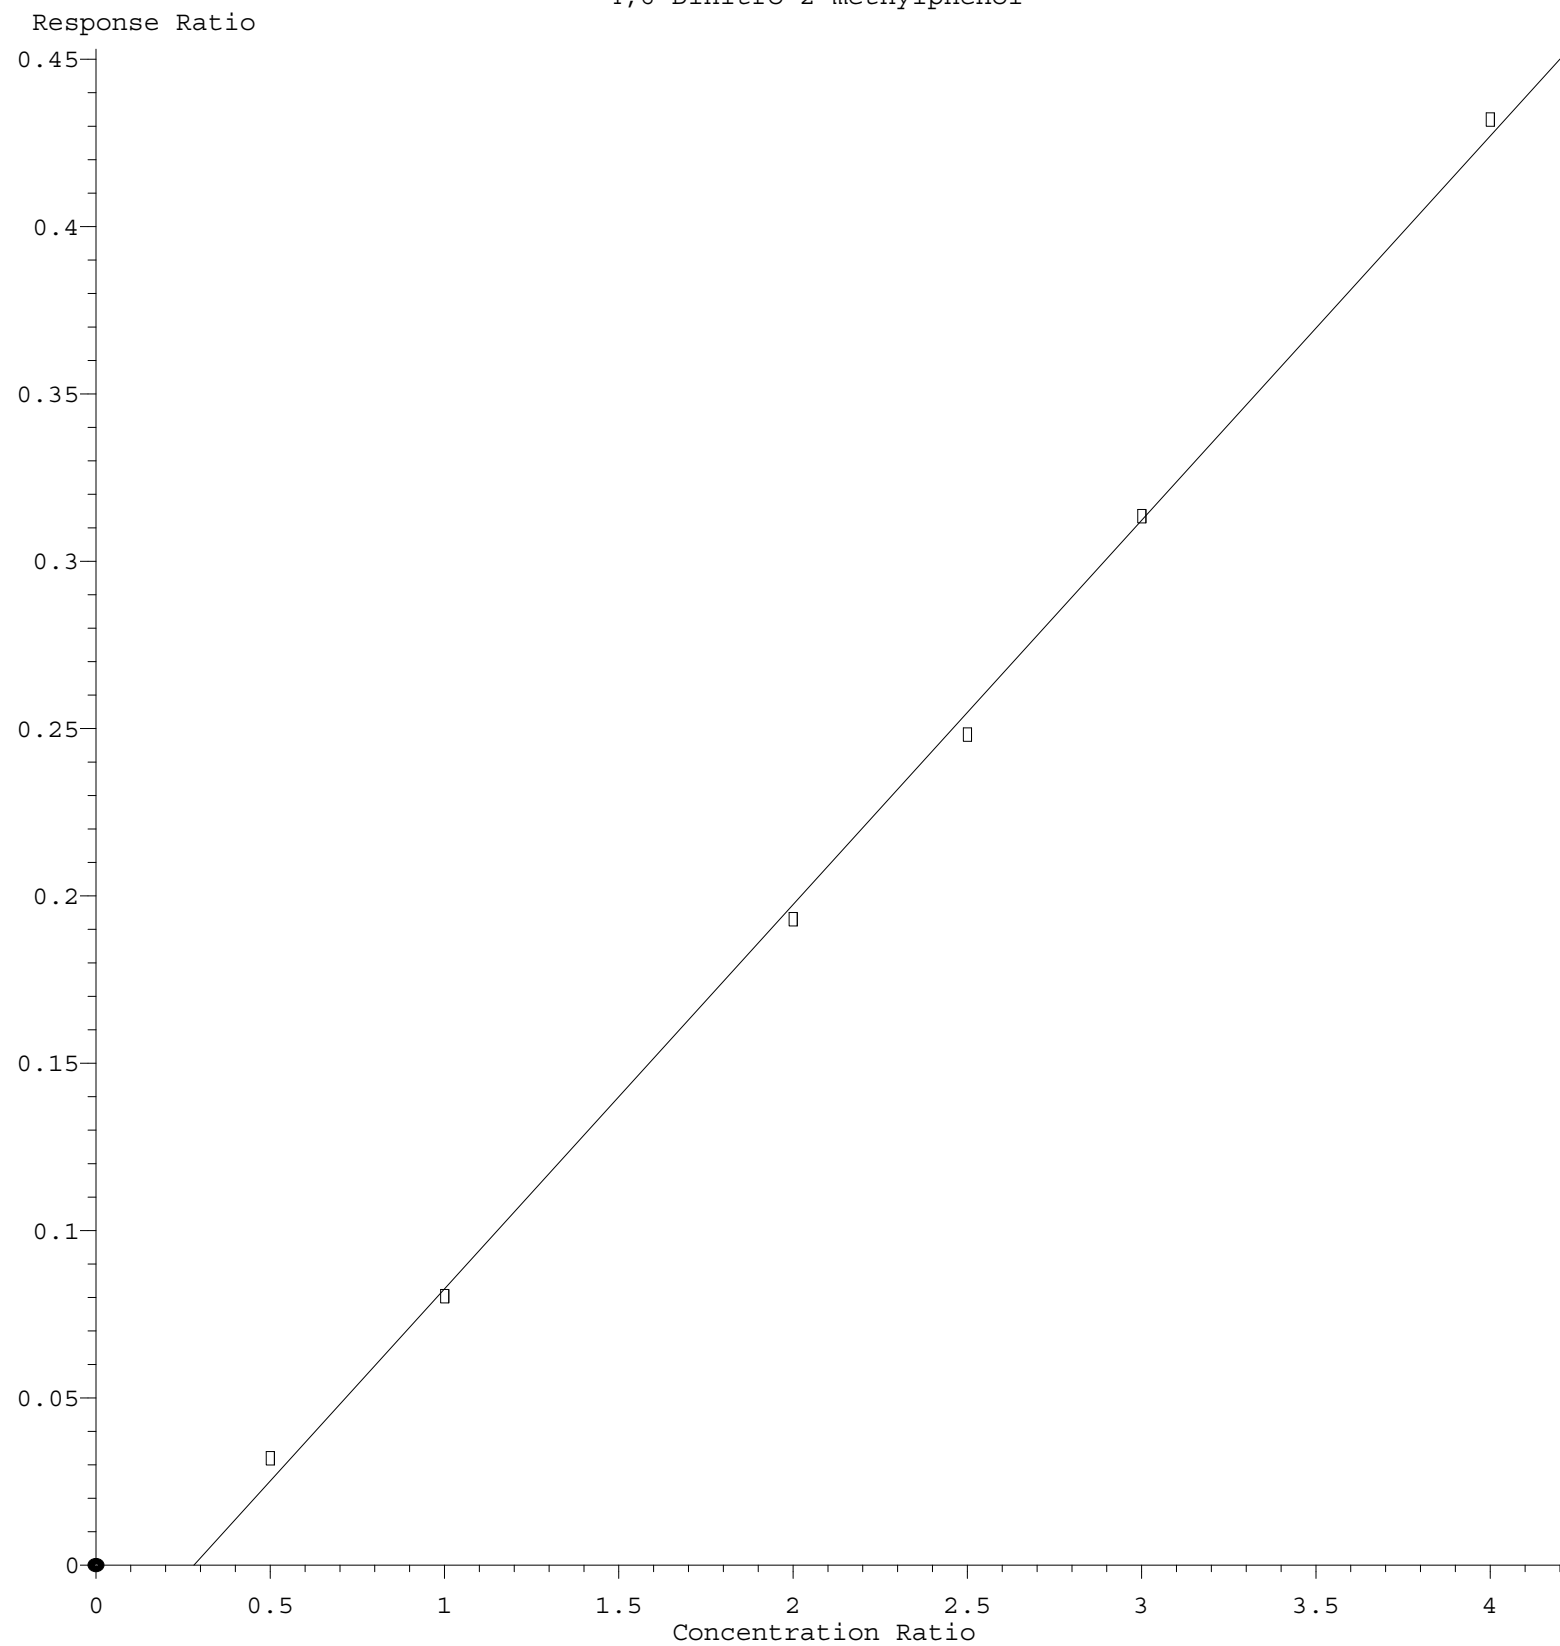

Response = $1.148 \times 10^{-1} \times \text{Amt} - 3.226 \times 10^{-2}$
 Coef of Det (r^2) = 0.998735 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M
 Calibration Table Last Updated: Thu Sep 22 02:45:14 2022


Pentachlorophenol

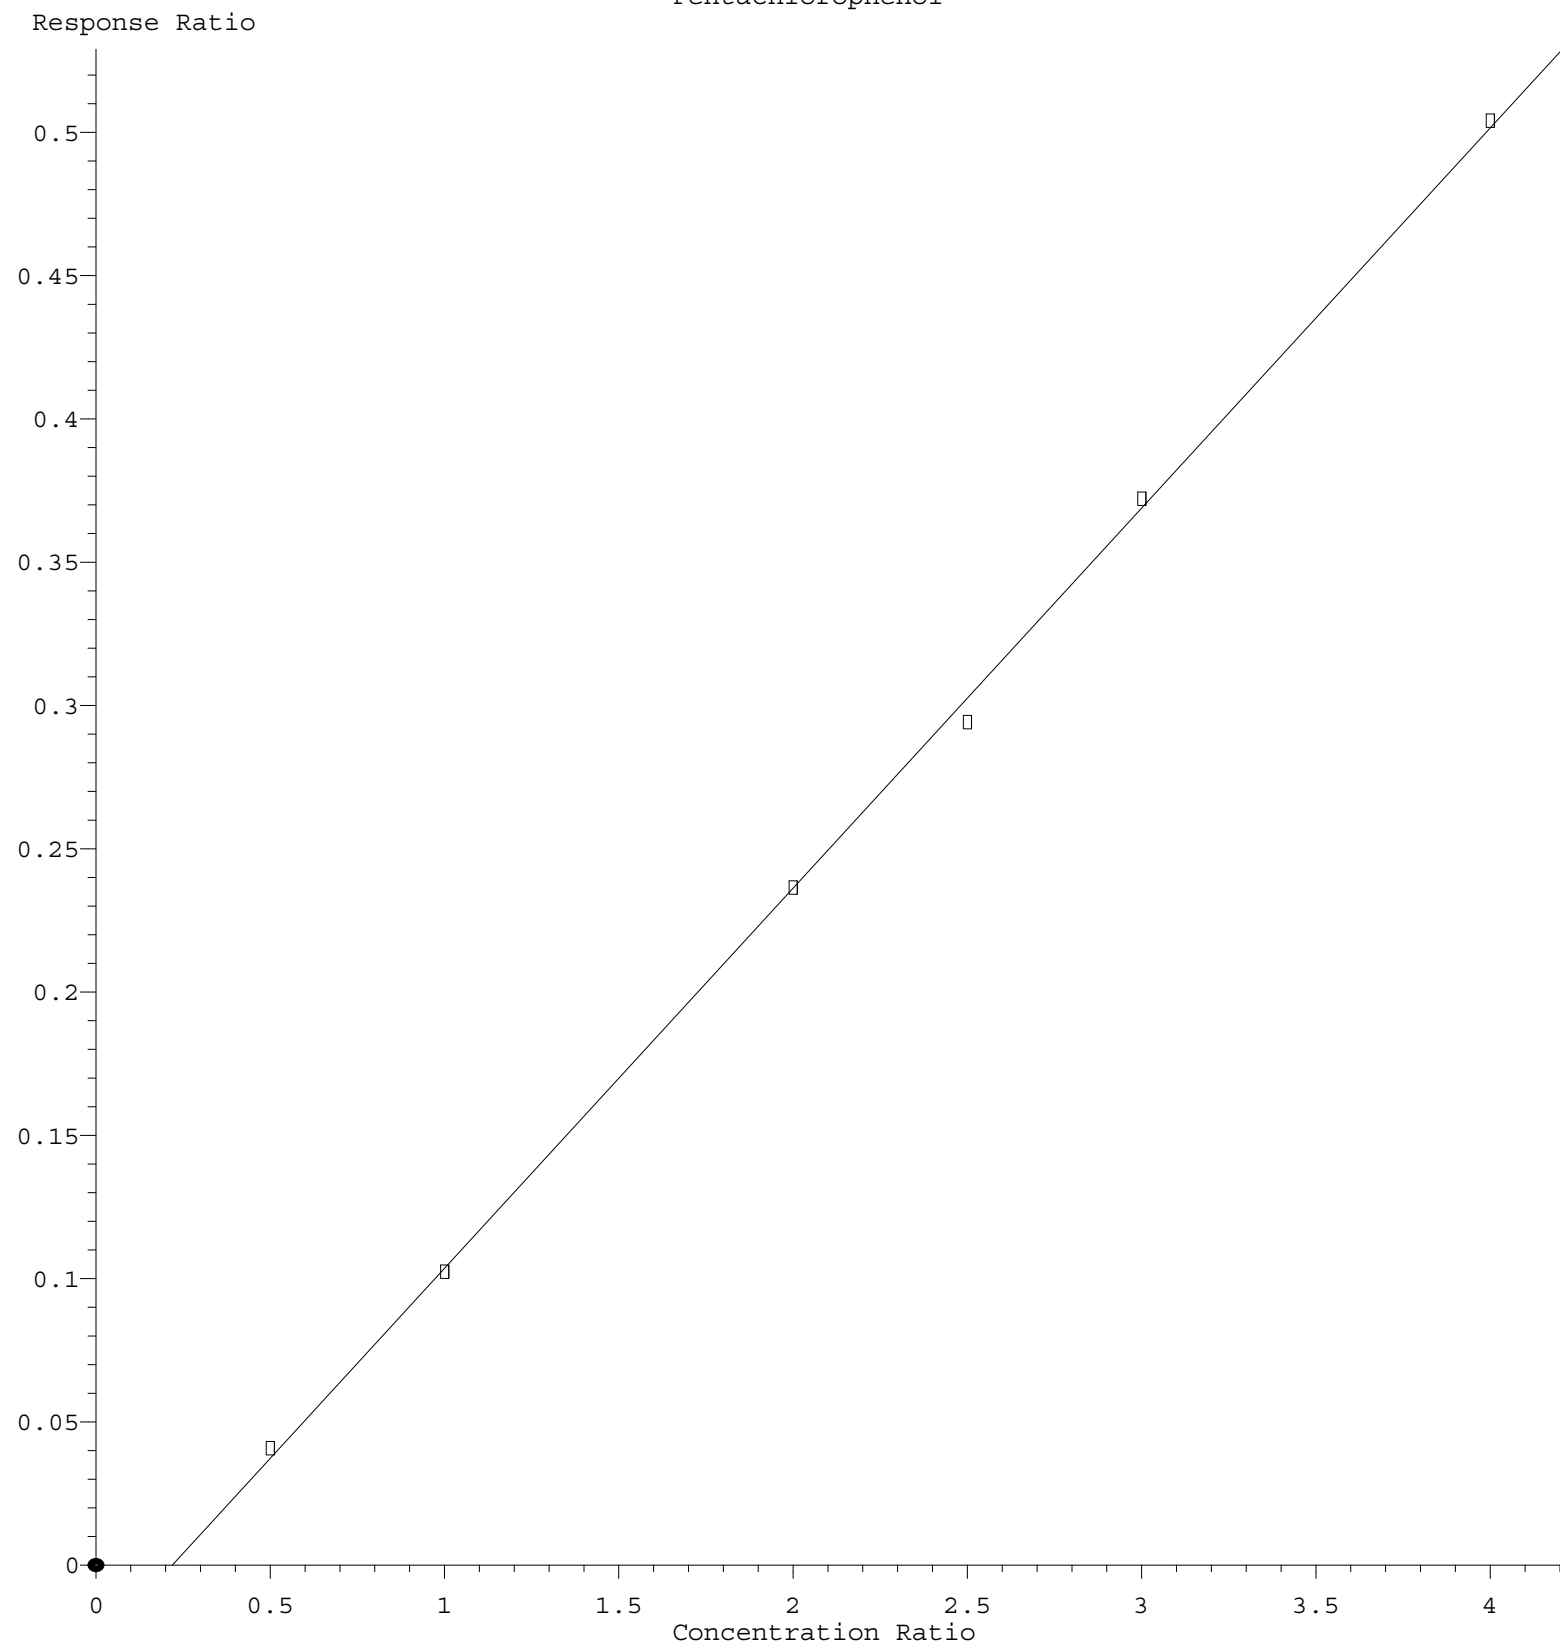

Response = 1.326e-001 * Amt - 2.908e-002
 Coef of Det (r^2) = 0.999311 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M
 Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

Bis(2-ethylhexyl)phthalate

Response Ratio

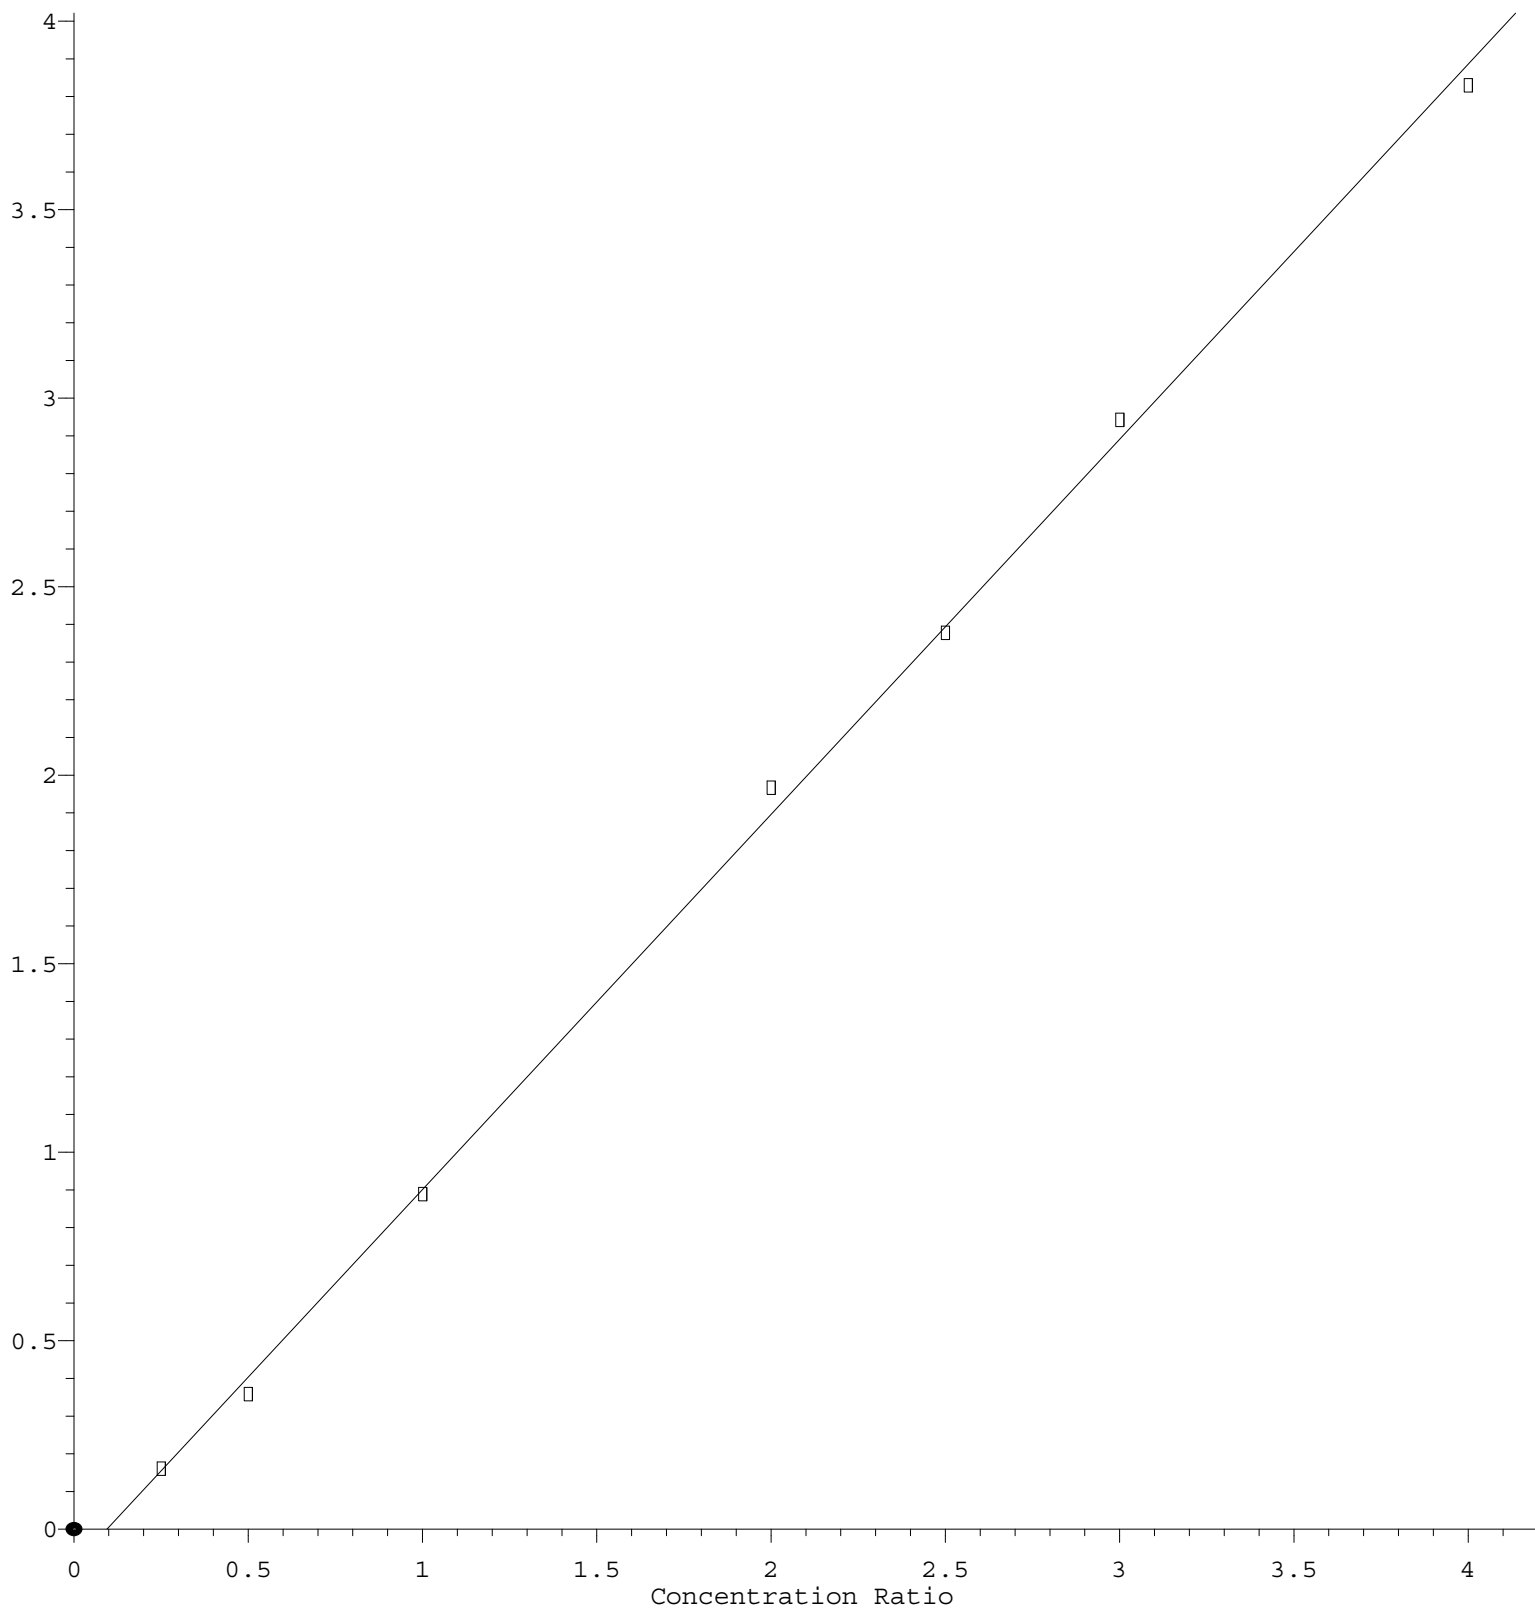

$$\text{Response} = 9.950\text{e-}001 * \text{Amt} - 9.439\text{e-}002$$


Coef of Det (r^2) = 0.998835 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M

Calibration Table Last Updated: Thu Sep 22 02:45:14 2022

Butylbenzylphthalate

Response Ratio

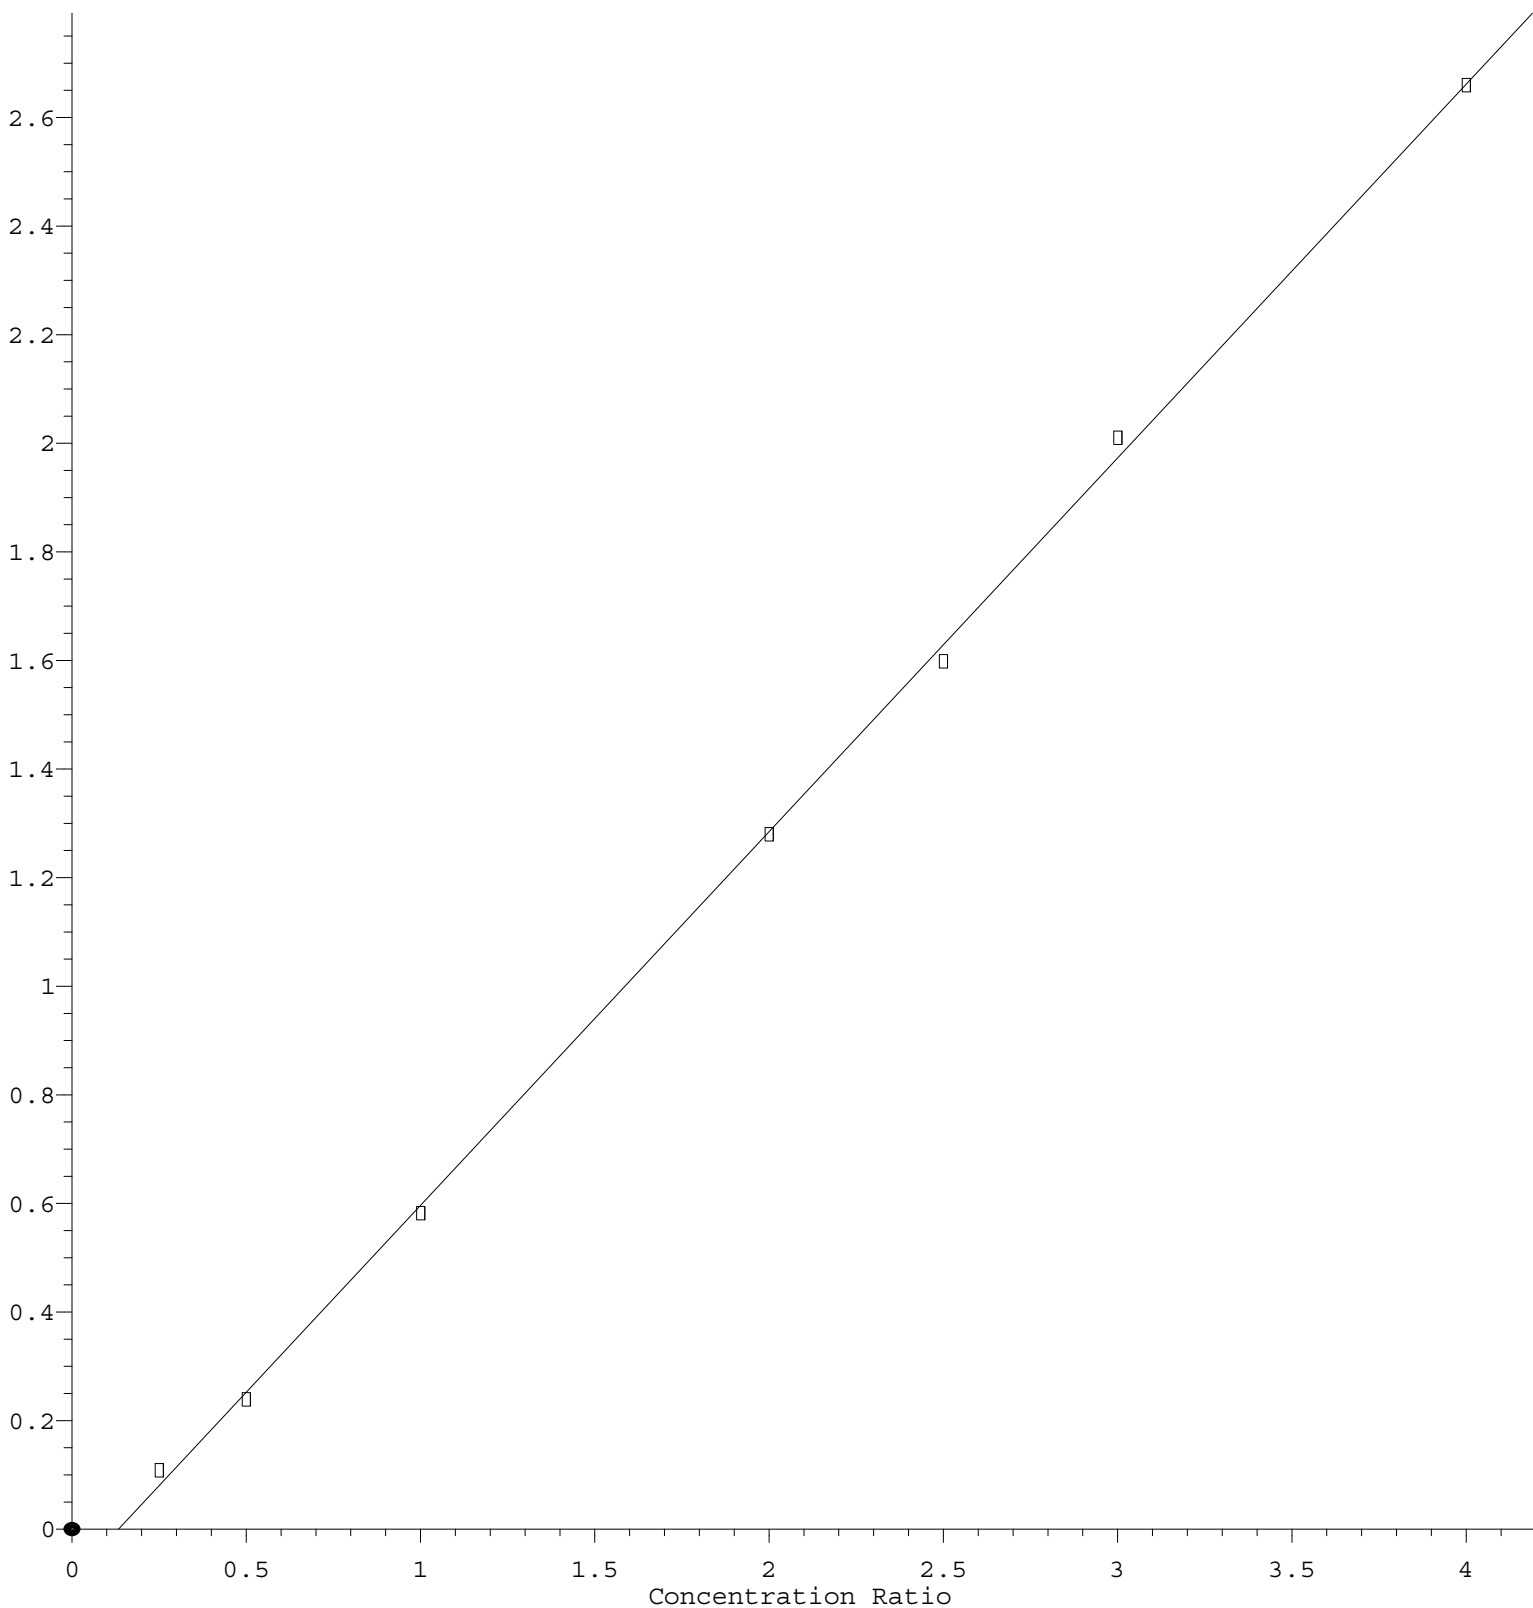

$$\text{Response} = 6.885\text{e-}001 * \text{Amt} - 9.237\text{e-}002$$

Coef of Det (r^2) = 0.999356 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP092122.M

Calibration Table Last Updated: Thu Sep 22 02:45:14 2022