


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092122\
 Data File : BP011768.D
 Acq On : 21 Sep 2022 15:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 22 02:45:14 2022

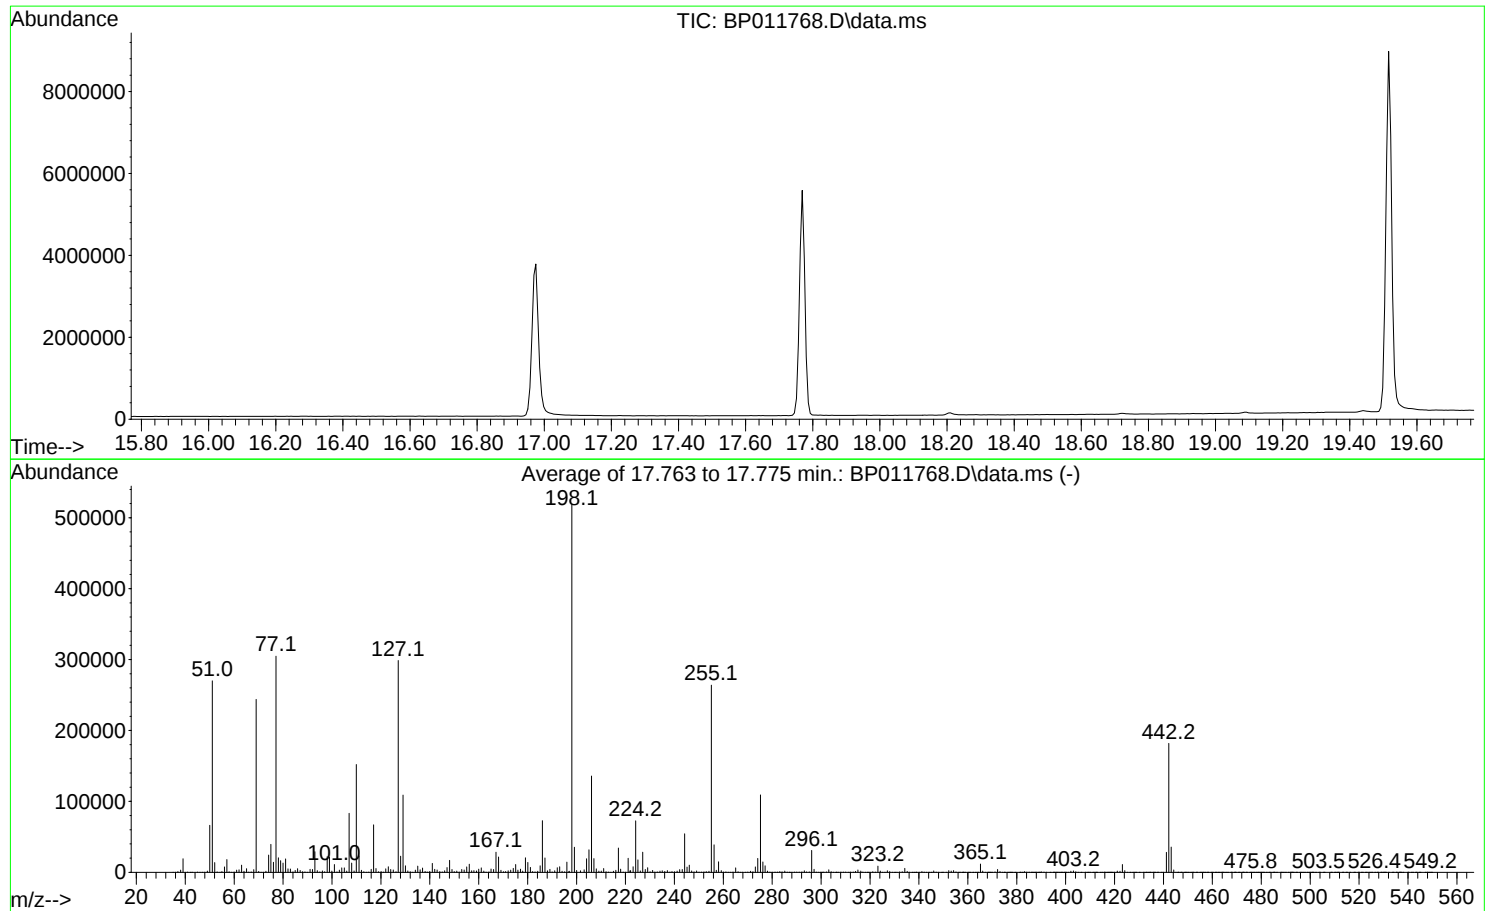




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	270044	PASS
68	69	0.00	2	1.6	3825	PASS
69	198	0.00	100	47.0	243787	PASS
70	69	0.00	2	0.6	1349	PASS
127	198	10	80	57.6	298607	PASS
197	198	0.00	2	0.3	1420	PASS
198	198	100	100	100.0	518811	PASS
199	198	5	9	6.8	35354	PASS
275	198	10	60	21.0	109075	PASS
365	198	1	100	2.2	11556	PASS
441	198	0.01	100	5.4	28189	PASS
442	442	100	100	100.0	181733	PASS
443	442	15	24	19.5	35472	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092122\
 Data File : BP011768.D
 Acq On : 21 Sep 2022 15:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 06:47:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

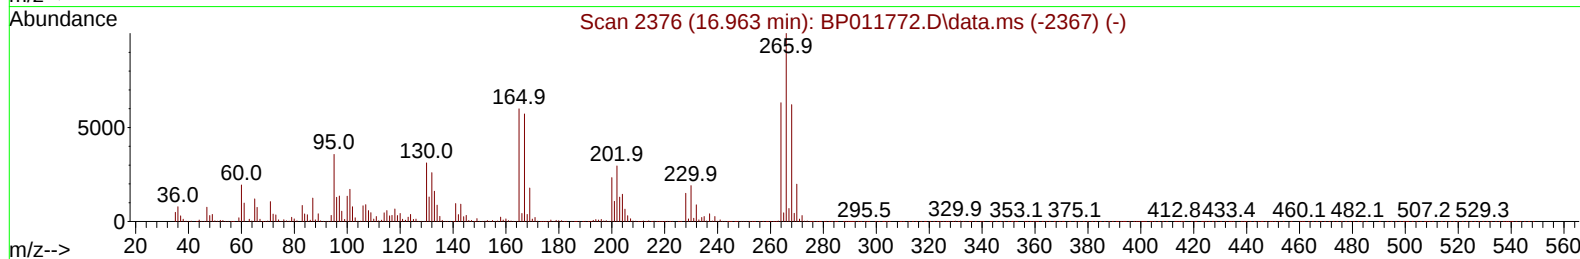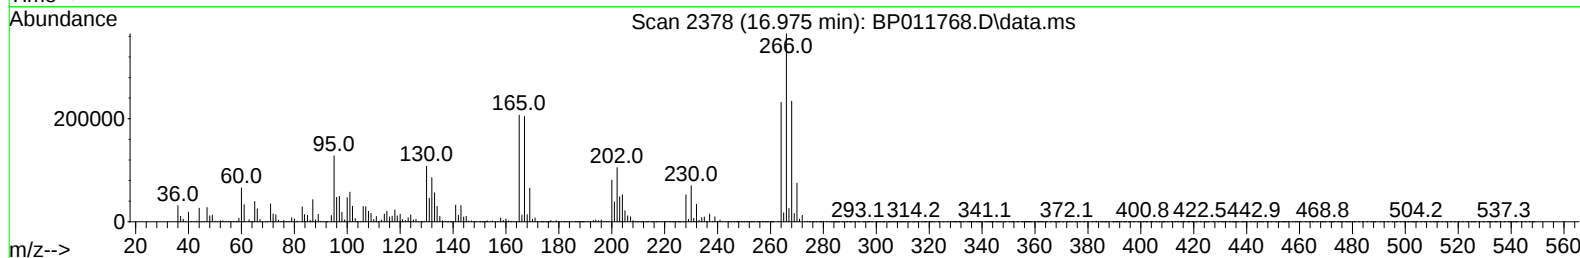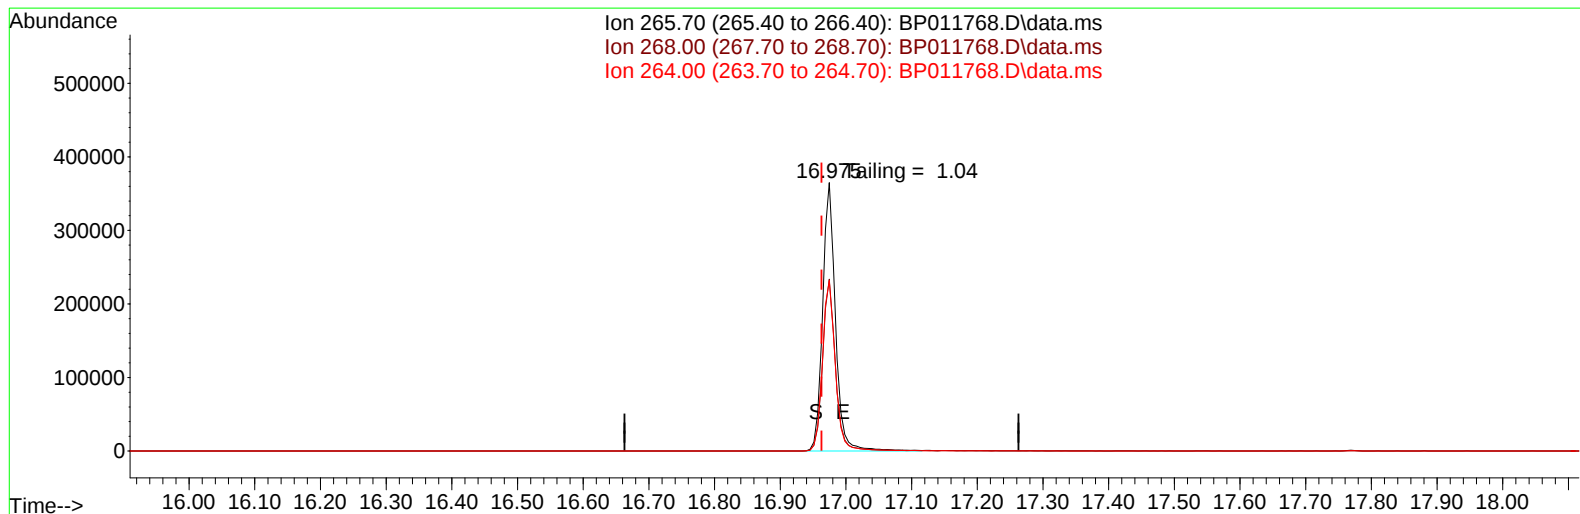

TIC: BP011768.D\data.ms

(70) Pentachlorophenol (C)

16.975min (+ 0.012) 205038.87 ng




response 494985

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	64.05
264.00	63.20	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092122\
 Data File : BP011768.D
 Acq On : 21 Sep 2022 15:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 06:47:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

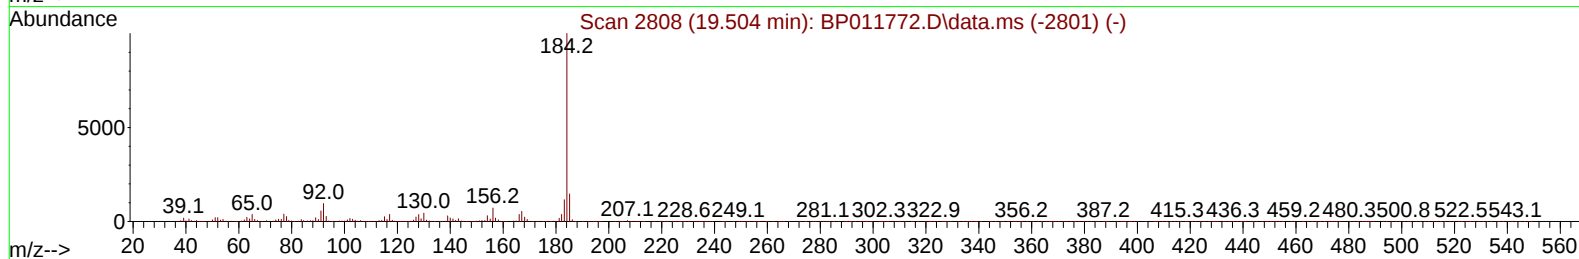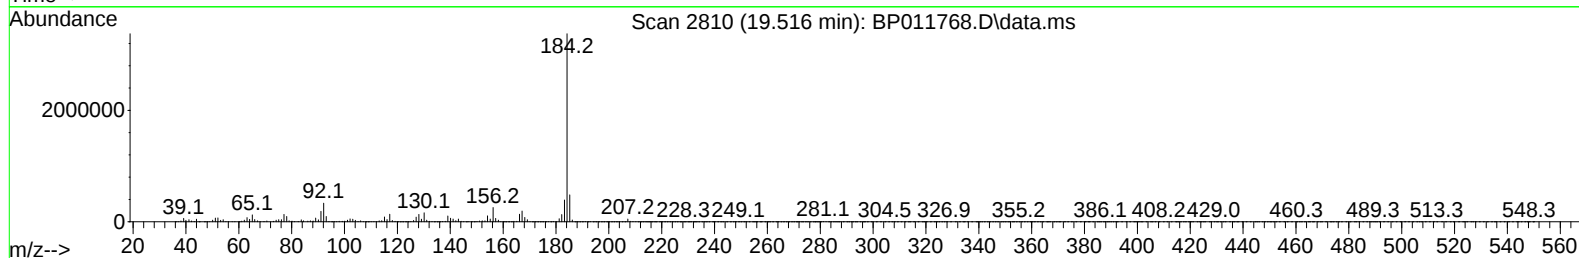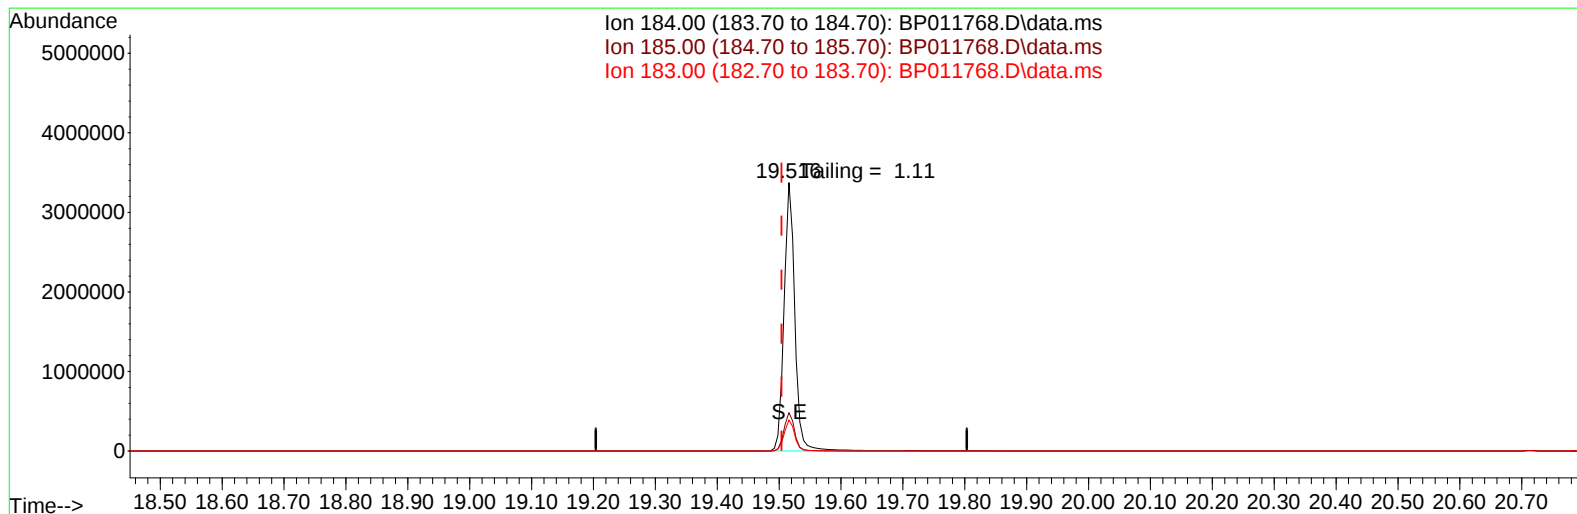

TIC: BP011768.D\data.ms

(77) Benzidine

19.516min (+ 0.012) 8799570.98 ng

response 4098778

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.31
183.00	11.60	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/21/2022	BNA_P	<u>BP011768.D</u>
Compound Name	Response	Retention Time
DDT	1708302	20.716
DDD	7697	20.333
DDE	119	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7816	1716118	0.46

Instrument :
BNA_P
ClientSampleId :
DFTPP