

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
 Data File : BP017260.D
 Acq On : 21 Sep 2023 10:56
 Operator : MA/JU
 Sample : 04387-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Quant Time: Sep 21 22:25:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 14:34:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	180417	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	756600	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	463607	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	1035569	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	980879	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1146466	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	16858	3.838	ng/uL	0.00
4) Pyridine-d5	3.740	84	91882	7.482	ng/u1	0.00
7) Phenol-d5	7.093	99	300513	20.281	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	186983	20.910	ng/u1	0.00
11) 2-Chlorophenol-d4	7.457	132	252872	21.517	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	204227	17.728	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	121727	22.255	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	133955	22.555	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	244467	21.787	ng/u1	0.00
31) 4-Chloroaniline-d4	10.928	131	245330	15.093	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	778538	23.442	ng/u1	0.00
49) Acenaphthylene-d8	14.298	160	863428	22.604	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	115540	19.969	ng/u1	0.00
60) Fluorene-d10	15.598	176	662441	23.169	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	89662	15.362	ng/u1	0.00
73) Anthracene-d10	17.475	188	1051270	22.889	ng/u1	0.00
81) Pyrene-d10	19.716	212	1327156	25.020	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	1312352	23.775	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.787	105	53277	2.993	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
Data File : BP017260.D
Acq On : 21 Sep 2023 10:56
Operator : MA/JU
Sample : 04387-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5


Quant Time: Sep 21 22:25:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 14:34:55 2023
Response via : Initial Calibration

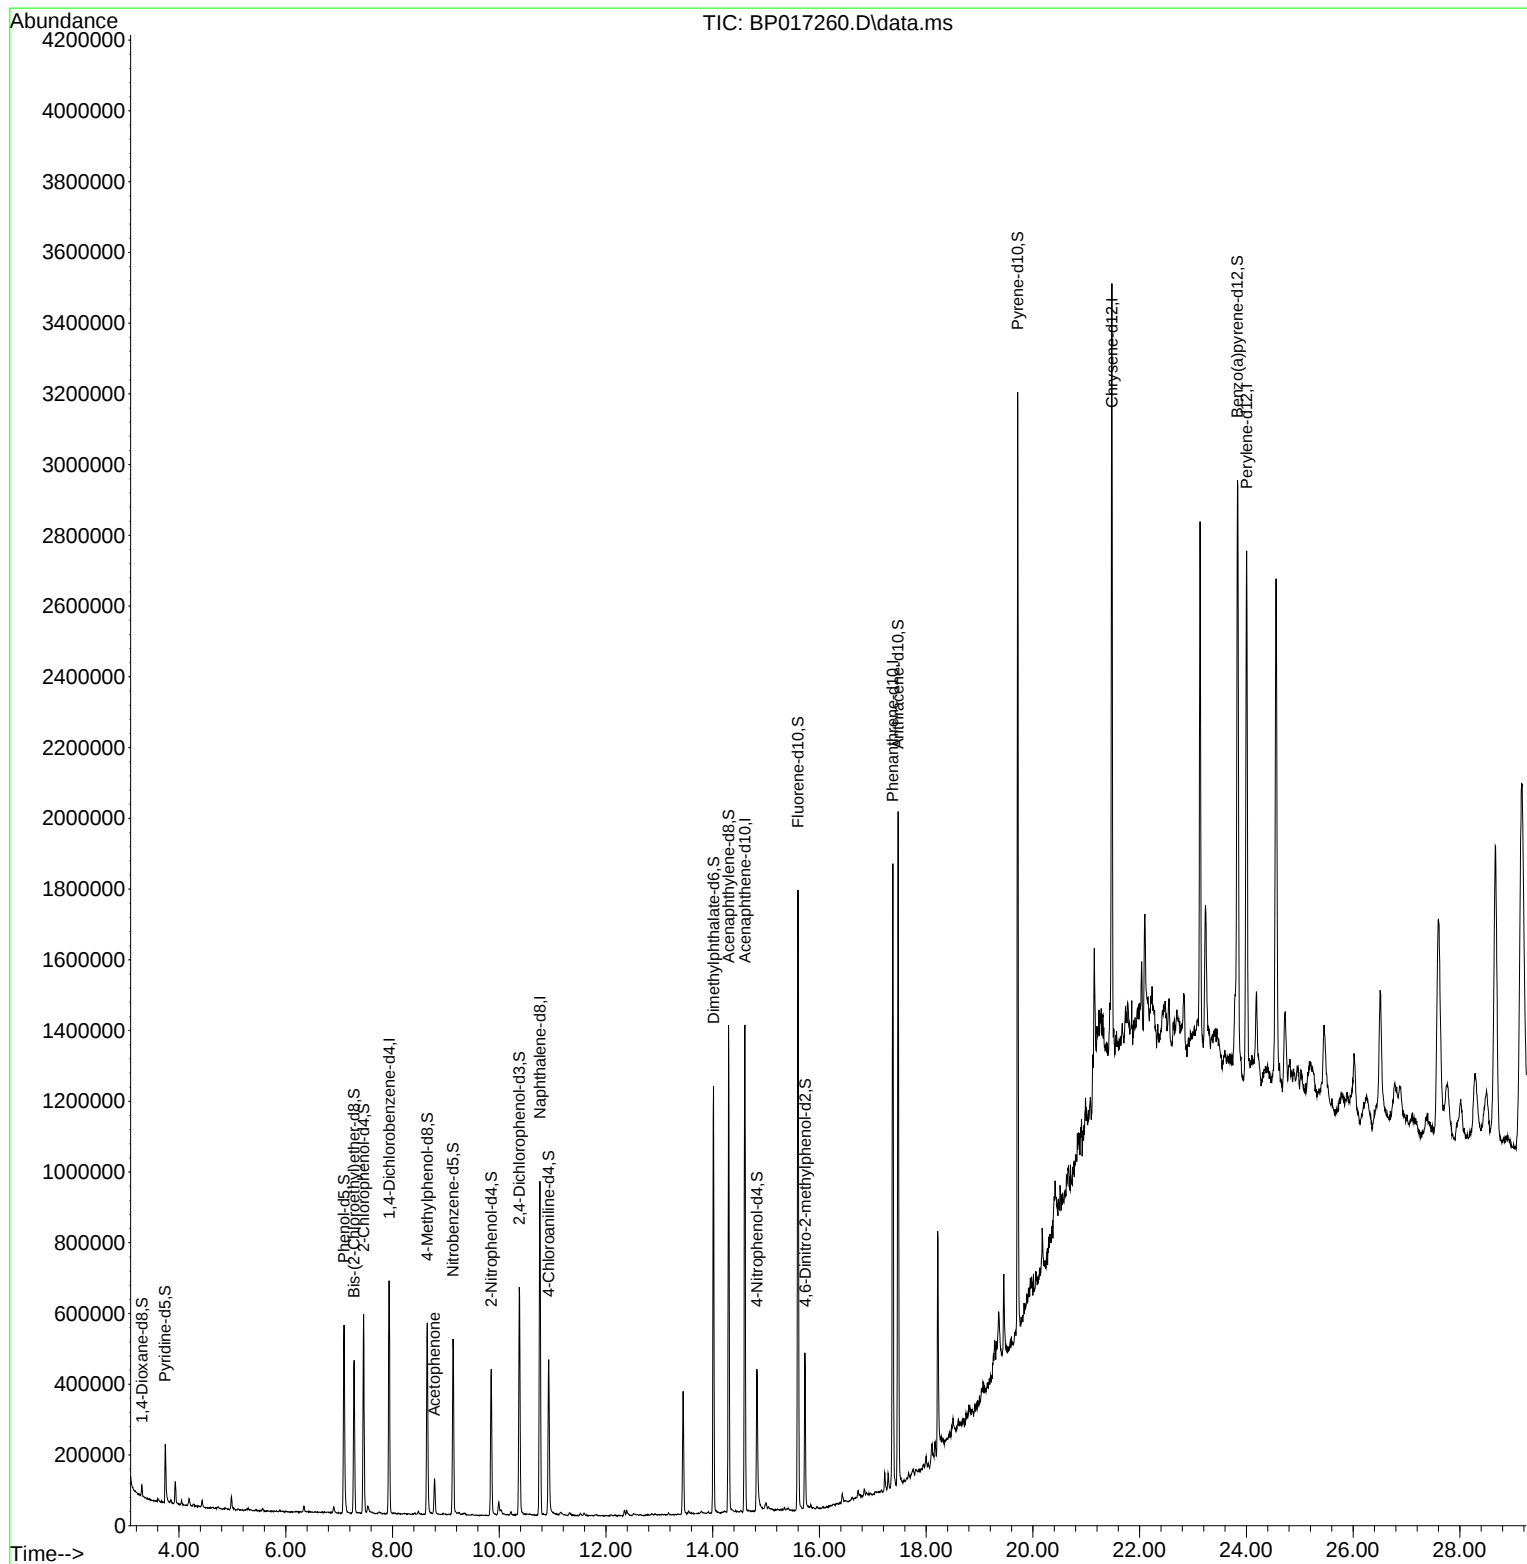

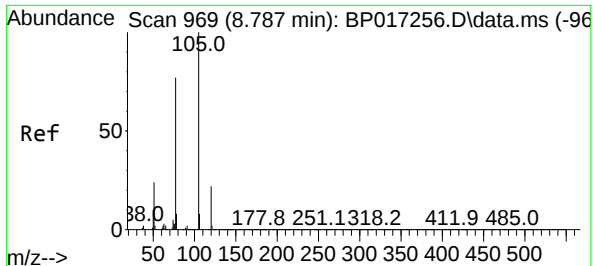

#16
 Acetophenone
 Concen: 2.993 ng/ul
 RT: 8.787 min Scan# 90
 Delta R.T. -0.006 min
 Lab File: BP017260.D
 Acq: 21 Sep 2023 10:56

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

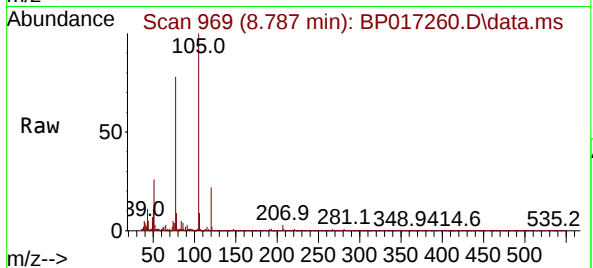

Tgt Ion:	105	Resp:	53277
Ion	Ratio	Lower	Upper
105	100		
77	78.5	63.6	95.4
51	25.6	19.2	28.8

