

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
 Data File : BP017267.D
 Acq On : 21 Sep 2023 14:55
 Operator : MA/JU
 Sample : 04387-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB5

Quant Time: Sep 21 22:27:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 14:34:55 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	168531	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	690710	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	413857	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	915793	20.000	ng/u1	0.00
79) Chrysene-d12	21.475	240	861394	20.000	ng/u1	-0.01
88) Perylene-d12	23.998	264	985493	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	18171	4.429	ng/uL	0.00
4) Pyridine-d5	3.746	84	84036	7.326	ng/u1	0.00
7) Phenol-d5	7.099	99	319944	23.115	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	198524	23.766	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	269660	24.564	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	205477	19.094	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	127509	25.535	ng/u1	0.00
24) 2-Nitrophenol-d4	9.852	143	145065	26.755	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	251307	24.533	ng/u1	0.00
31) 4-Chloroaniline-d4	10.928	131	275179	18.545	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	768954	25.937	ng/u1	0.00
49) Acenaphthylene-d8	14.299	160	865892	25.394	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	99626	19.288	ng/u1	0.00
60) Fluorene-d10	15.598	176	667611	26.157	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	85798	16.622	ng/u1	0.00
73) Anthracene-d10	17.475	188	1009980	24.867	ng/u1	0.00
81) Pyrene-d10	19.716	212	1271746	27.301	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	1242236	26.181	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.793	105	38870	2.337	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
 Data File : BP017267.D
 Acq On : 21 Sep 2023 14:55
 Operator : MA/JU
 Sample : 04387-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB5

Quant Time: Sep 21 22:27:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 14:34:55 2023
 Response via : Initial Calibration

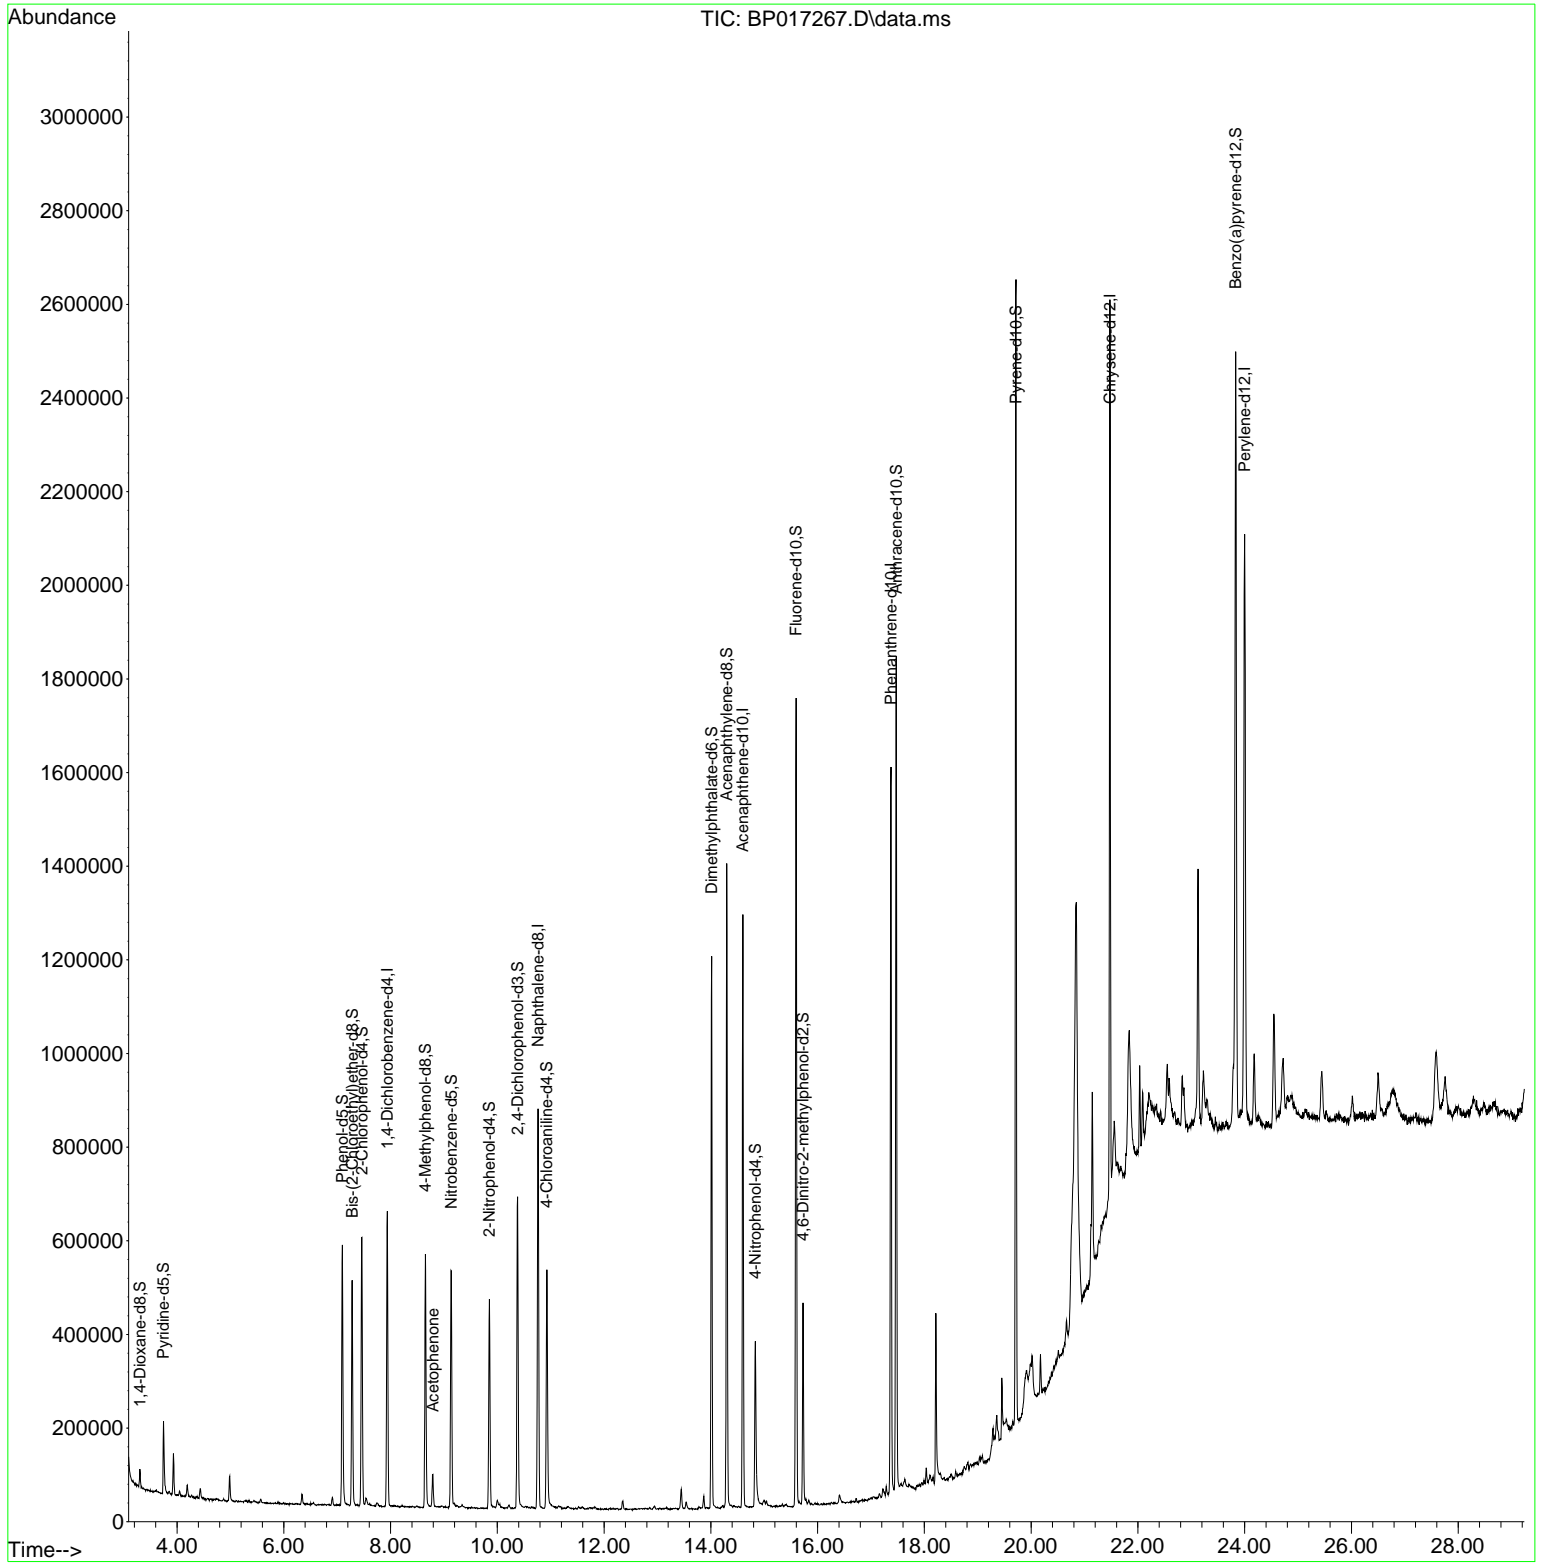

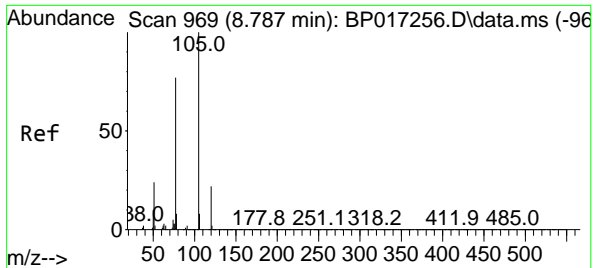

#16
 Acetophenone
 Concen: 2.337 ng/ul
 RT: 8.793 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP017267.D
 Acq: 21 Sep 2023 14:55

Instrument :
 BNA_P
 ClientSampleId :
 C0AB5

Tgt Ion:105 Resp: 38870

Ion	Ratio	Lower	Upper
105	100		
77	75.3	63.6	95.4
51	24.9	19.2	28.8

