

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
 Data File : BP017257.D
 Acq On : 21 Sep 2023 09:11
 Operator : MA/JU
 Sample : PB155652BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	45	rVB	55396	76358	1.70%	0.172%
2	3.740	107	111	129	rBV	628004	929636	20.72%	2.092%
3	4.046	160	163	170	rVB4	9446	14188	0.32%	0.032%
4	7.093	673	681	694	rBV	726296	1130659	25.20%	2.544%
5	7.281	707	713	723	rVB	610152	910715	20.30%	2.049%
6	7.458	736	743	753	rBV	753818	1174495	26.18%	2.643%
7	7.940	818	825	835	rVB	578981	923352	20.58%	2.077%
8	8.322	886	890	893	rBV6	2877	4540	0.10%	0.010%
9	8.652	936	946	957	rBV	848498	1411605	31.46%	3.176%
10	9.134	1021	1028	1039	rBV	650499	1069026	23.83%	2.405%
11	9.440	1077	1080	1084	rVB6	3251	4632	0.10%	0.010%
12	9.852	1141	1150	1156	rBV	555869	914196	20.38%	2.057%
13	10.375	1231	1239	1262	rBV	847550	1455493	32.44%	3.275%
14	10.763	1297	1305	1314	rBV	812138	1336468	29.79%	3.007%
15	10.928	1325	1333	1348	rBV	836116	1493282	33.28%	3.360%
16	12.346	1568	1574	1581	rBV	15146	29223	0.65%	0.066%
17	12.628	1620	1622	1628	rVB7	2951	4498	0.10%	0.010%
18	13.440	1756	1760	1770	rVB7	11646	24469	0.55%	0.055%
19	13.557	1777	1780	1785	rVB6	3671	5918	0.13%	0.013%
20	13.722	1801	1808	1811	rBV9	2444	4775	0.11%	0.011%
21	14.016	1850	1858	1871	rBV	1506125	2146790	47.85%	4.830%
22	14.298	1899	1906	1925	rBV	1781623	2587145	57.66%	5.821%
23	14.598	1950	1957	1966	rBV	1246789	1802442	40.17%	4.055%
24	14.828	1986	1996	2014	rBV	510988	981458	21.88%	2.208%
25	15.598	2118	2127	2142	rBV	2250260	3275785	73.01%	7.370%
26	15.728	2143	2149	2164	rVV	596313	827305	18.44%	1.861%
27	15.834	2164	2167	2172	rVB6	12576	18813	0.42%	0.042%
28	17.034	2367	2371	2378	rBV10	3993	8228	0.18%	0.019%
29	17.369	2422	2428	2439	rBV	1583323	2211429	49.29%	4.976%
30	17.469	2439	2445	2462	rVV	2538904	3672584	81.86%	8.263%
31	17.610	2467	2469	2471	rBV3	4586	4821	0.11%	0.011%
32	18.298	2584	2586	2590	rBV3	4657	5680	0.13%	0.013%
33	19.286	2750	2754	2759	rBV3	37743	49647	1.11%	0.112%
34	19.357	2762	2766	2769	rVV	28113	38321	0.85%	0.086%
35	19.710	2821	2826	2834	rBV	3472607	4418336	98.48%	9.941%
36	21.475	3121	3126	3132	rBV	1911915	2445581	54.51%	5.502%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
Data File : BP017257.D
Acq On : 21 Sep 2023 09:11
Operator : MA/JU
Sample : PB155652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	23.827	3520	3526	3536	rVB2	2206979	4486579	100.00%	10.094%
38	23.992	3548	3554	3562	rVB	1220688	2547786	56.79%	5.732%




Sum of corrected areas: 44446258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
Data File : BP017257.D
Acq On : 21 Sep 2023 09:11
Operator : MA/JU
Sample : PB155652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

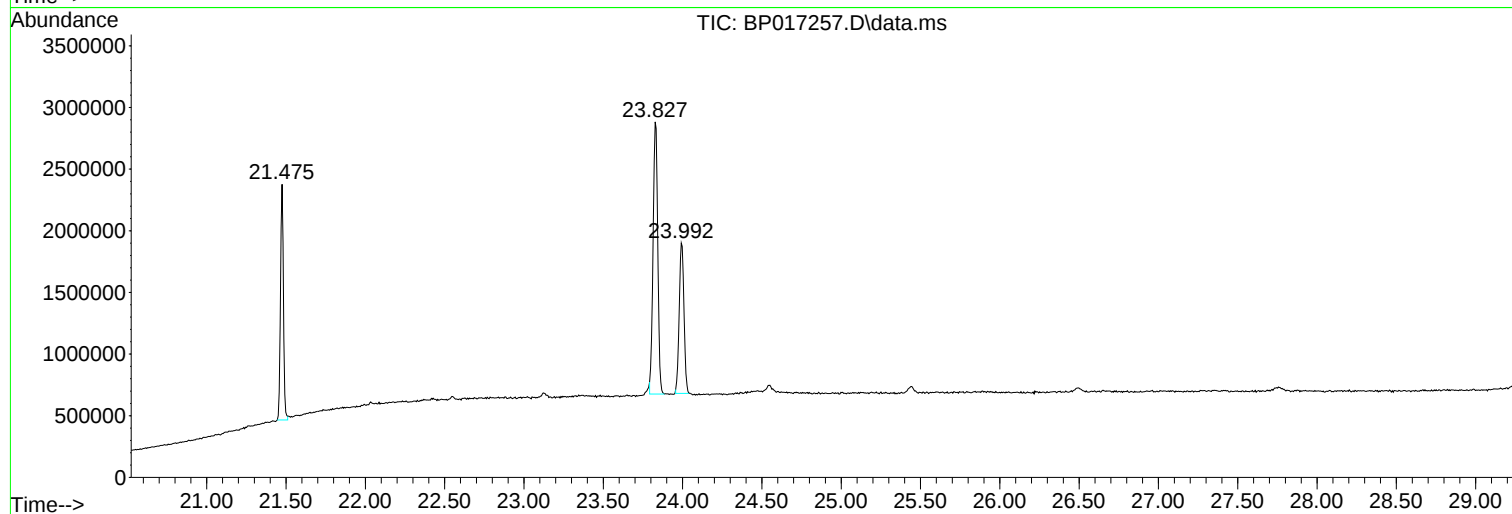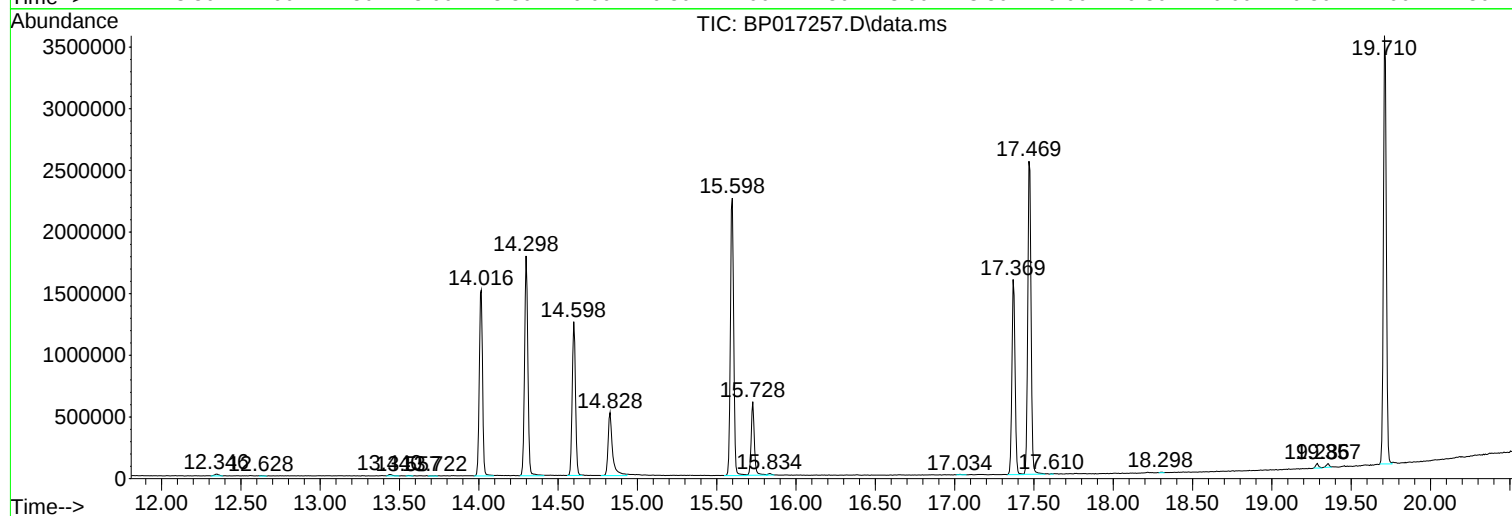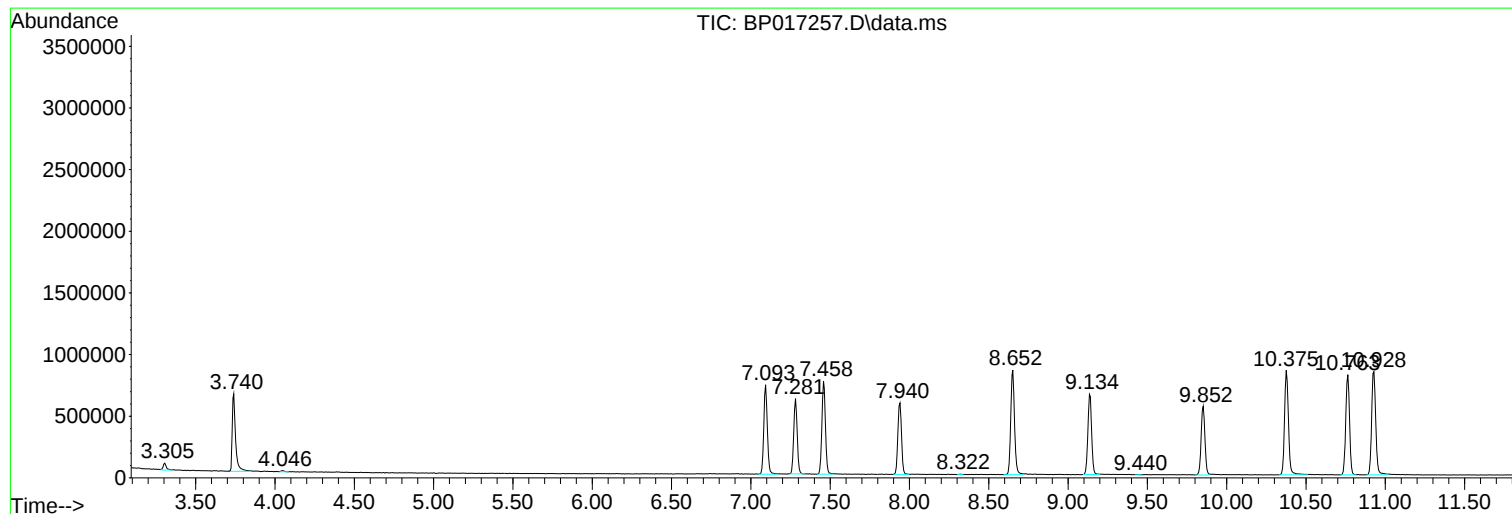

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
Data File : BP017257.D
Acq On : 21 Sep 2023 09:11
Operator : MA/JU
Sample : PB155652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092123\
Data File : BP017257.D
Acq On : 21 Sep 2023 09:11
Operator : MA/JU
Sample : PB155652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc