

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017285.D
 Acq On : 22 Sep 2023 14:03
 Operator : MA/JU
 Sample : 04410-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBK3

Quant Time: Sep 22 16:27:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 23:51:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	153312	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	598703	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	345300	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.369	188	784287	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	781928	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	890089	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	17129	4.589	ng/uL	0.00
4) Pyridine-d5	3.740	84	118790	11.384	ng/u1	0.00
7) Phenol-d5	7.093	99	107009	8.499	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	267248	35.169	ng/u1	0.00
11) 2-Chlorophenol-d4	7.457	132	292880	29.327	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	187923	19.197	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	166133	38.383	ng/u1	0.00
24) 2-Nitrophenol-d4	9.846	143	178766	38.038	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	310742	34.997	ng/u1	0.00
31) 4-Chloroaniline-d4	10.922	131	311184	24.194	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	1060657	42.879	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1157585	40.689	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	33413	7.753	ng/u1	0.00
60) Fluorene-d10	15.592	176	918781	43.144	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	129561	29.310	ng/u1	0.00
73) Anthracene-d10	17.469	188	1580071	45.426	ng/u1	0.00
81) Pyrene-d10	19.710	212	1954125	46.214	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	1978078	46.157	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.340	88	4023	1.052	ng/uL#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017285.D
Acq On : 22 Sep 2023 14:03
Operator : MA/JU
Sample : 04410-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBK3

Quant Time: Sep 22 16:27:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 21 23:51:07 2023
Response via : Initial Calibration

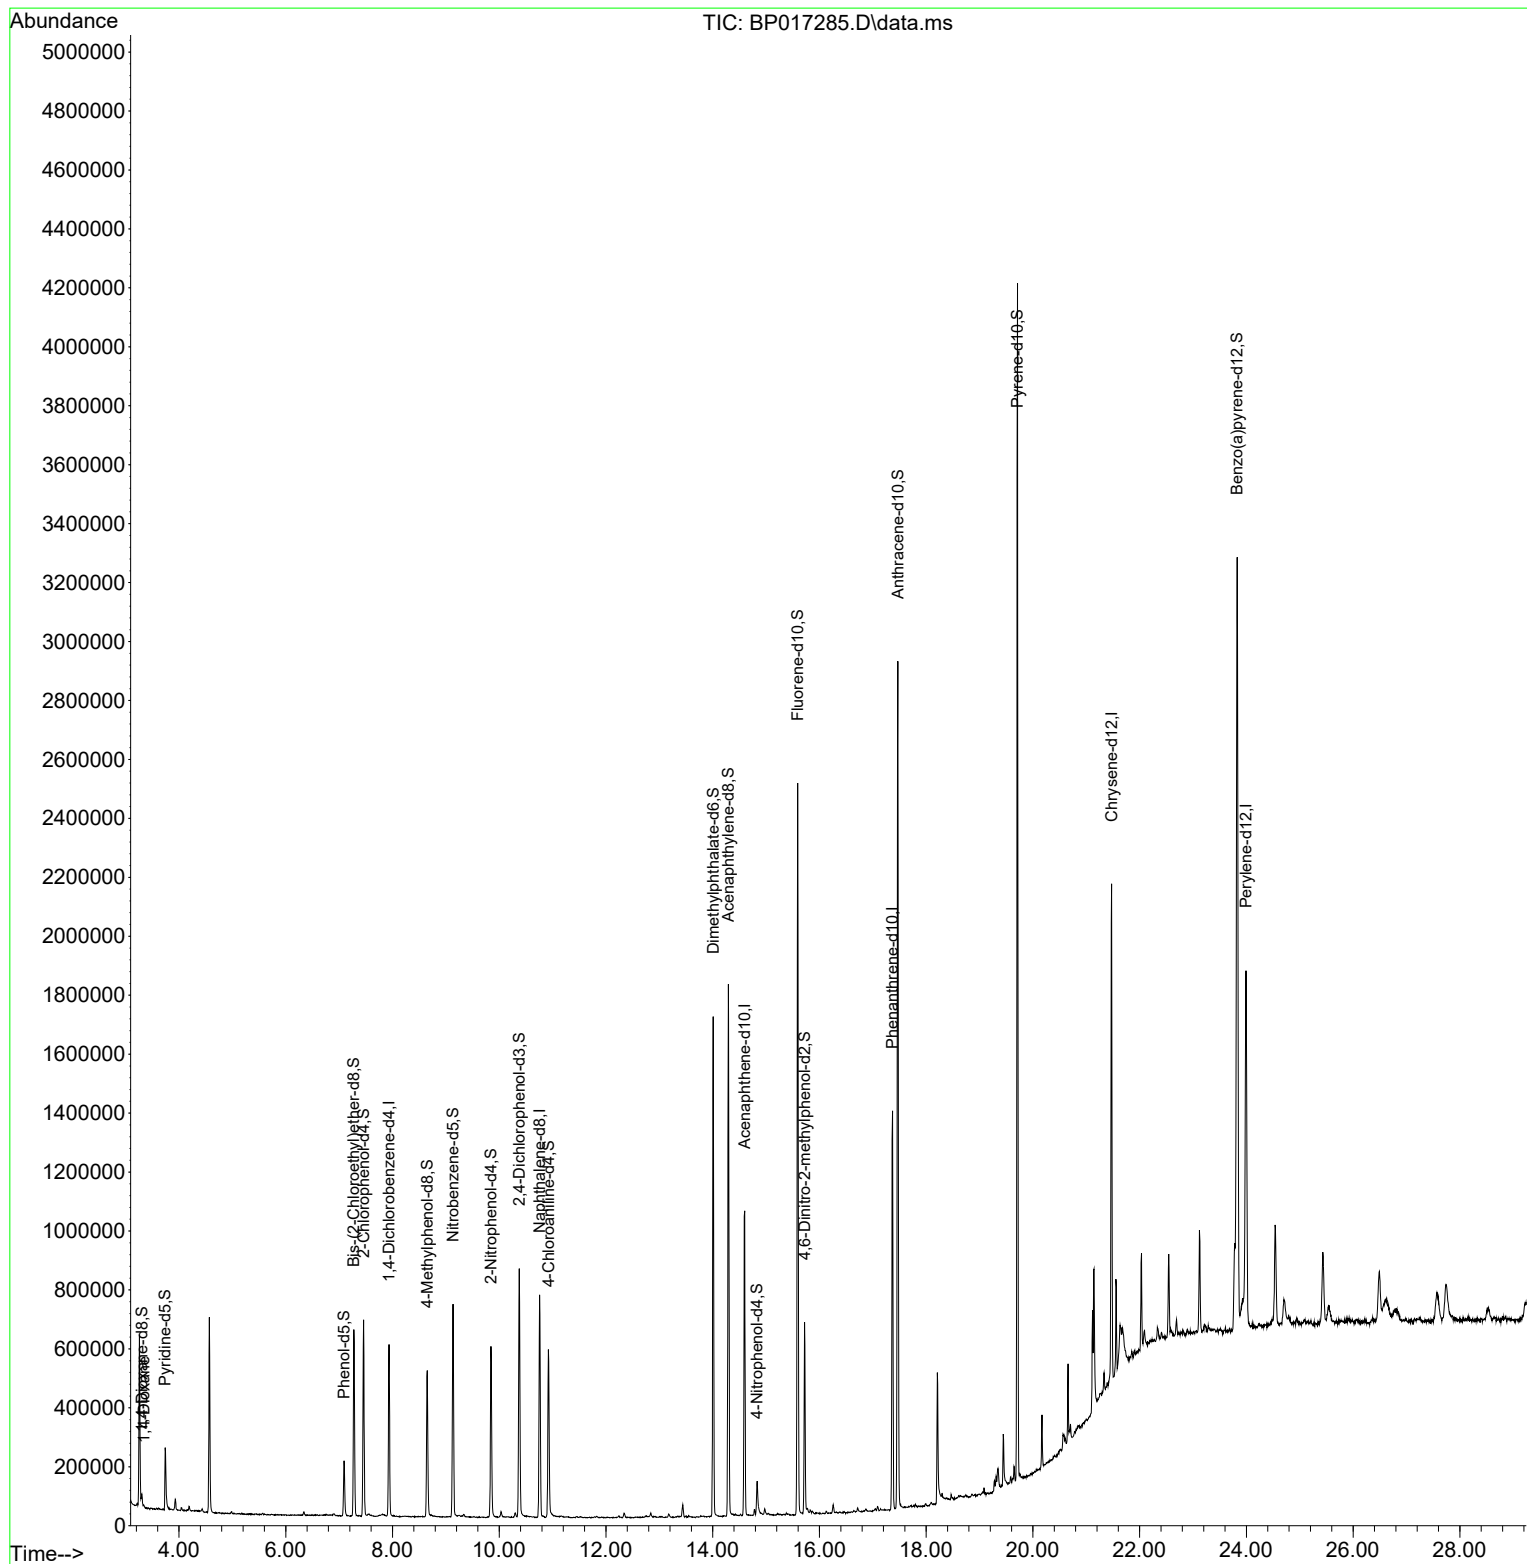

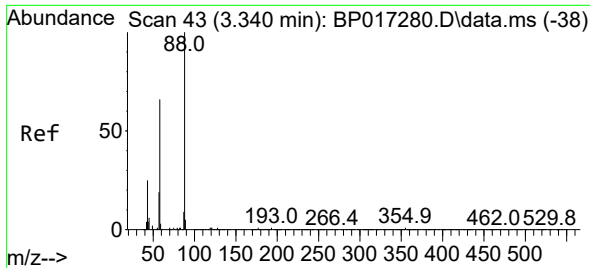

#2
1,4-Dioxane
Concen: 1.052 ng/uL
RT: 3.340 min Scan# 41
Delta R.T. 0.000 min
Lab File: BP017285.D
Acq: 22 Sep 2023 14:03

Instrument :
BNA_P
ClientSampleId :
BBBK3

Tgt Ion: 88 Resp: 4023
Ion Ratio Lower Upper
88 100
43 46.7 25.0 37.4#
58 67.2 56.6 84.8

