

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017301.D
 Acq On : 22 Sep 2023 23:26
 Operator : MA/JU
 Sample : 04410-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ0

Quant Time: Sep 23 02:07:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 23:51:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	140357	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	567363	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	337264	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.363	188	777142	20.000	ng/u1	0.00
79) Chrysene-d12	21.469	240	735626	20.000	ng/u1	0.00
88) Perylene-d12	23.980	264	813412	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	20718	6.063	ng/uL	0.00
4) Pyridine-d5	3.740	84	153334	16.051	ng/u1	0.00
7) Phenol-d5	7.087	99	114992	9.975	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.275	67	307379	44.184	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	329961	36.090	ng/u1	-0.01
15) 4-Methylphenol-d8	8.646	113	204250	22.790	ng/u1	-0.01
21) Nitrobenzene-d5	9.128	128	194400	47.395	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.846	143	206098	46.276	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	350865	41.699	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.922	131	367854	30.180	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	1174355	48.606	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1296441	46.655	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	30566	7.262	ng/u1	0.00
60) Fluorene-d10	15.592	176	1020130	49.045	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.722	200	154207	35.206	ng/u1	0.00
73) Anthracene-d10	17.463	188	1757373	50.987	ng/u1	0.00
81) Pyrene-d10	19.704	212	2101729	52.833	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.816	264	2057436	52.535	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	15908	4.546	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017301.D
Acq On : 22 Sep 2023 23:26
Operator : MA/JU
Sample : 04410-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ0

Quant Time: Sep 23 02:07:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 21 23:51:07 2023
Response via : Initial Calibration

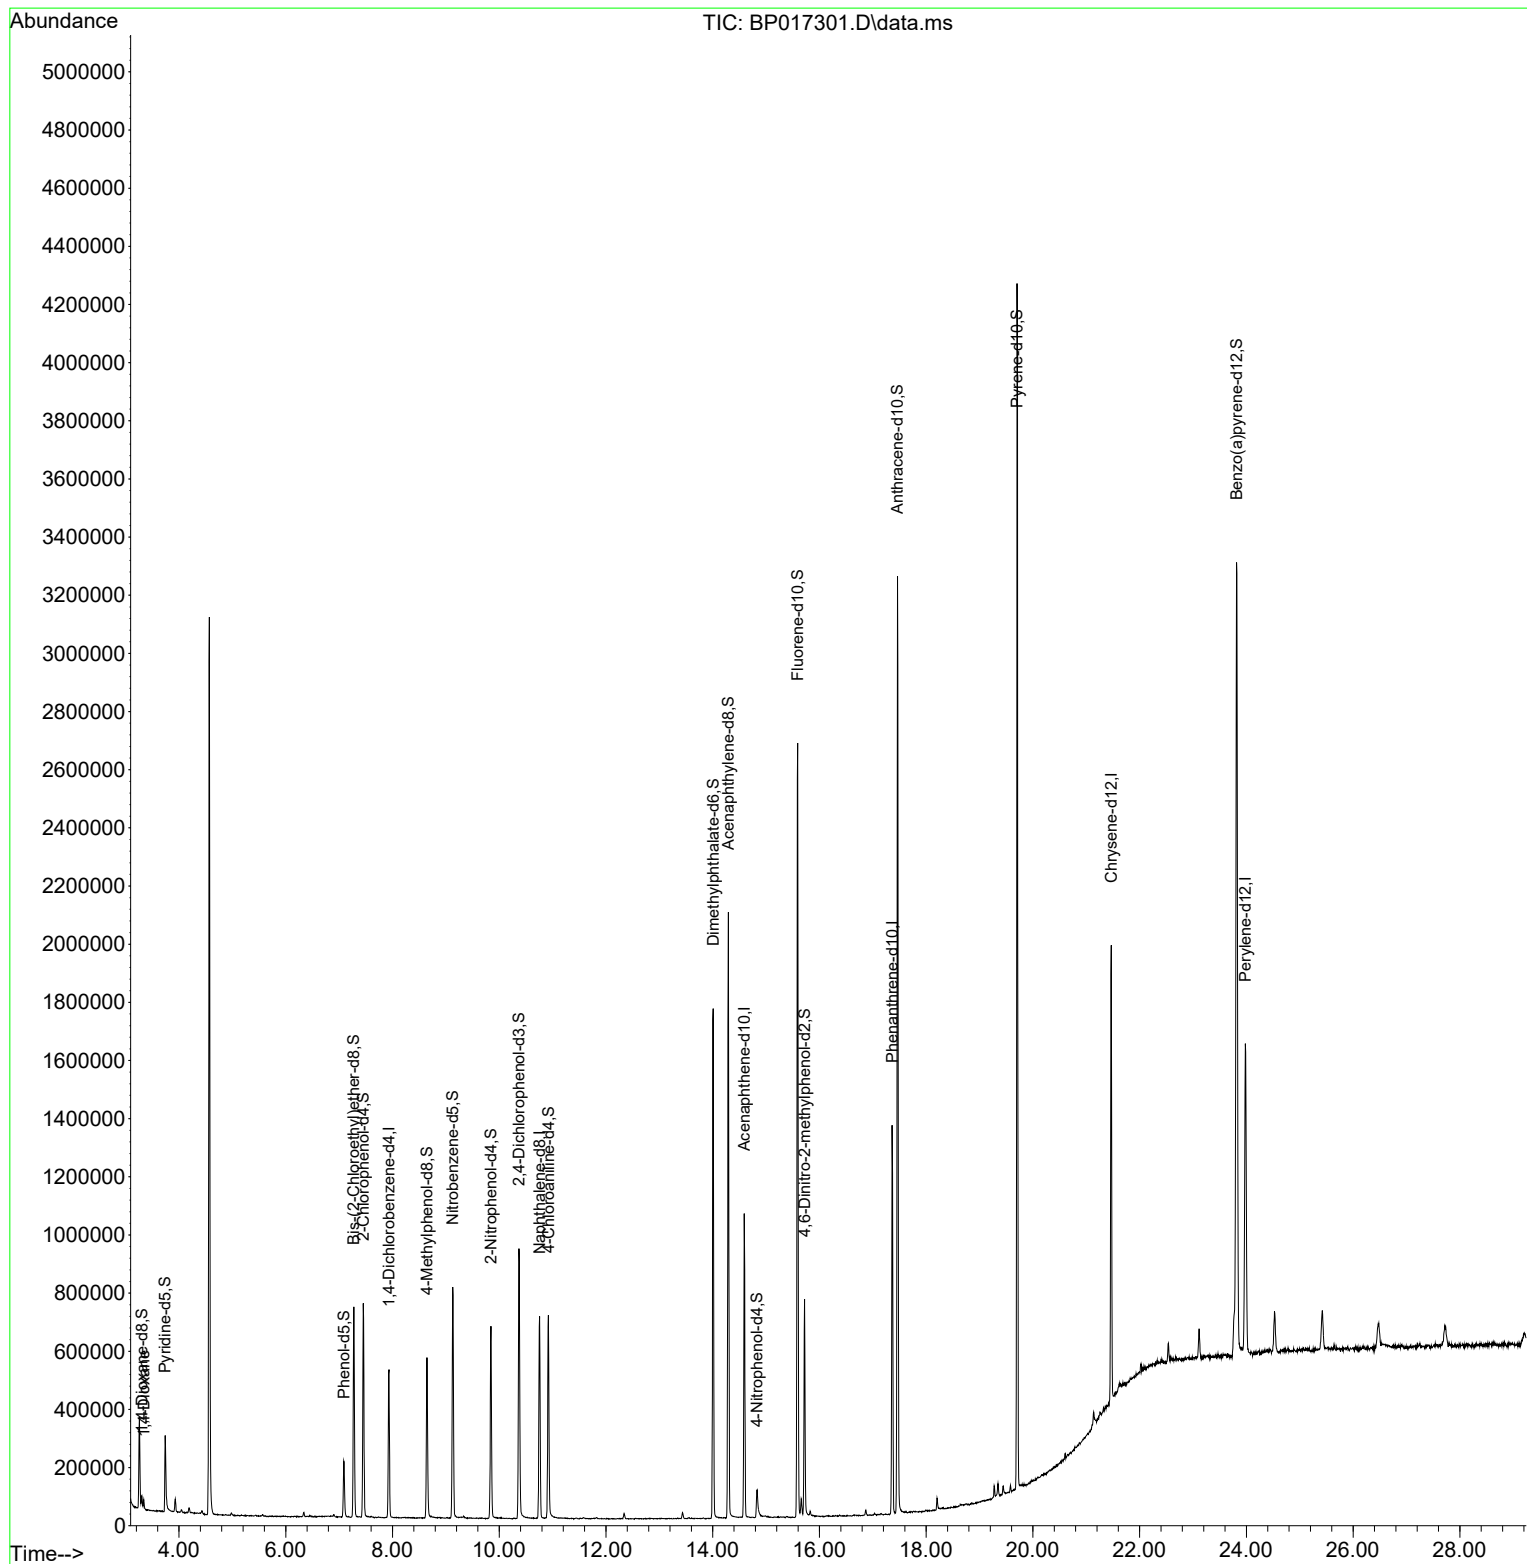

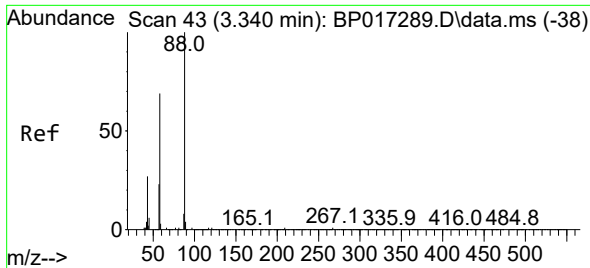

#2
 1,4-Dioxane
 Concen: 4.546 ng/uL
 RT: 3.340 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP017301.D
 Acq: 22 Sep 2023 23:26

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ0

Tgt Ion: 88 Resp: 15908
 Ion Ratio Lower Upper
 88 100
 43 26.6 25.0 37.4
 58 64.1 56.6 84.8

