

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017282.D
 Acq On : 22 Sep 2023 10:04
 Operator : MA/JU
 Sample : PB155610BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	42	rBV	60943	71383	1.45%	0.159%
2	3.740	107	111	128	rBV	728958	1066469	21.73%	2.375%
3	4.046	160	163	168	rVB2	10815	14560	0.30%	0.032%
4	7.093	674	681	695	rBV	833248	1286683	26.22%	2.865%
5	7.275	706	712	723	rVB	650257	1014506	20.67%	2.259%
6	7.458	736	743	752	rBV	850649	1322879	26.95%	2.946%
7	7.934	817	824	833	rBV	581175	887870	18.09%	1.977%
8	8.652	939	946	960	rBV	949264	1558562	31.76%	3.471%
9	9.134	1019	1028	1040	rBV	732833	1176546	23.97%	2.620%
10	9.846	1142	1149	1159	rBV	599164	985843	20.09%	2.195%
11	10.375	1231	1239	1252	rBV	951113	1566739	31.92%	3.489%
12	10.757	1294	1304	1314	rBV	756314	1230739	25.08%	2.741%
13	10.922	1324	1332	1350	rBV	908782	1572534	32.04%	3.502%
14	12.346	1568	1574	1581	rBV4	16188	30166	0.61%	0.067%
15	13.440	1755	1760	1763	rBV6	10410	15951	0.32%	0.036%
16	13.557	1778	1780	1786	rVB7	4062	5640	0.11%	0.013%
17	14.010	1850	1857	1869	rBV	1591307	2093751	42.66%	4.662%
18	14.298	1897	1906	1919	rBV	1730993	2551982	52.00%	5.683%
19	14.598	1950	1957	1964	rBV	1070257	1528918	31.15%	3.405%
20	14.828	1989	1996	2015	rBV	555522	1021096	20.80%	2.274%
21	15.592	2119	2126	2137	rBV	2306013	3227947	65.77%	7.188%
22	15.722	2142	2148	2161	rVV	554254	773303	15.76%	1.722%
23	15.828	2162	2166	2171	rVB4	11033	15156	0.31%	0.034%
24	16.375	2255	2259	2264	rBV8	2997	5036	0.10%	0.011%
25	17.039	2367	2372	2374	rBV6	4257	5048	0.10%	0.011%
26	17.369	2418	2428	2438	rBV	1351944	1918042	39.08%	4.271%
27	17.469	2438	2445	2464	rVV	2735898	3758191	76.57%	8.369%
28	19.281	2749	2753	2758	rBV2	37387	47001	0.96%	0.105%
29	19.351	2761	2765	2768	rVB3	29959	38695	0.79%	0.086%
30	19.710	2820	2826	2832	rBV	3689320	4650733	94.76%	10.356%
31	21.469	3121	3125	3134	rBV	1678441	2180488	44.43%	4.856%
32	23.821	3519	3525	3538	rVB2	2447597	4908040	100.00%	10.929%
33	23.992	3548	3554	3565	rVB	1154263	2376079	48.41%	5.291%




Sum of corrected areas: 44906576

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017282.D
Acq On : 22 Sep 2023 10:04
Operator : MA/JU
Sample : PB155610BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

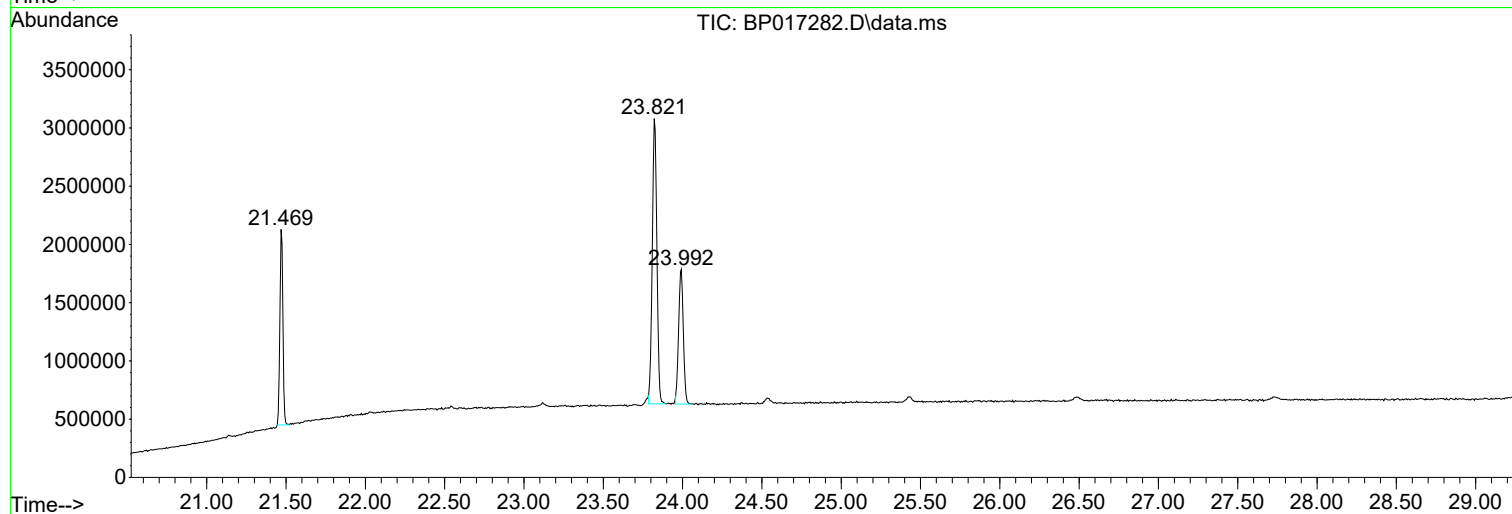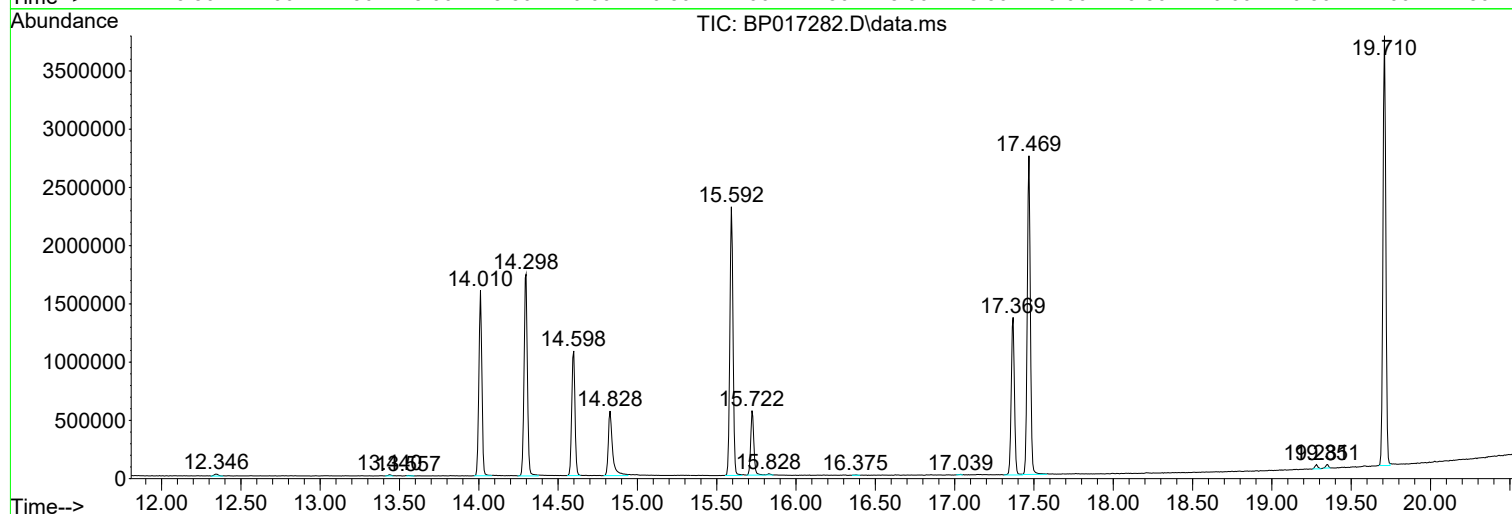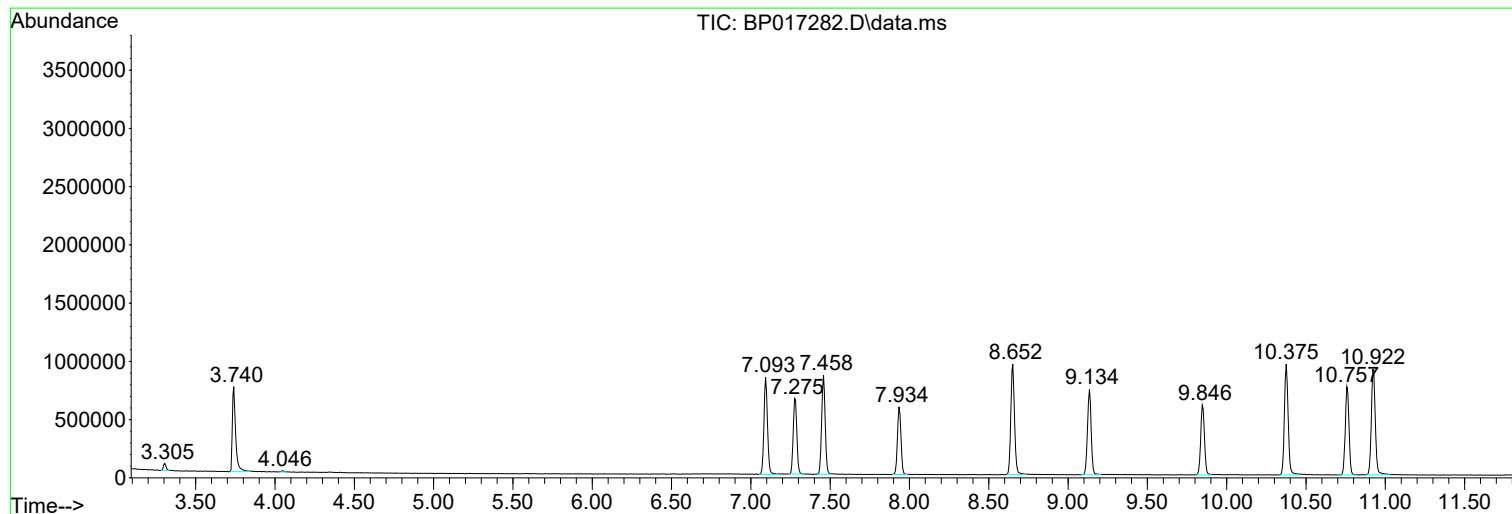

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017282.D
Acq On : 22 Sep 2023 10:04
Operator : MA/JU
Sample : PB155610BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017282.D
Acq On : 22 Sep 2023 10:04
Operator : MA/JU
Sample : PB155610BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc