

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017290.D
 Acq On : 22 Sep 2023 17:09
 Operator : MA/JU
 Sample : PB155616BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK616

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	46	rVB	58153	79569	1.64%	0.180%
2	3.734	107	110	126	rBV	663165	1022739	21.07%	2.310%
3	4.046	160	163	169	rVB5	9859	16042	0.33%	0.036%
4	7.093	674	681	693	rBV	796652	1262018	26.00%	2.850%
5	7.275	706	712	722	rVB	653611	994961	20.49%	2.247%
6	7.458	736	743	751	rBV	829420	1296113	26.70%	2.927%
7	7.934	817	824	834	rBV	499863	771439	15.89%	1.742%
8	8.646	936	945	956	rBV	956479	1550965	31.95%	3.503%
9	9.134	1021	1028	1040	rBV	708876	1161782	23.93%	2.624%
10	9.846	1140	1149	1158	rBV	601180	972212	20.03%	2.196%
11	10.375	1231	1239	1252	rBV	904060	1563356	32.20%	3.531%
12	10.757	1296	1304	1314	rBV	659407	1081165	22.27%	2.442%
13	10.922	1323	1332	1348	rBV	943789	1587909	32.71%	3.586%
14	12.340	1570	1573	1580	rVB	15915	24278	0.50%	0.055%
15	13.440	1752	1760	1767	rBV2	13546	25528	0.53%	0.058%
16	13.551	1776	1779	1787	rVB9	4578	8303	0.17%	0.019%
17	14.010	1850	1857	1868	rBV	1584908	2170129	44.70%	4.901%
18	14.293	1896	1905	1919	rBV	1815632	2657405	54.74%	6.002%
19	14.593	1948	1956	1967	rBV	955373	1395916	28.75%	3.153%
20	14.828	1989	1996	2015	rBV	531243	1038402	21.39%	2.345%
21	15.593	2119	2126	2137	rBV	2455717	3366709	69.35%	7.603%
22	15.722	2142	2148	2160	rVV	565354	767715	15.81%	1.734%
23	15.828	2163	2166	2171	rVB6	12843	19782	0.41%	0.045%
24	17.028	2367	2370	2375	rBV7	4787	6497	0.13%	0.015%
25	17.157	2386	2392	2394	rBV6	4688	7598	0.16%	0.017%
26	17.363	2421	2427	2434	rBV	1206753	1753092	36.11%	3.959%
27	17.469	2438	2445	2459	rVV	2848693	3929475	80.94%	8.874%
28	19.281	2749	2753	2758	rBV2	38702	47454	0.98%	0.107%
29	19.351	2761	2765	2769	rVB2	30028	42768	0.88%	0.097%
30	19.710	2820	2826	2833	rBV	3739209	4814091	99.16%	10.872%
31	21.469	3121	3125	3131	rBV	1464056	1948821	40.14%	4.401%
32	23.827	3519	3526	3536	rVB	2402219	4854689	100.00%	10.964%
33	23.992	3548	3554	3562	rVB	984480	2039959	42.02%	4.607%




Sum of corrected areas: 44278881

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017290.D
Acq On : 22 Sep 2023 17:09
Operator : MA/JU
Sample : PB155616BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

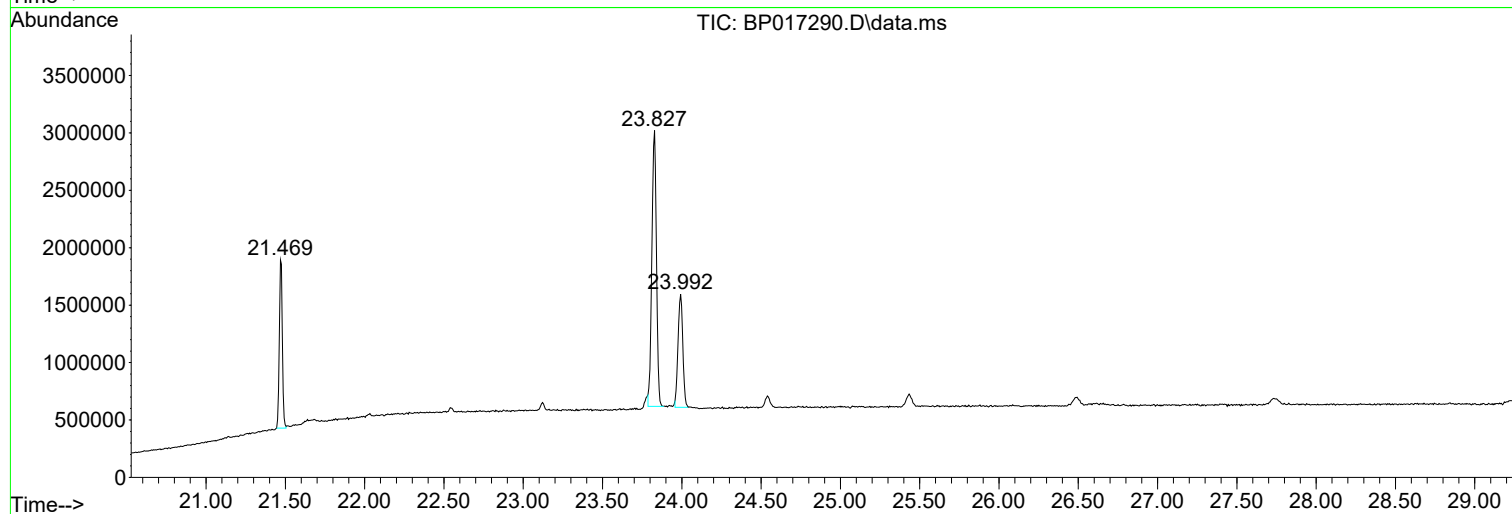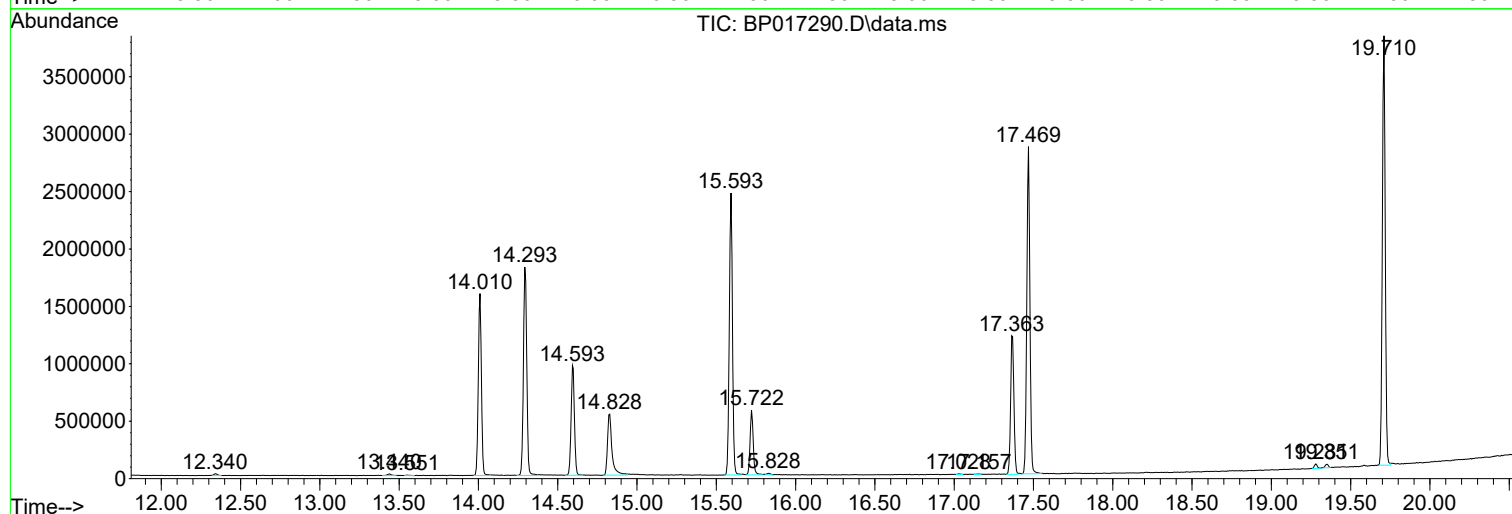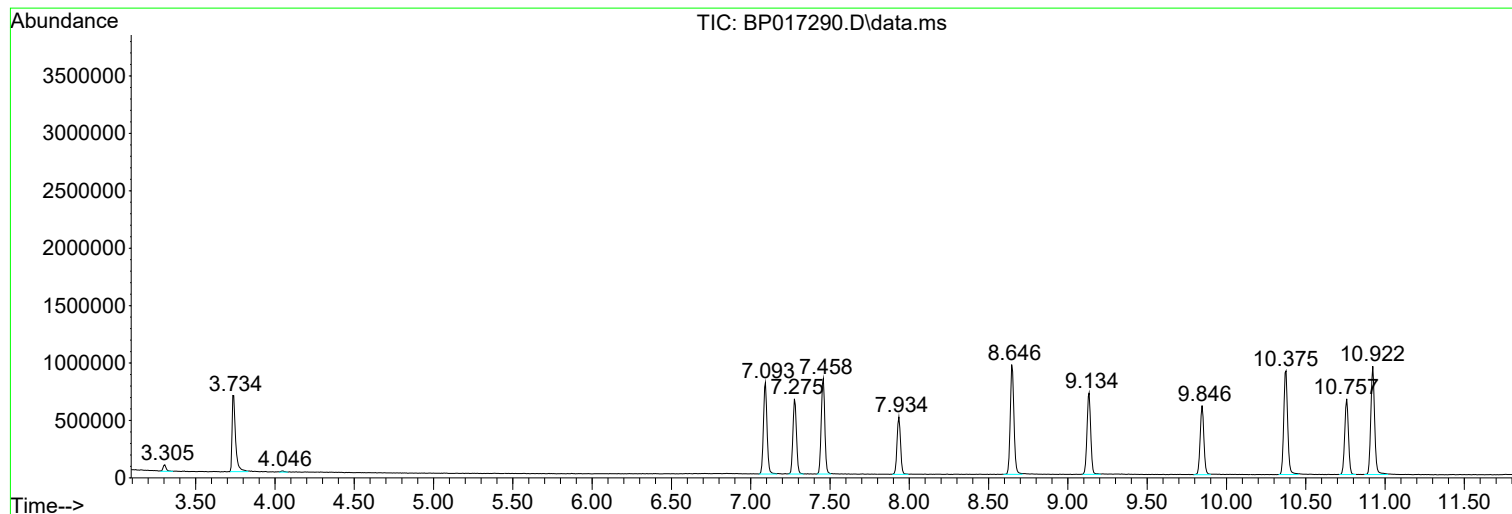

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017290.D
Acq On : 22 Sep 2023 17:09
Operator : MA/JU
Sample : PB155616BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017290.D
Acq On : 22 Sep 2023 17:09
Operator : MA/JU
Sample : PB155616BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------