

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017291.D
 Acq On : 22 Sep 2023 17:43
 Operator : MA/JU
 Sample : PB155619BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	43	rVB	57554	67925	1.34%	0.148%
2	3.734	107	110	123	rBV	699723	1065688	20.96%	2.315%
3	4.046	160	163	168	rVB3	9527	12879	0.25%	0.028%
4	7.093	673	681	692	rBV	818323	1322554	26.01%	2.873%
5	7.275	706	712	721	rVB	681760	1028863	20.24%	2.235%
6	7.458	735	743	756	rBV	861410	1362224	26.79%	2.959%
7	7.934	817	824	831	rBV	527203	811314	15.96%	1.762%
8	8.646	938	945	956	rBV	993949	1602860	31.53%	3.482%
9	8.887	982	986	992	rBV9	2705	5503	0.11%	0.012%
10	9.134	1020	1028	1041	rBV	738449	1201797	23.64%	2.610%
11	9.846	1140	1149	1159	rBV	629492	1009428	19.85%	2.193%
12	10.375	1230	1239	1254	rBV	946016	1635206	32.16%	3.552%
13	10.758	1295	1304	1315	rBV	700381	1157038	22.76%	2.513%
14	10.922	1325	1332	1348	rBV	971228	1650056	32.46%	3.584%
15	12.340	1568	1573	1580	rVB	16532	27066	0.53%	0.059%
16	13.375	1746	1749	1754	rBV7	3247	5382	0.11%	0.012%
17	13.440	1754	1760	1766	rVV5	13396	24093	0.47%	0.052%
18	13.557	1776	1780	1783	rVB6	5854	6840	0.13%	0.015%
19	14.010	1850	1857	1867	rBV	1629810	2215745	43.58%	4.813%
20	14.293	1897	1905	1922	rBV	1880466	2717652	53.45%	5.903%
21	14.593	1949	1956	1966	rBV	1031722	1467076	28.86%	3.187%
22	14.828	1988	1996	2016	rBV	545111	1080109	21.24%	2.346%
23	15.393	2087	2092	2095	rBV7	3769	7389	0.15%	0.016%
24	15.593	2118	2126	2137	rBV	2478092	3448101	67.82%	7.490%
25	15.722	2142	2148	2162	rVV	588983	794366	15.62%	1.725%
26	15.828	2162	2166	2171	rVB4	12976	20162	0.40%	0.044%
27	16.375	2257	2259	2267	rVB9	4642	6184	0.12%	0.013%
28	17.363	2421	2427	2438	rBV	1267207	1836108	36.11%	3.988%
29	17.469	2438	2445	2458	rBV	2757397	4019026	79.05%	8.730%
30	19.281	2749	2753	2757	rBV2	41823	53532	1.05%	0.116%
31	19.351	2761	2765	2769	rVB	32787	43216	0.85%	0.094%
32	19.710	2820	2826	2833	rBV	3908400	4998200	98.31%	10.857%
33	21.469	3121	3125	3132	rBV	1612964	2027071	39.87%	4.403%
34	23.827	3519	3526	3537	rVB2	2477852	5084065	100.00%	11.043%
35	23.992	3547	3554	3565	rVB	1048009	2224033	43.75%	4.831%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017291.D
Acq On : 22 Sep 2023 17:43
Operator : MA/JU
Sample : PB155619BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK619

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46038751

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017291.D
Acq On : 22 Sep 2023 17:43
Operator : MA/JU
Sample : PB155619BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

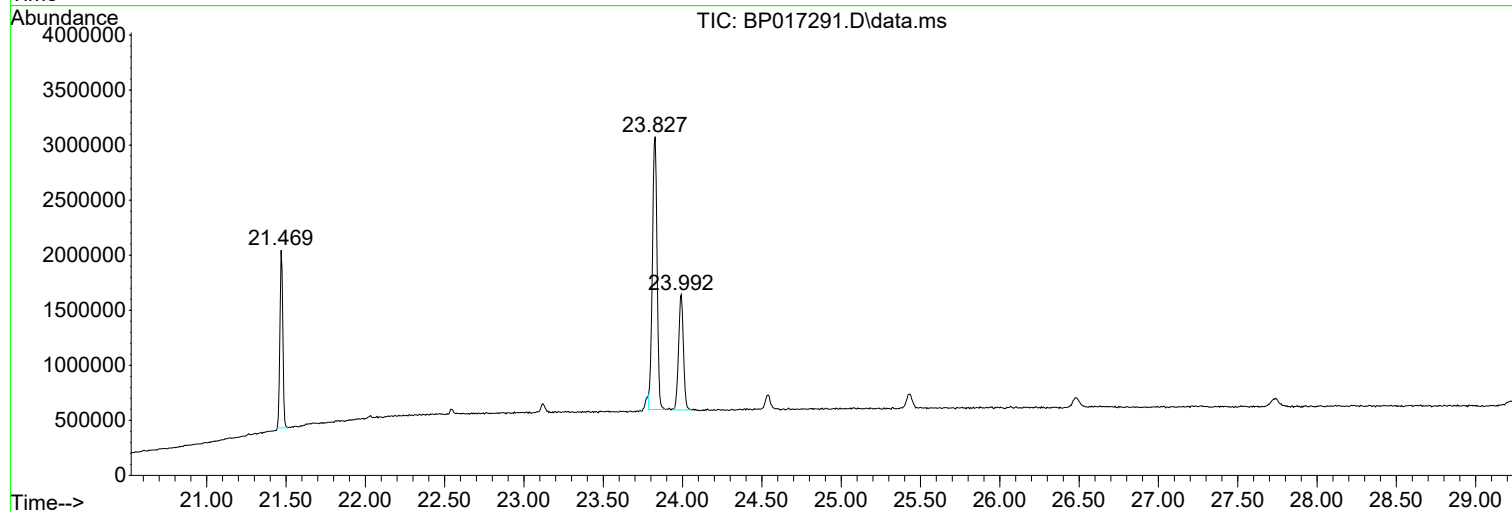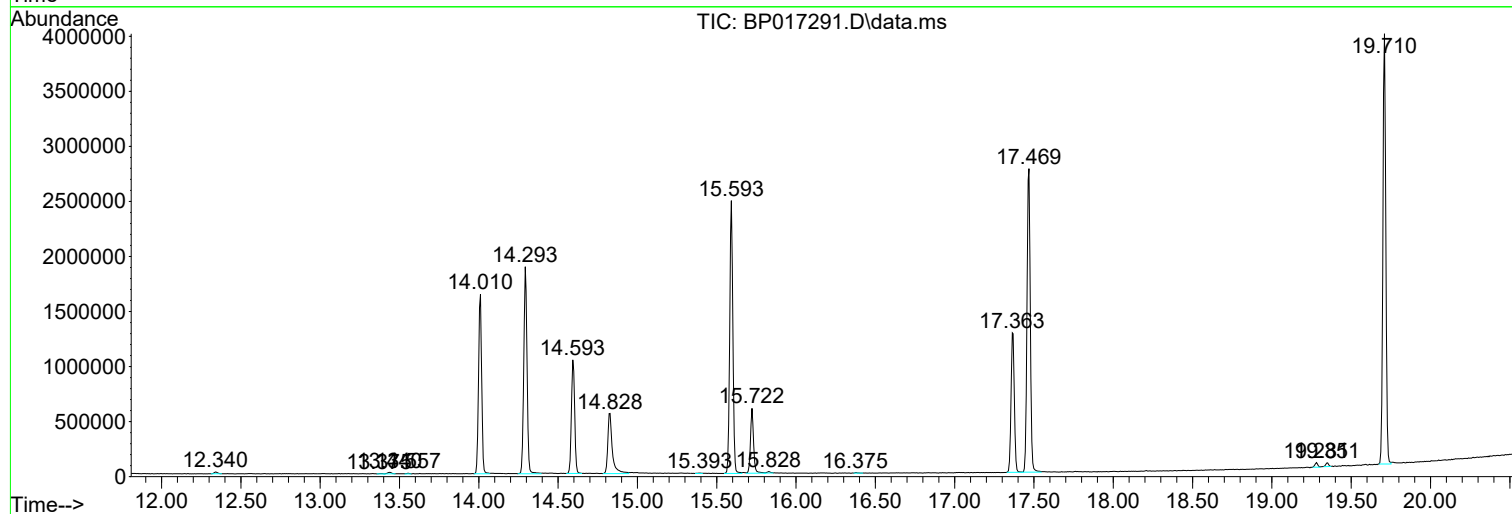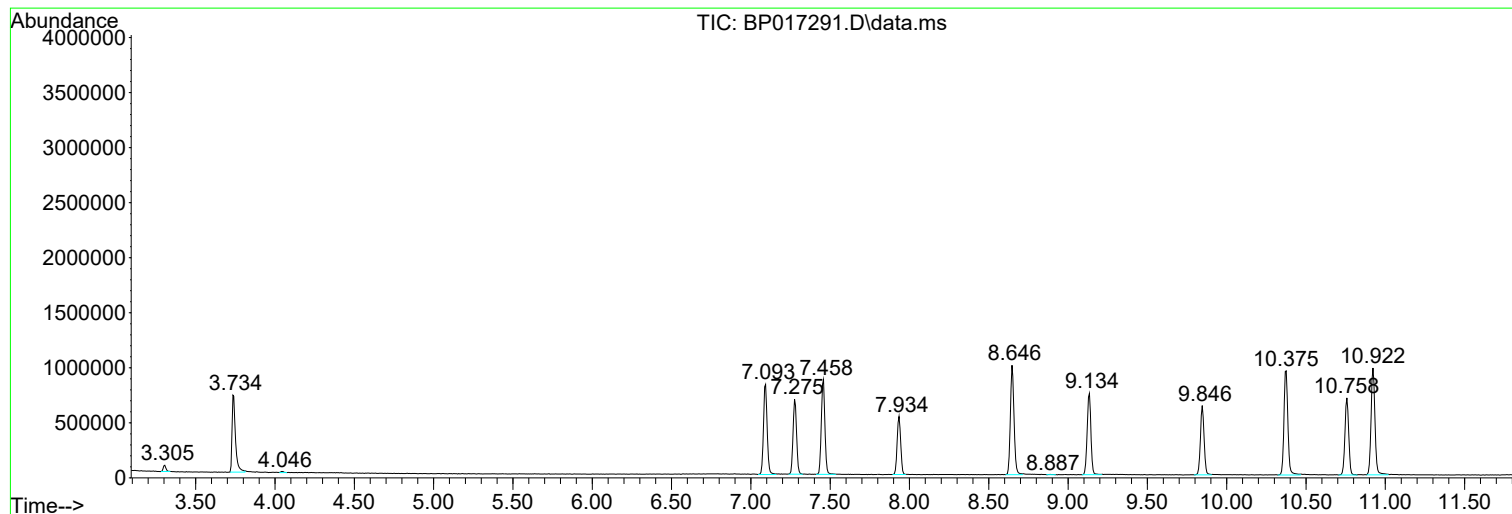

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017291.D
Acq On : 22 Sep 2023 17:43
Operator : MA/JU
Sample : PB155619BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017291.D
Acq On : 22 Sep 2023 17:43
Operator : MA/JU
Sample : PB155619BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK619

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc