

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017300.D
 Acq On : 22 Sep 2023 22:51
 Operator : MA/JU
 Sample : 04410-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	24	29	34	rBV	139379	186011	2.33%	0.348%
2	3.305	34	37	43	rVB	36565	48511	0.61%	0.091%
3	3.740	108	111	124	rBV	202879	322687	4.03%	0.604%
4	3.928	139	143	148	rVB	37492	51651	0.65%	0.097%
5	4.046	160	163	166	rVB3	8876	10970	0.14%	0.021%
6	4.187	184	187	192	rVB2	14987	20607	0.26%	0.039%
7	4.428	226	228	233	rVB3	11018	12948	0.16%	0.024%
8	4.569	245	252	267	rBV	5382705	7997527	100.00%	14.981%
9	4.987	320	323	327	rVB2	6914	8248	0.10%	0.015%
10	6.334	547	552	558	rBV3	11711	20658	0.26%	0.039%
11	6.452	570	572	579	rVB6	9392	14289	0.18%	0.027%
12	6.899	645	648	654	rVB5	6440	11063	0.14%	0.021%
13	7.093	675	681	692	rVB	147628	246627	3.08%	0.462%
14	7.275	706	712	721	rBV	635867	968824	12.11%	1.815%
15	7.452	736	742	752	rBV	613142	975478	12.20%	1.827%
16	7.934	817	824	832	rBV	565048	891504	11.15%	1.670%
17	8.646	939	945	958	rBV	441541	719405	9.00%	1.348%
18	9.128	1020	1027	1038	rBV	722474	1170238	14.63%	2.192%
19	9.334	1058	1062	1068	rVB7	6208	10595	0.13%	0.020%
20	9.846	1142	1149	1161	rBV	570192	932050	11.65%	1.746%
21	10.369	1230	1238	1249	rBV	811863	1402711	17.54%	2.628%
22	10.757	1295	1304	1311	rBV	743672	1260741	15.76%	2.362%
23	10.922	1324	1332	1349	rBV	773750	1334867	16.69%	2.500%
24	12.340	1568	1573	1579	rVB4	15135	27922	0.35%	0.052%
25	13.434	1753	1759	1766	rVB4	13532	27105	0.34%	0.051%
26	13.557	1775	1780	1786	rBV10	4148	9264	0.12%	0.017%
27	14.004	1850	1856	1867	rBV	1678778	2368128	29.61%	4.436%
28	14.292	1898	1905	1916	rBV	1957305	2738251	34.24%	5.129%
29	14.592	1949	1956	1964	rBV	1144958	1639681	20.50%	3.071%
30	14.828	1990	1996	2014	rBV	87974	205378	2.57%	0.385%
31	15.198	2055	2059	2065	rBV7	4645	8865	0.11%	0.017%
32	15.410	2092	2095	2101	rVB2	10987	13993	0.17%	0.026%
33	15.587	2118	2125	2141	rBV	2543326	3707707	46.36%	6.945%
34	15.722	2141	2148	2161	rVV	765625	1066757	13.34%	1.998%
35	15.828	2162	2166	2172	rVB5	13721	24883	0.31%	0.047%
36	16.869	2338	2343	2351	rVB3	34708	51404	0.64%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017300.D
 Acq On : 22 Sep 2023 22:51
 Operator : MA/JU
 Sample : 04410-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	17.022	2363	2369	2371	rBV7	6280	11902	0.15%	0.022%
38	17.363	2421	2427	2436	rBV	1468256	2050931	25.64%	3.842%
39	17.463	2438	2444	2457	rBV2	3244920	4493422	56.19%	8.417%
40	18.204	2566	2570	2578	rBV2	54912	79310	0.99%	0.149%
41	18.292	2583	2585	2591	rVB	11034	13429	0.17%	0.025%
42	19.280	2749	2753	2757	rBV2	40675	51434	0.64%	0.096%
43	19.345	2761	2764	2769	rVB	43791	58994	0.74%	0.111%
44	19.445	2778	2781	2787	rBV7	24035	33397	0.42%	0.063%
45	19.710	2820	2826	2832	rBV	4292797	5687381	71.11%	10.654%
46	21.469	3120	3125	3131	rBV	1774076	2276193	28.46%	4.264%
47	23.821	3518	3525	3537	rVB	2844111	5694360	71.20%	10.667%
48	23.986	3547	3553	3565	rVB	1175827	2426777	30.34%	4.546%




Sum of corrected areas: 53385078

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017300.D
Acq On : 22 Sep 2023 22:51
Operator : MA/JU
Sample : 04410-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

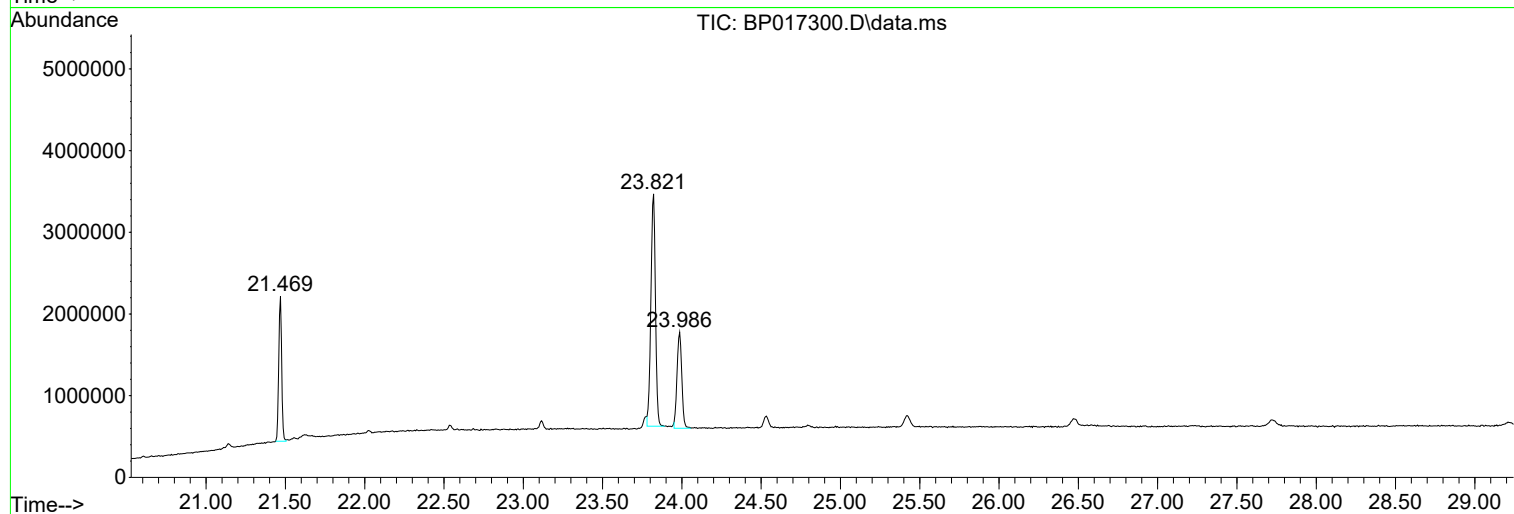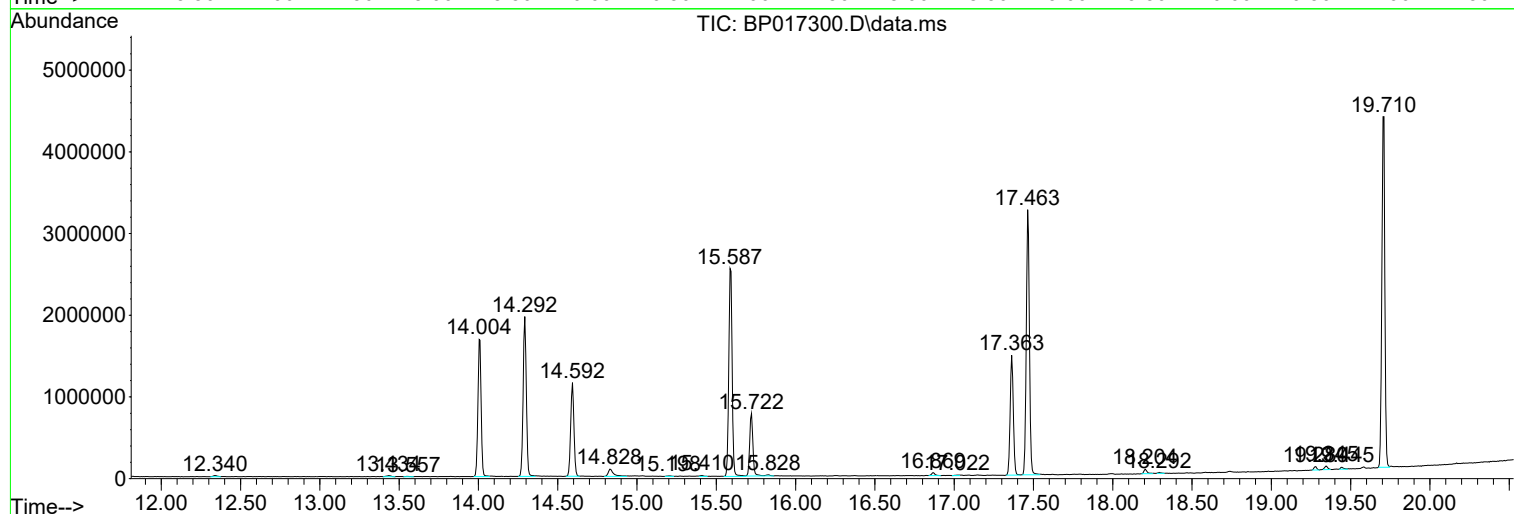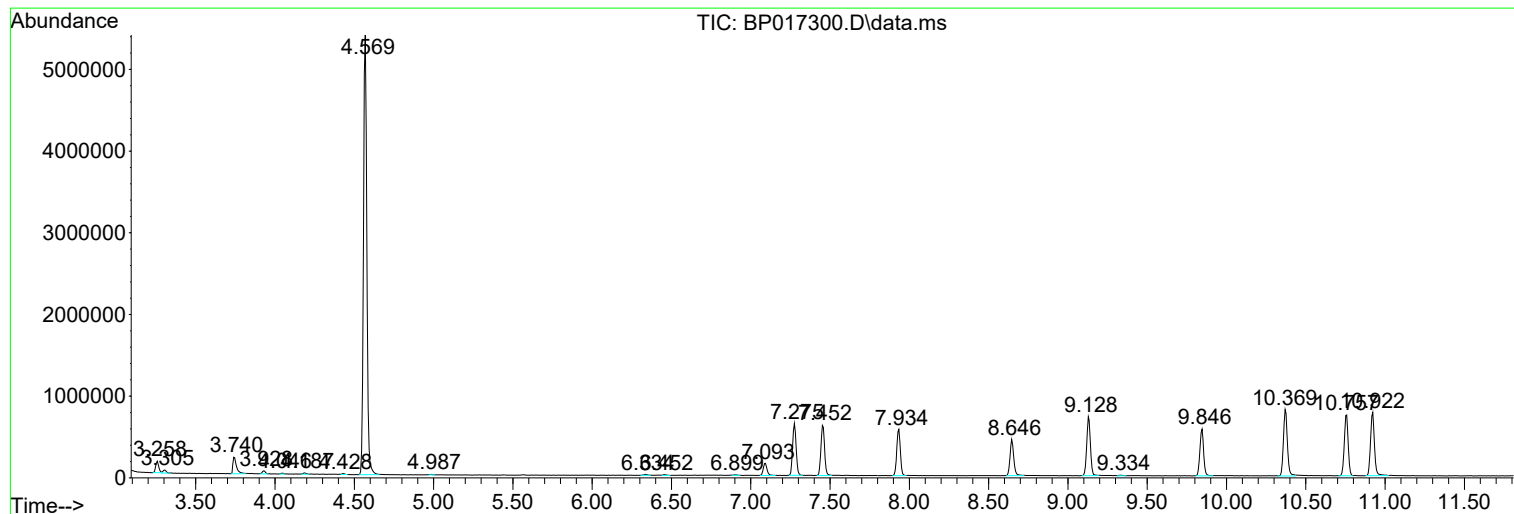

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017300.D
Acq On : 22 Sep 2023 22:51
Operator : MA/JU
Sample : 04410-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHM4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	179.42 ng/ul	7997530	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

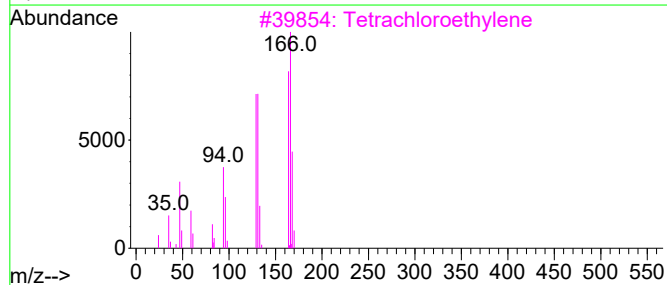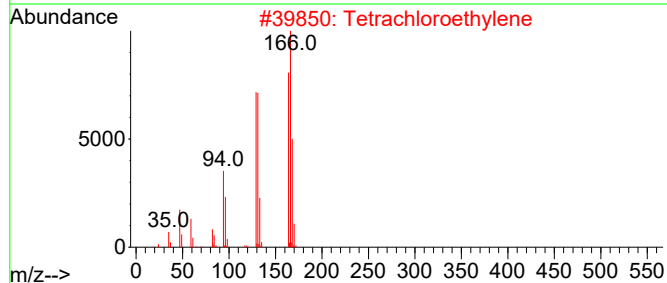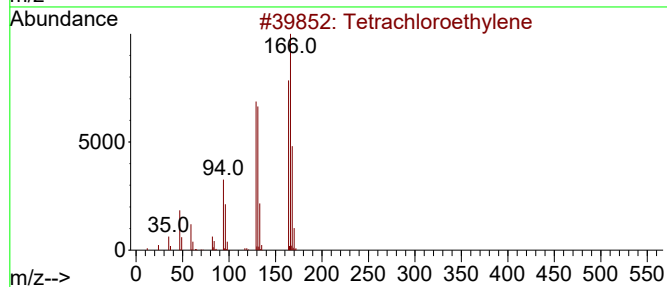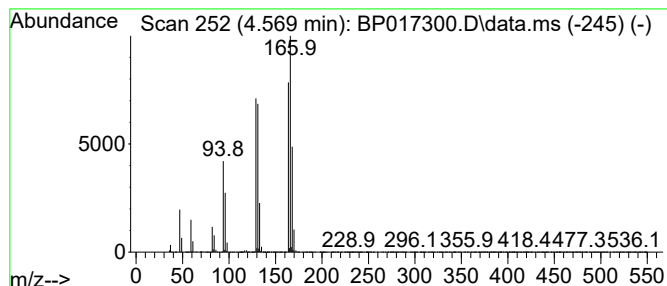

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017300.D
Acq On : 22 Sep 2023 22:51
Operator : MA/JU
Sample : 04410-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.569	179.4	ng/ul	7997530	1	7.934	891504	20.0