

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017301.D
 Acq On : 22 Sep 2023 23:26
 Operator : MA/JU
 Sample : 04410-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	24	29	34	rBV	313408	432178	7.96%	0.861%
2	3.305	34	37	40	rVV	45931	60195	1.11%	0.120%
3	3.340	40	43	49	rVB	35198	45426	0.84%	0.091%
4	3.740	107	111	131	rBV	262310	420252	7.74%	0.837%
5	3.928	138	143	151	rVB	45961	71199	1.31%	0.142%
6	4.046	160	163	168	rVB3	9895	13184	0.24%	0.026%
7	4.187	184	187	193	rVB3	16861	24479	0.45%	0.049%
8	4.428	226	228	233	rVB3	12255	15761	0.29%	0.031%
9	4.569	245	252	268	rBV	3086438	4507392	82.99%	8.982%
10	4.981	318	322	328	rVB2	9061	15245	0.28%	0.030%
11	6.340	546	553	557	rBV2	15318	22190	0.41%	0.044%
12	6.905	646	649	656	rVB7	9336	14363	0.26%	0.029%
13	7.087	674	680	691	rBV	193347	315398	5.81%	0.629%
14	7.275	704	712	721	rBV	723291	1104049	20.33%	2.200%
15	7.452	735	742	752	rBV	735797	1143493	21.05%	2.279%
16	7.934	817	824	834	rBV	508458	811330	14.94%	1.617%
17	8.646	938	945	956	rBV	552453	889715	16.38%	1.773%
18	8.722	956	958	964	rVB7	4038	6567	0.12%	0.013%
19	9.128	1018	1027	1035	rBV	795549	1307431	24.07%	2.605%
20	9.581	1099	1104	1109	rVB9	2752	5690	0.10%	0.011%
21	9.846	1141	1149	1160	rBV	660822	1051986	19.37%	2.096%
22	10.369	1231	1238	1254	rBV	928286	1598246	29.43%	3.185%
23	10.757	1295	1304	1311	rBV	694892	1162448	21.40%	2.316%
24	10.922	1325	1332	1350	rBV	696752	1182496	21.77%	2.356%
25	11.581	1438	1444	1452	rVB	3846	9112	0.17%	0.018%
26	11.828	1482	1486	1490	rVB6	3833	6330	0.12%	0.013%
27	12.340	1569	1573	1578	rBV	18400	28961	0.53%	0.058%
28	12.557	1606	1610	1614	rBV7	3969	7176	0.13%	0.014%
29	13.434	1754	1759	1766	rBV2	20928	33309	0.61%	0.066%
30	13.557	1776	1780	1786	rVB8	3951	6579	0.12%	0.013%
31	13.822	1822	1825	1832	rVB9	3802	6879	0.13%	0.014%
32	14.010	1850	1857	1867	rBV	1753394	2448372	45.08%	4.879%
33	14.292	1898	1905	1921	rBV	2083231	2974050	54.76%	5.926%
34	14.592	1949	1956	1965	rBV	1045210	1495913	27.54%	2.981%
35	14.834	1991	1997	2010	rBV	95427	214320	3.95%	0.427%
36	15.387	2087	2091	2093	rBV5	4309	6093	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
 Data File : BP017301.D
 Acq On : 22 Sep 2023 23:26
 Operator : MA/JU
 Sample : 04410-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.592	2119	2126	2133	rBV	2661687	3799424	69.95%	7.571%
38	15.657	2133	2137	2142	rVV	61286	103684	1.91%	0.207%
39	15.722	2142	2148	2161	rVV	746570	1028992	18.95%	2.050%
40	15.828	2162	2166	2171	rVB5	14987	21516	0.40%	0.043%
41	16.869	2339	2343	2349	rVB6	18919	27768	0.51%	0.055%
42	17.034	2367	2371	2376	rBV8	6360	8375	0.15%	0.017%
43	17.157	2388	2392	2396	rBV6	4282	6868	0.13%	0.014%
44	17.363	2421	2427	2434	rBV	1337457	1881243	34.64%	3.749%
45	17.463	2438	2444	2457	rBV	3220772	4469013	82.28%	8.905%
46	17.622	2469	2471	2475	rVB5	6132	5470	0.10%	0.011%
47	17.716	2485	2487	2491	rBV5	4413	5817	0.11%	0.012%
48	18.204	2566	2570	2577	rBV3	42283	66435	1.22%	0.132%
49	19.275	2749	2752	2756	rBV2	39995	49145	0.90%	0.098%
50	19.345	2761	2764	2769	rVB	43653	58068	1.07%	0.116%
51	19.445	2777	2781	2787	rBV5	31069	50377	0.93%	0.100%
52	19.704	2820	2825	2834	rBV	4139489	5389984	99.24%	10.741%
53	21.469	3120	3125	3132	rBV	1562096	2069678	38.11%	4.124%
54	23.816	3518	3524	3535	rVB2	2702294	5431276	100.00%	10.823%
55	23.980	3546	3552	3568	rVB	1068437	2251682	41.46%	4.487%




Sum of corrected areas: 50182622

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017301.D
Acq On : 22 Sep 2023 23:26
Operator : MA/JU
Sample : 04410-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

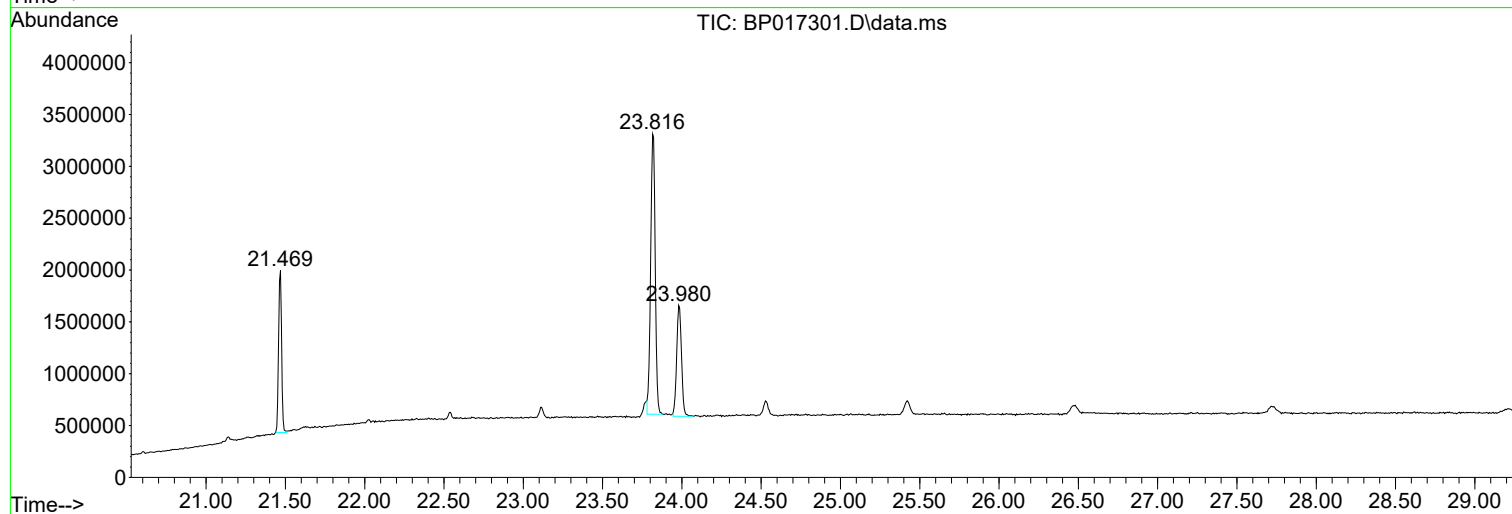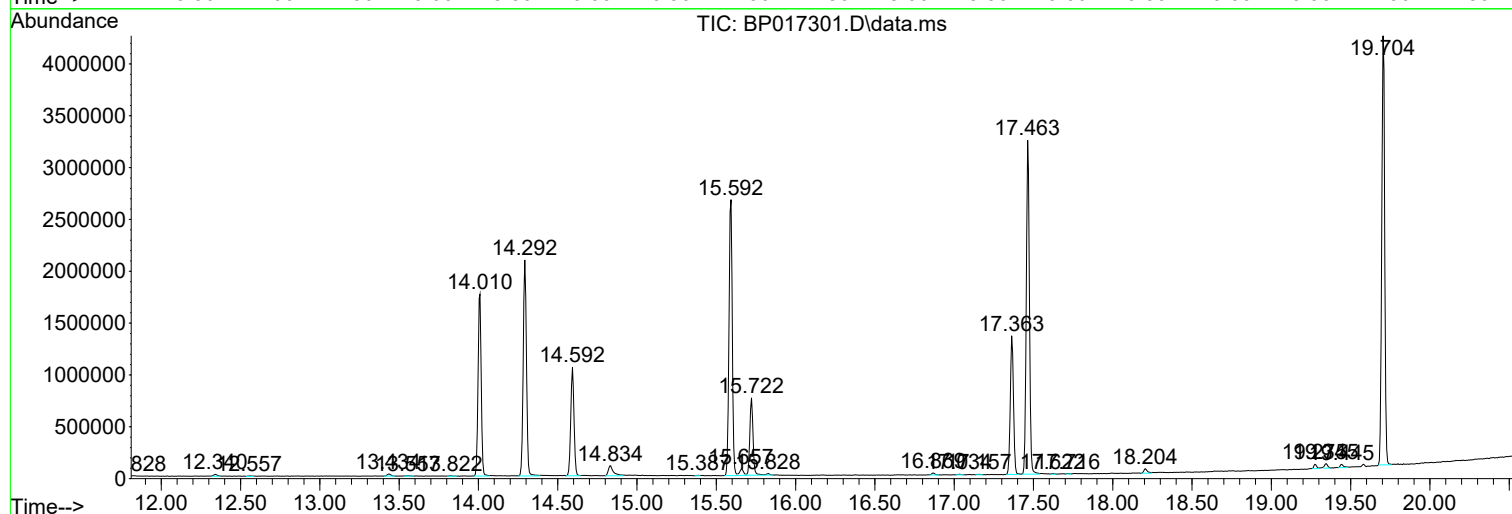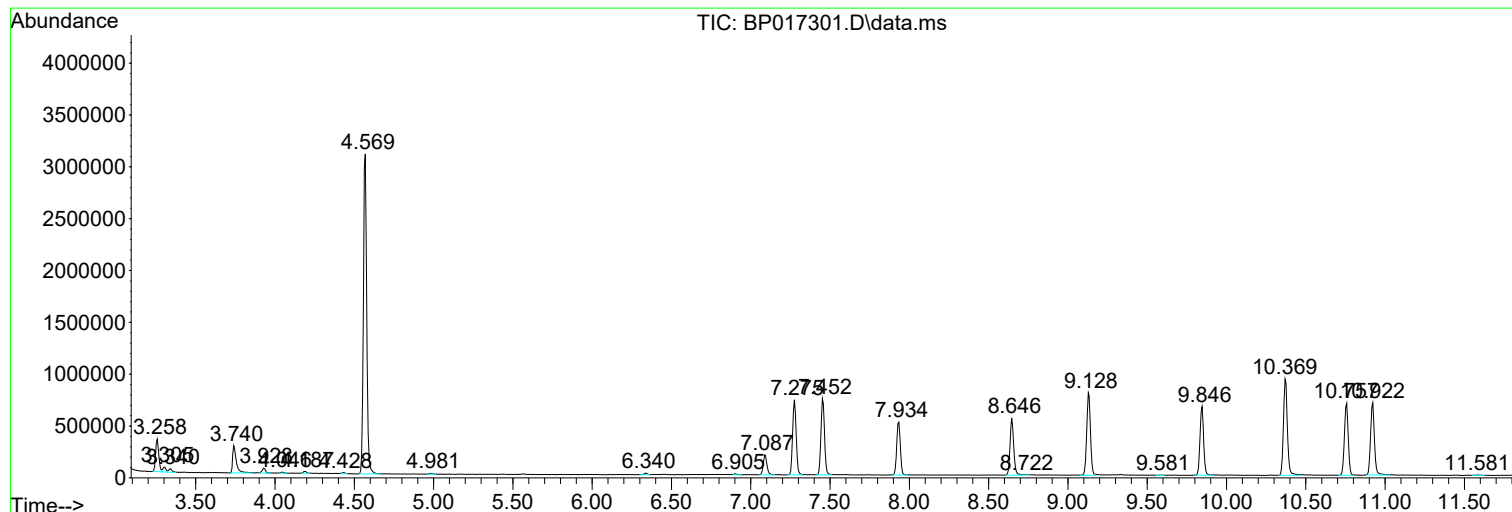

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017301.D
Acq On : 22 Sep 2023 23:26
Operator : MA/JU
Sample : 04410-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	111.11 ng/ul	4507390	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

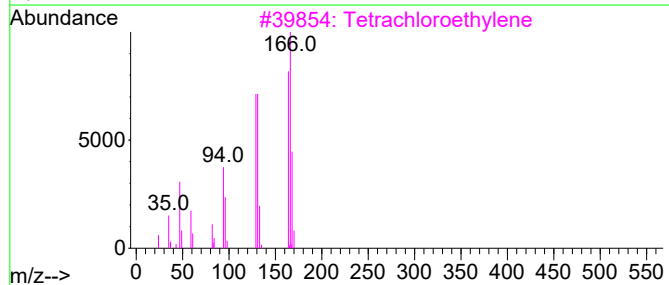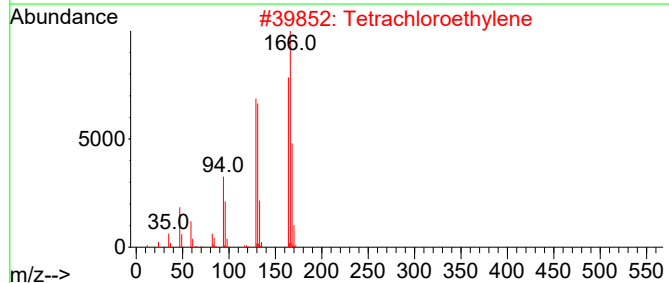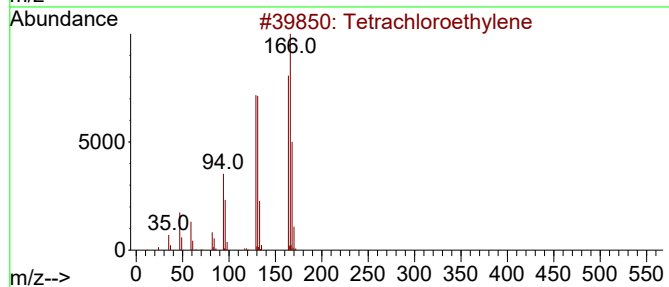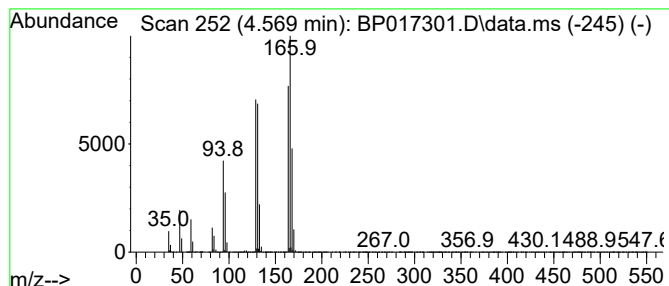

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092223\
Data File : BP017301.D
Acq On : 22 Sep 2023 23:26
Operator : MA/JU
Sample : 04410-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.569	111.1	ng/ul	4507390	1	7.934	811330	20.0