

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092319\
 Data File : BP000370.D
 Acq On : 23 Sep 2019 19:03
 Operator : HP/JU
 Sample : PB123244BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123244BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	562	566	570	rBV	4241952	4057977	41.53%	7.053%
2	6.428	733	738	741	rBV	4430481	4124527	42.21%	7.169%
3	6.563	756	761	764	rBV	5112823	4527458	46.34%	7.869%
4	6.787	796	799	803	rBV	1581430	1331414	13.63%	2.314%
5	6.946	822	826	830	rBV	5970101	5472806	56.01%	9.512%
6	7.352	889	895	898	rBV	3977449	3889235	39.80%	6.760%
7	8.069	1013	1017	1021	rBV	2044024	1696243	17.36%	2.948%
8	9.151	1196	1201	1204	rBV	10769711	9672721	99.00%	16.811%
9	9.828	1313	1316	1320	rBV	2737780	2477719	25.36%	4.306%
10	10.622	1447	1451	1478	rBV	3931333	3883767	39.75%	6.750%
11	11.328	1567	1571	1574	rBV	2287713	2119960	21.70%	3.685%
12	12.934	1838	1844	1847	rBV	9438929	9770839	100.00%	16.982%
13	13.992	2019	2024	2027	rBV	2379734	2245555	22.98%	3.903%
14	15.475	2270	2276	2281	rBV	1822924	2266507	23.20%	3.939%


Sum of corrected areas: 57536728

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092319\
Data File : BP000370.D
Acq On : 23 Sep 2019 19:03
Operator : HP/JU
Sample : PB123244BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123244BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

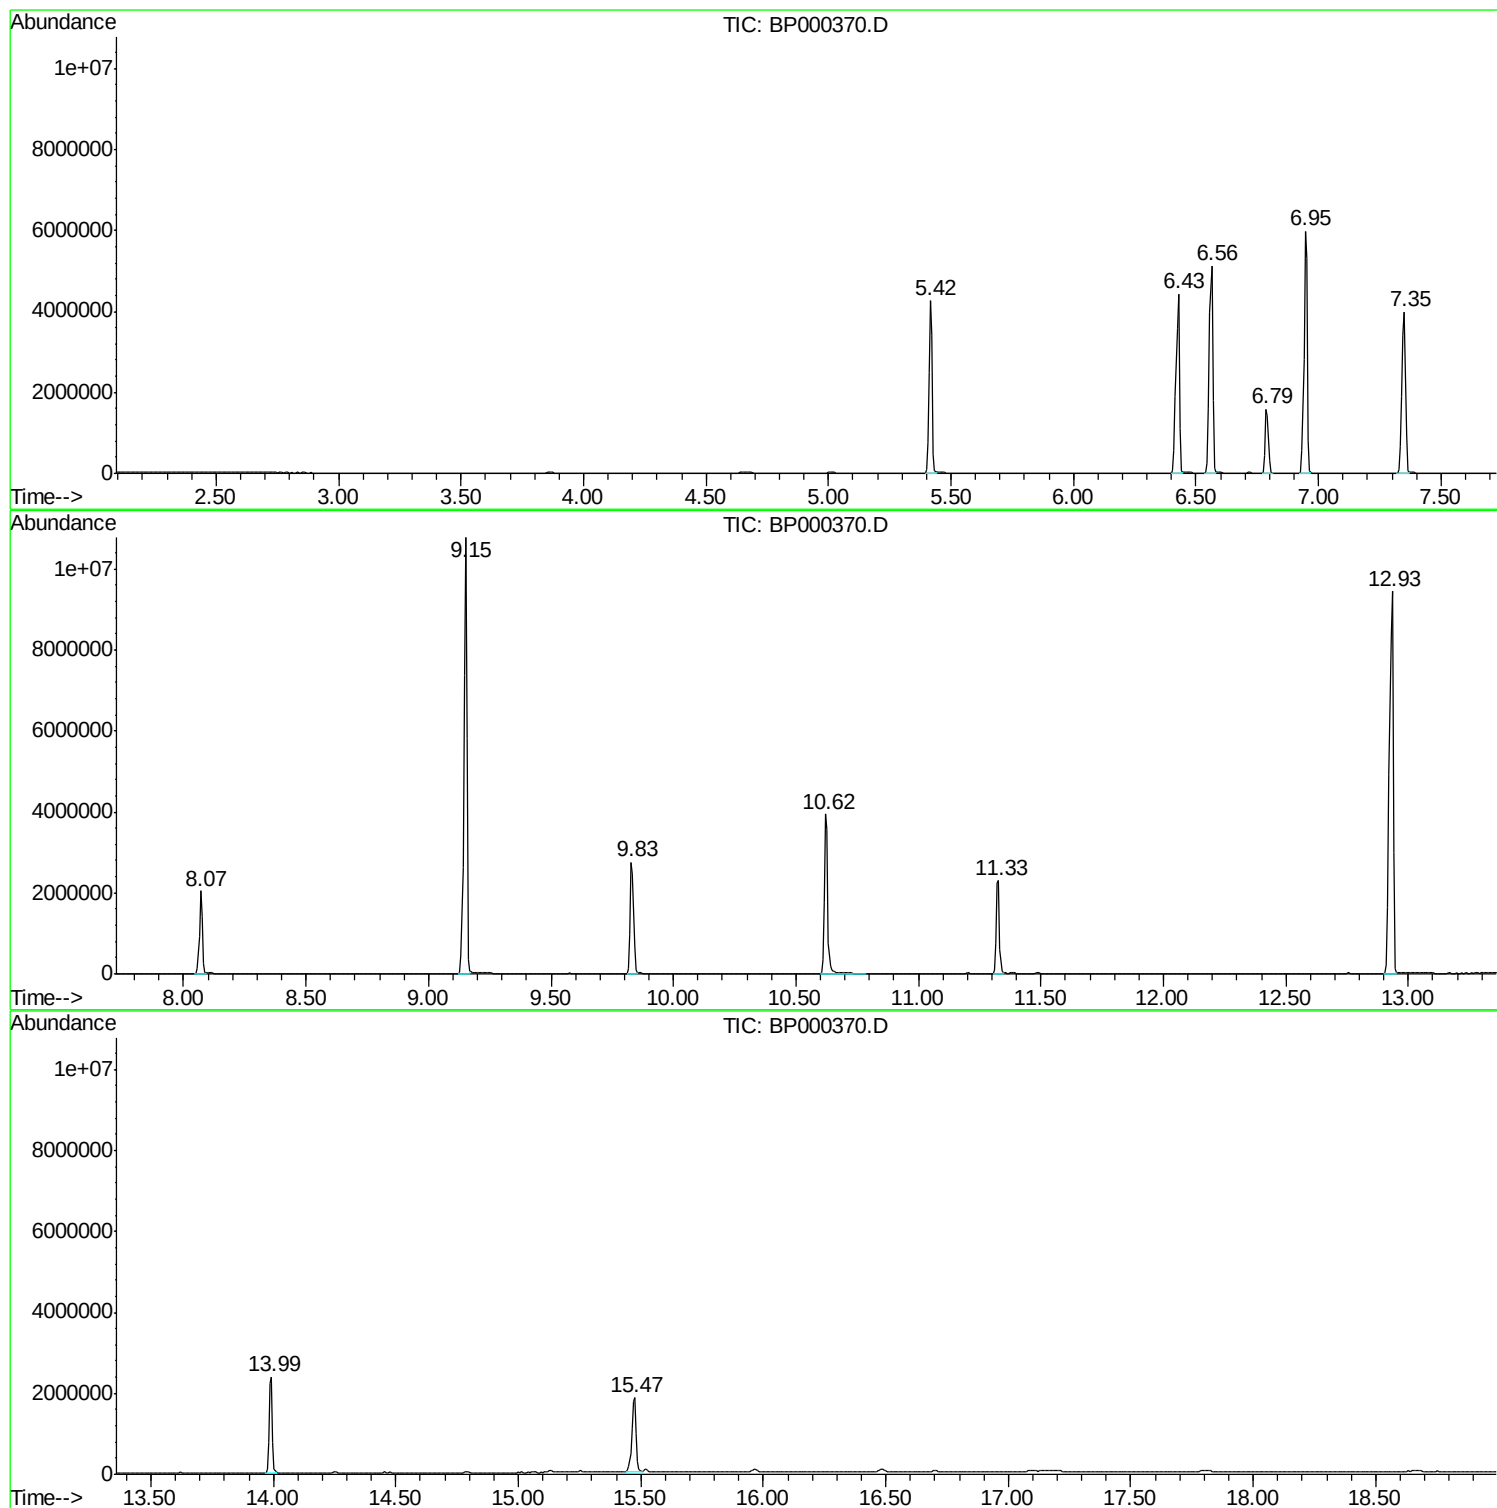

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP092319\
Data File : BP000370.D
Acq On : 23 Sep 2019 19:03
Operator : HP/JU
Sample : PB123244BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123244BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	68.01 ng	4527460	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	12
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

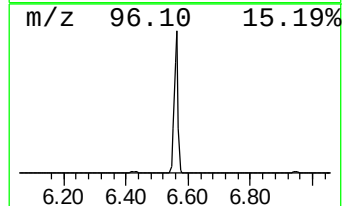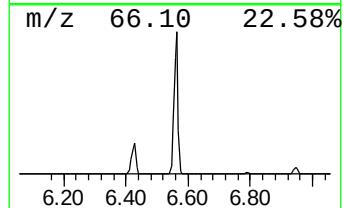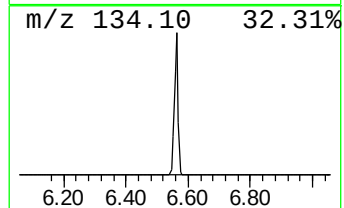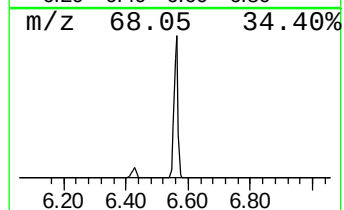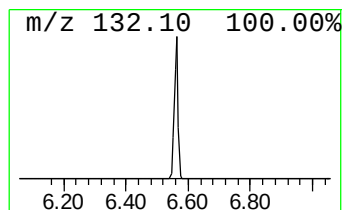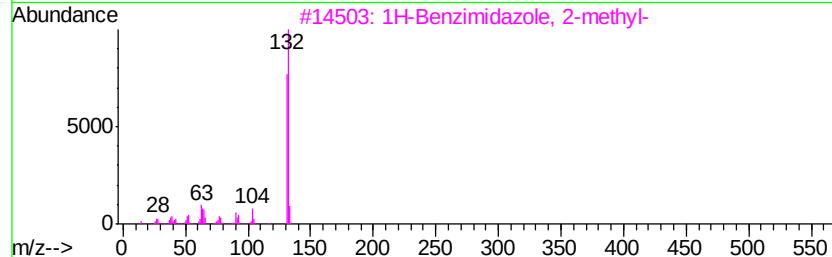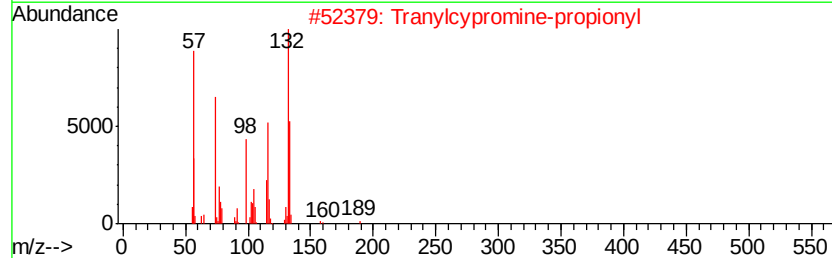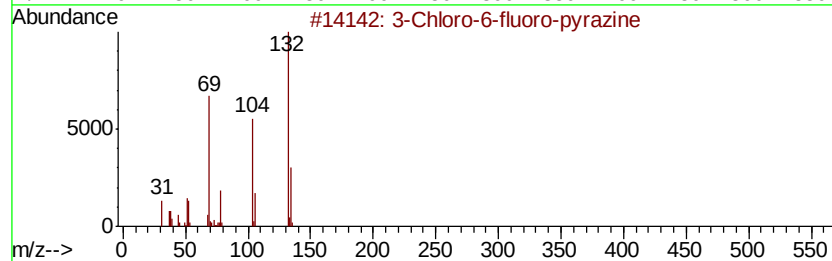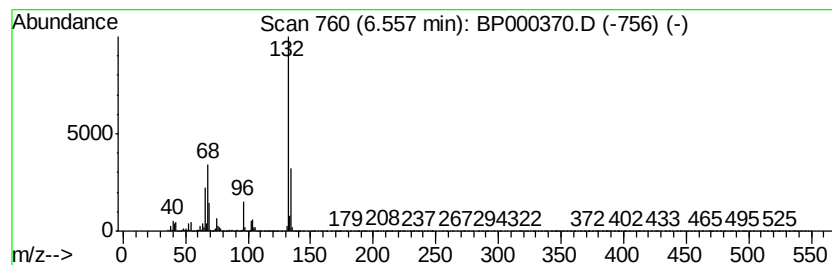

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092319\
Data File : BP000370.D
Acq On : 23 Sep 2019 19:03
Operator : HP/JU
Sample : PB123244BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123244BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	68.0	ng	4527460	1	6.79	1331410	20.0