


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP092319\
 Data File : BP000366.D
 Acq On : 23 Sep 2019 16:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 19 14:44:51 2019

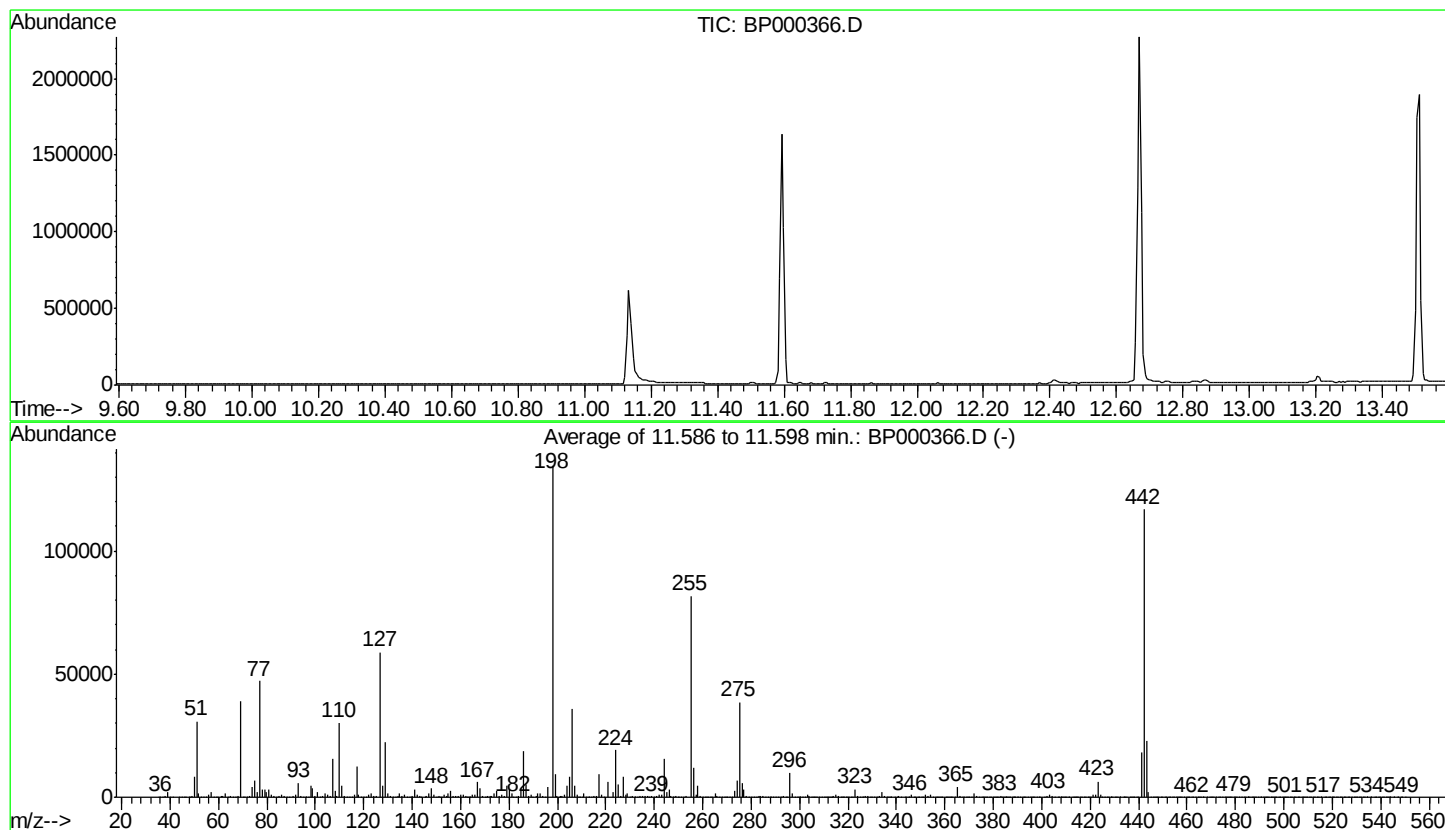

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.8	30722	PASS
68	69	0.00	2	2.0	789	PASS
69	198	0.00	100	29.0	38980	PASS
70	69	0.00	2	0.6	226	PASS
127	198	10	80	43.7	58837	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134594	PASS
199	198	5	9	6.9	9235	PASS
275	198	10	60	28.7	38609	PASS
365	198	1	100	3.2	4324	PASS
441	198	0.01	100	13.6	18253	PASS
442	198	50	100	86.8	116830	PASS
443	442	15	24	19.5	22810	PASS