
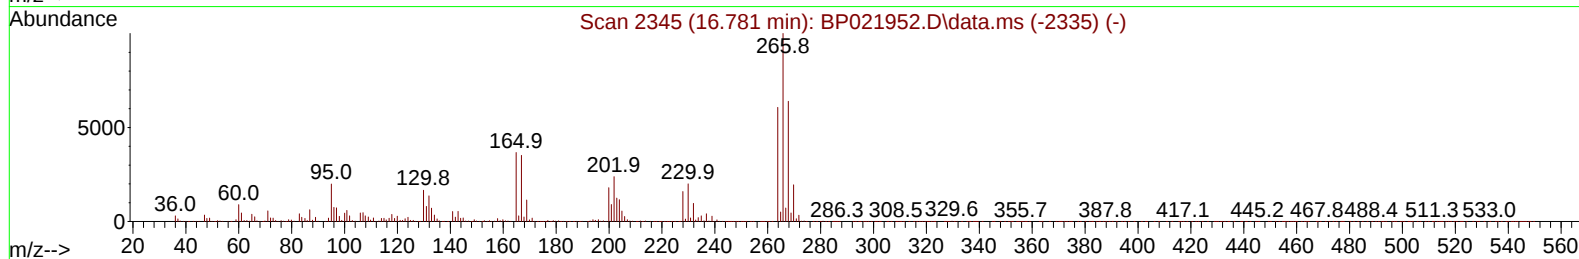
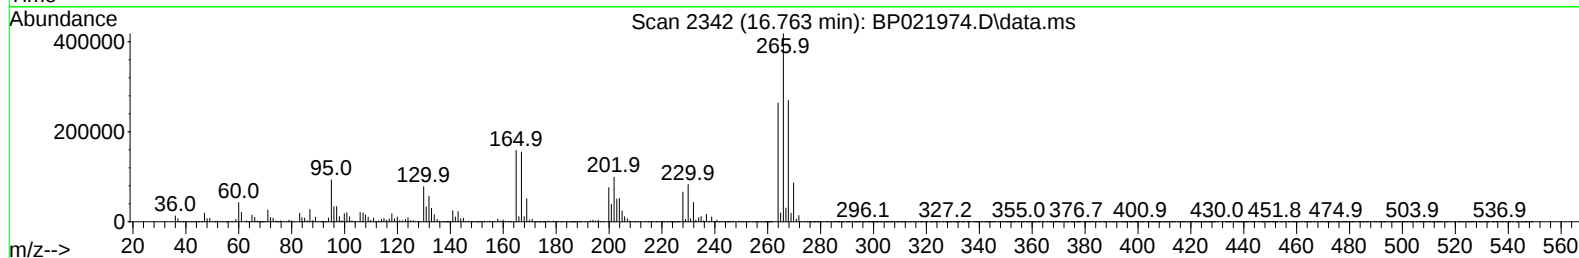


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092324\
Data File : BP021974.D
Acq On : 23 Sep 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 12:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

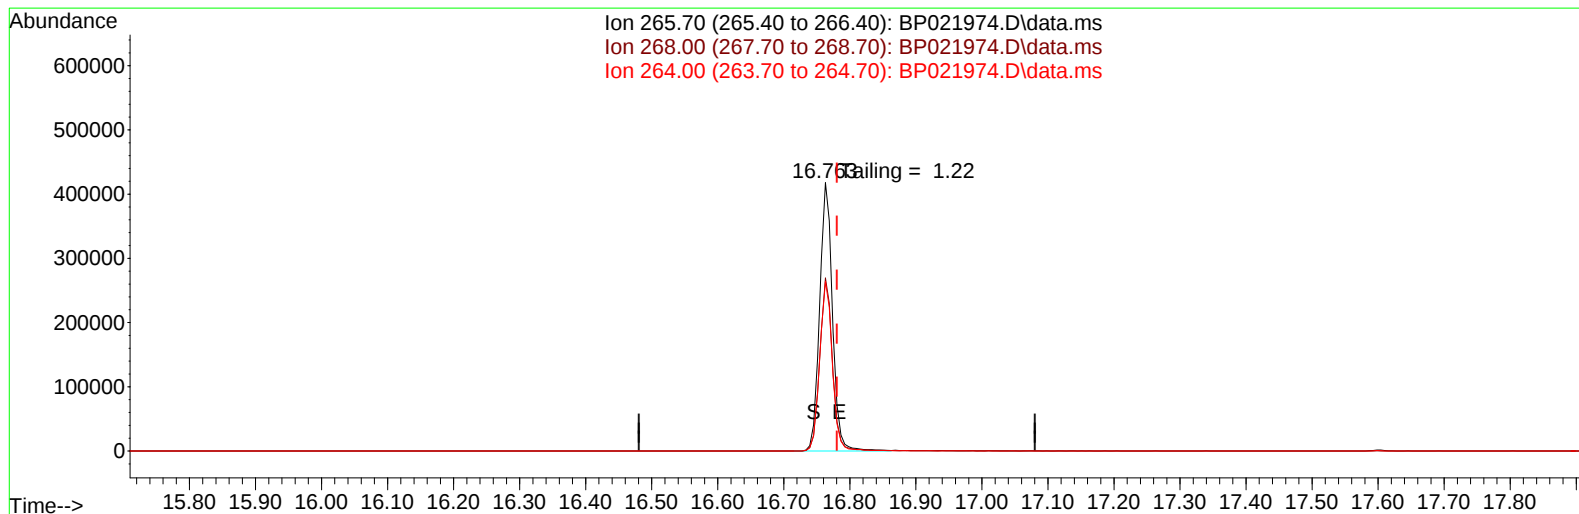

TIC: BP021974.D\data.ms

(70) Pentachlorophenol (C)




16.763min (-0.018) 5779292.50 ng

response 565102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.50
264.00	60.70	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092324\
Data File : BP021974.D
Acq On : 23 Sep 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 12:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

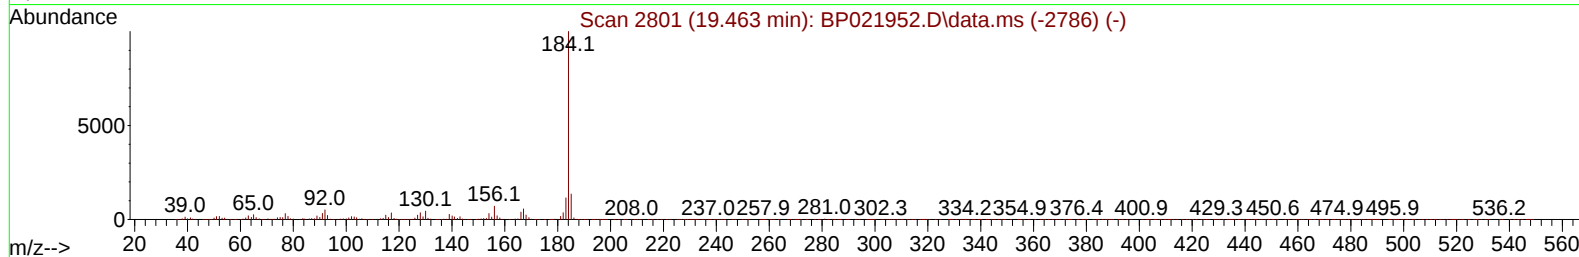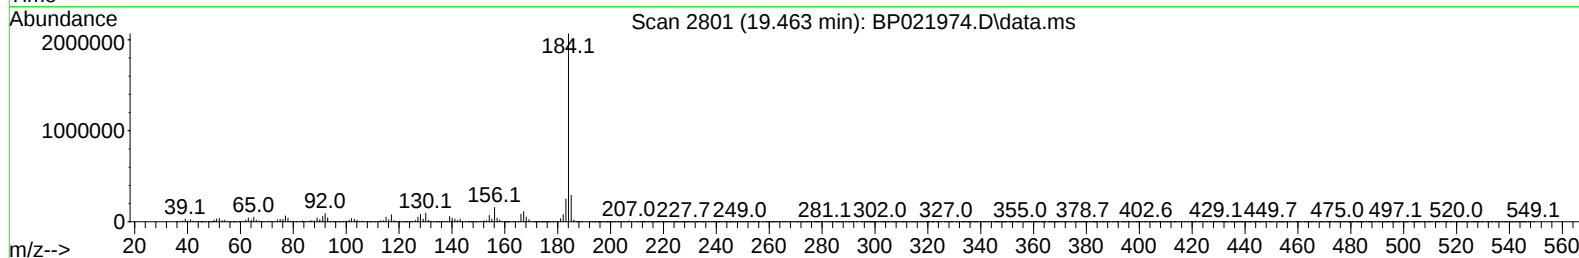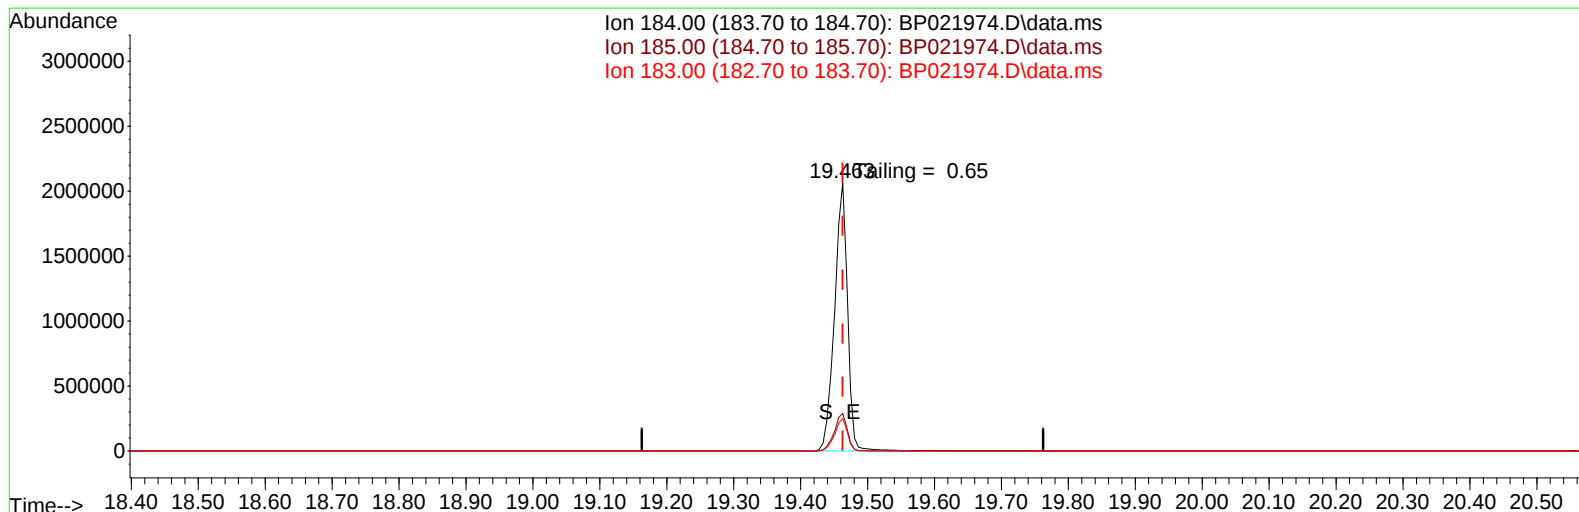

TIC: BP021974.D\data.ms

(77) Benzidine**19.463min (+ 0.000) 13419701.31 ng****response 2787920**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.05
183.00	11.50	12.08
0.00	0.00	0.00