

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022059.D
 Acq On : 26 Sep 2024 12:28
 Operator : RC/JU
 Sample : P4080-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AP3

Quant Time: Sep 27 01:16:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	79803	20.000	ng/ul	0.00
20) Naphthalene-d8	10.463	136	311385	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	276061	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	755244	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	916496	20.000	ng/ul	0.00
88) Perylene-d12	24.821	264	1032431	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	11191	5.493	ng/uL	0.00
4) Pyridine-d5	3.634	84	55931	9.604	ng/ul	0.00
7) Phenol-d5	6.887	99	88420	13.545	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	147545	36.706	ng/ul	0.00
11) 2-Chlorophenol-d4	7.240	132	176422	37.353	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	156648	30.283	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	94376	40.494	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	109506	41.440	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.093	165	235927	41.111	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	183355	26.778	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	827741	38.789	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	863486	38.218	ng/ul	0.00
54) 4-Nitrophenol-d4	14.528	143	47037	12.886	ng/ul	0.00
60) Fluorene-d10	15.328	176	799280	42.343	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	167731	35.772	ng/ul	0.00
73) Anthracene-d10	17.216	188	1448590	41.086	ng/ul	0.00
81) Pyrene-d10	19.598	212	2033765	42.833	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.592	264	2321430	42.750	ng/ul	-0.02
Target Compounds						
					Qvalue	
22) Nitrobenzene	8.875	77	7317	1.027	ng/ul#	25
30) Naphthalene	10.510	128	161135	9.835	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022059.D
Acq On : 26 Sep 2024 12:28
Operator : RC/JU
Sample : P4080-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AP3

Quant Time: Sep 27 01:16:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration




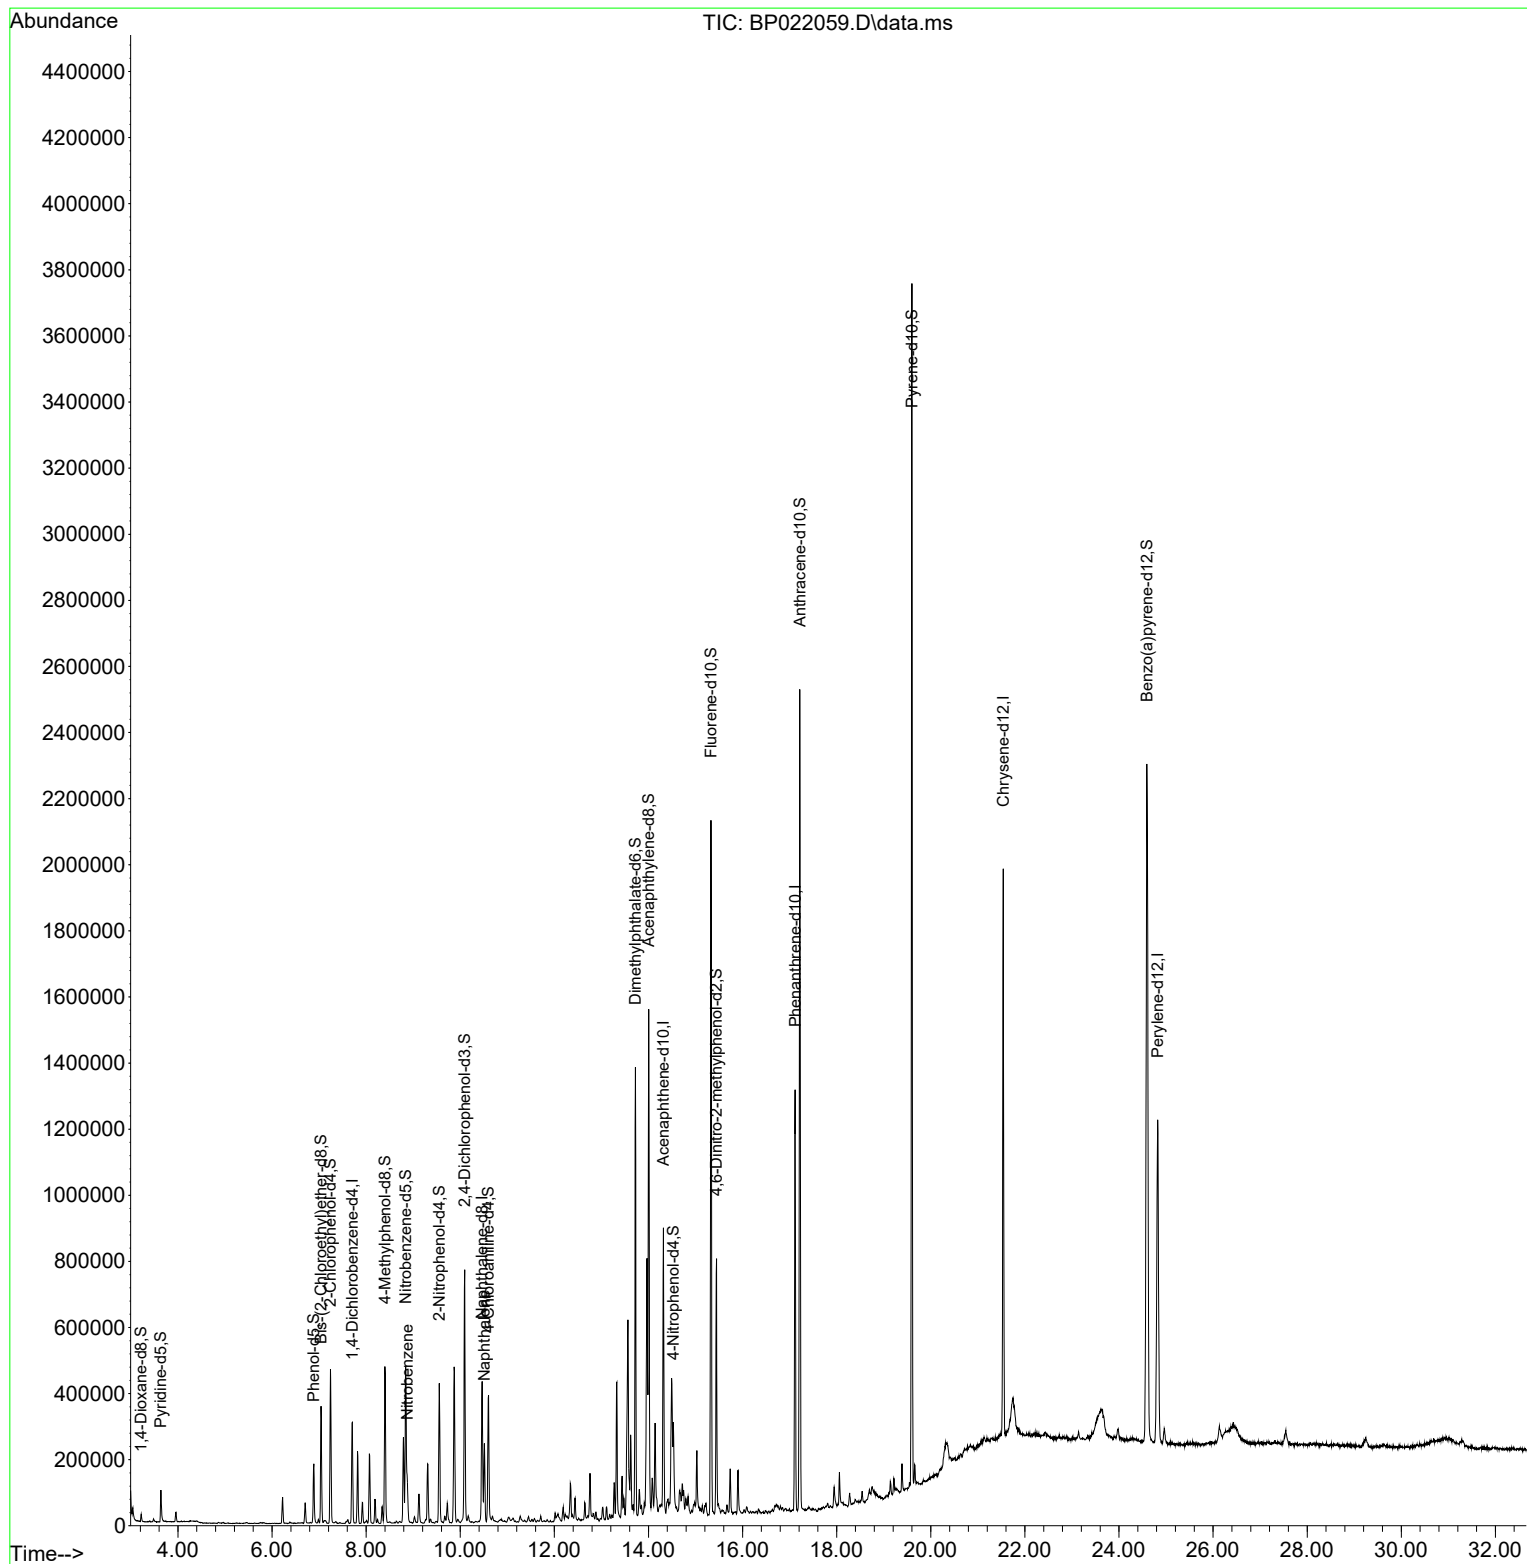


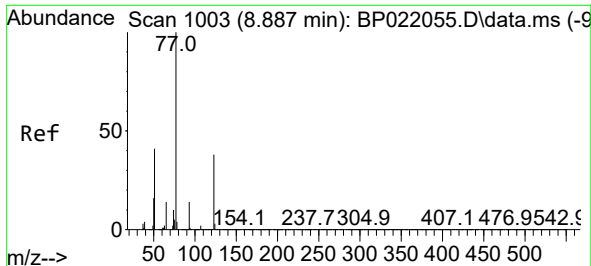

#22
Nitrobenzene
Concen: 1.027 ng/ul
RT: 8.875 min Scan# 1001
Delta R.T. -0.012 min
Lab File: BP022059.D
Acq: 26 Sep 2024 12:28

Instrument :
BNA_P
ClientSampleId :
C0AP3

Tgt Ion: 77 Resp: 7317
Ion Ratio Lower Upper
77 100
123 1.1 29.8 44.8#
65 60.1 11.3 16.9#

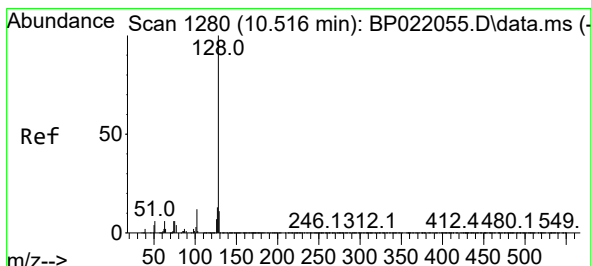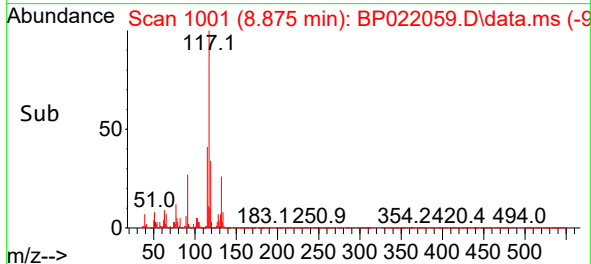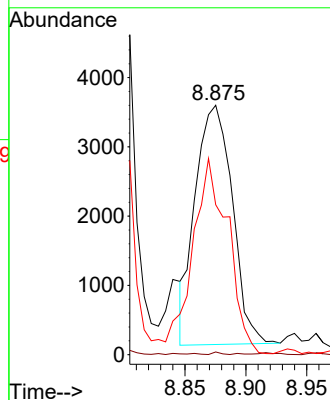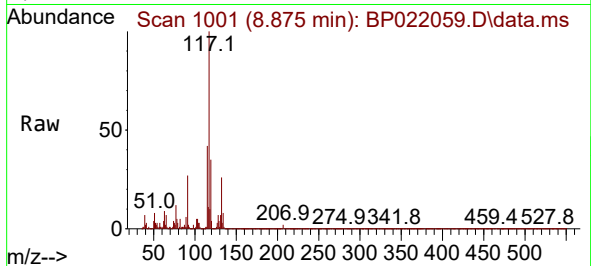

#30
Naphthalene
Concen: 9.835 ng/ul
RT: 10.510 min Scan# 1279
Delta R.T. -0.012 min
Lab File: BP022059.D
Acq: 26 Sep 2024 12:28

Tgt Ion: 128 Resp: 161135
Ion Ratio Lower Upper
128 100
129 11.3 8.9 13.3
127 13.7 10.9 16.3

