

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022060.D
 Acq On : 26 Sep 2024 13:08
 Operator : RC/JU
 Sample : P4080-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AP5

Quant Time: Sep 27 01:16:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	105804	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	395644	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	310406	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	809938	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	999559	20.000	ng/ul	0.00
88) Perylene-d12	24.816	264	1142863	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	15208	5.630	ng/uL	0.00
4) Pyridine-d5	3.640	84	61989	8.029	ng/ul	0.00
7) Phenol-d5	6.887	99	109689	12.674	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	189757	35.606	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	220789	35.259	ng/ul	0.00
15) 4-Methylphenol-d8	8.405	113	185905	27.107	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	114432	38.643	ng/ul	0.00
24) 2-Nitrophenol-d4	9.557	143	134222	39.976	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	278101	38.140	ng/ul	0.00
31) 4-Chloroaniline-d4	10.593	131	251748	28.936	ng/ul	-0.01
46) Dimethylphthalate-d6	13.722	166	965538	40.240	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	962634	37.892	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	50107	12.208	ng/ul	0.01
60) Fluorene-d10	15.322	176	835844	39.380	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.440	200	156556	31.134	ng/ul	0.00
73) Anthracene-d10	17.216	188	1543286	40.816	ng/ul	0.00
81) Pyrene-d10	19.586	212	2152666	41.569	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.598	264	2516359	41.862	ng/ul	-0.01
Target Compounds						
					Qvalue	
19) Hexachloroethane	8.793	117	6610	2.157	ng/ul#	1
30) Naphthalene	10.516	128	47965	2.304	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022060.D
Acq On : 26 Sep 2024 13:08
Operator : RC/JU
Sample : P4080-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AP5

Quant Time: Sep 27 01:16:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration




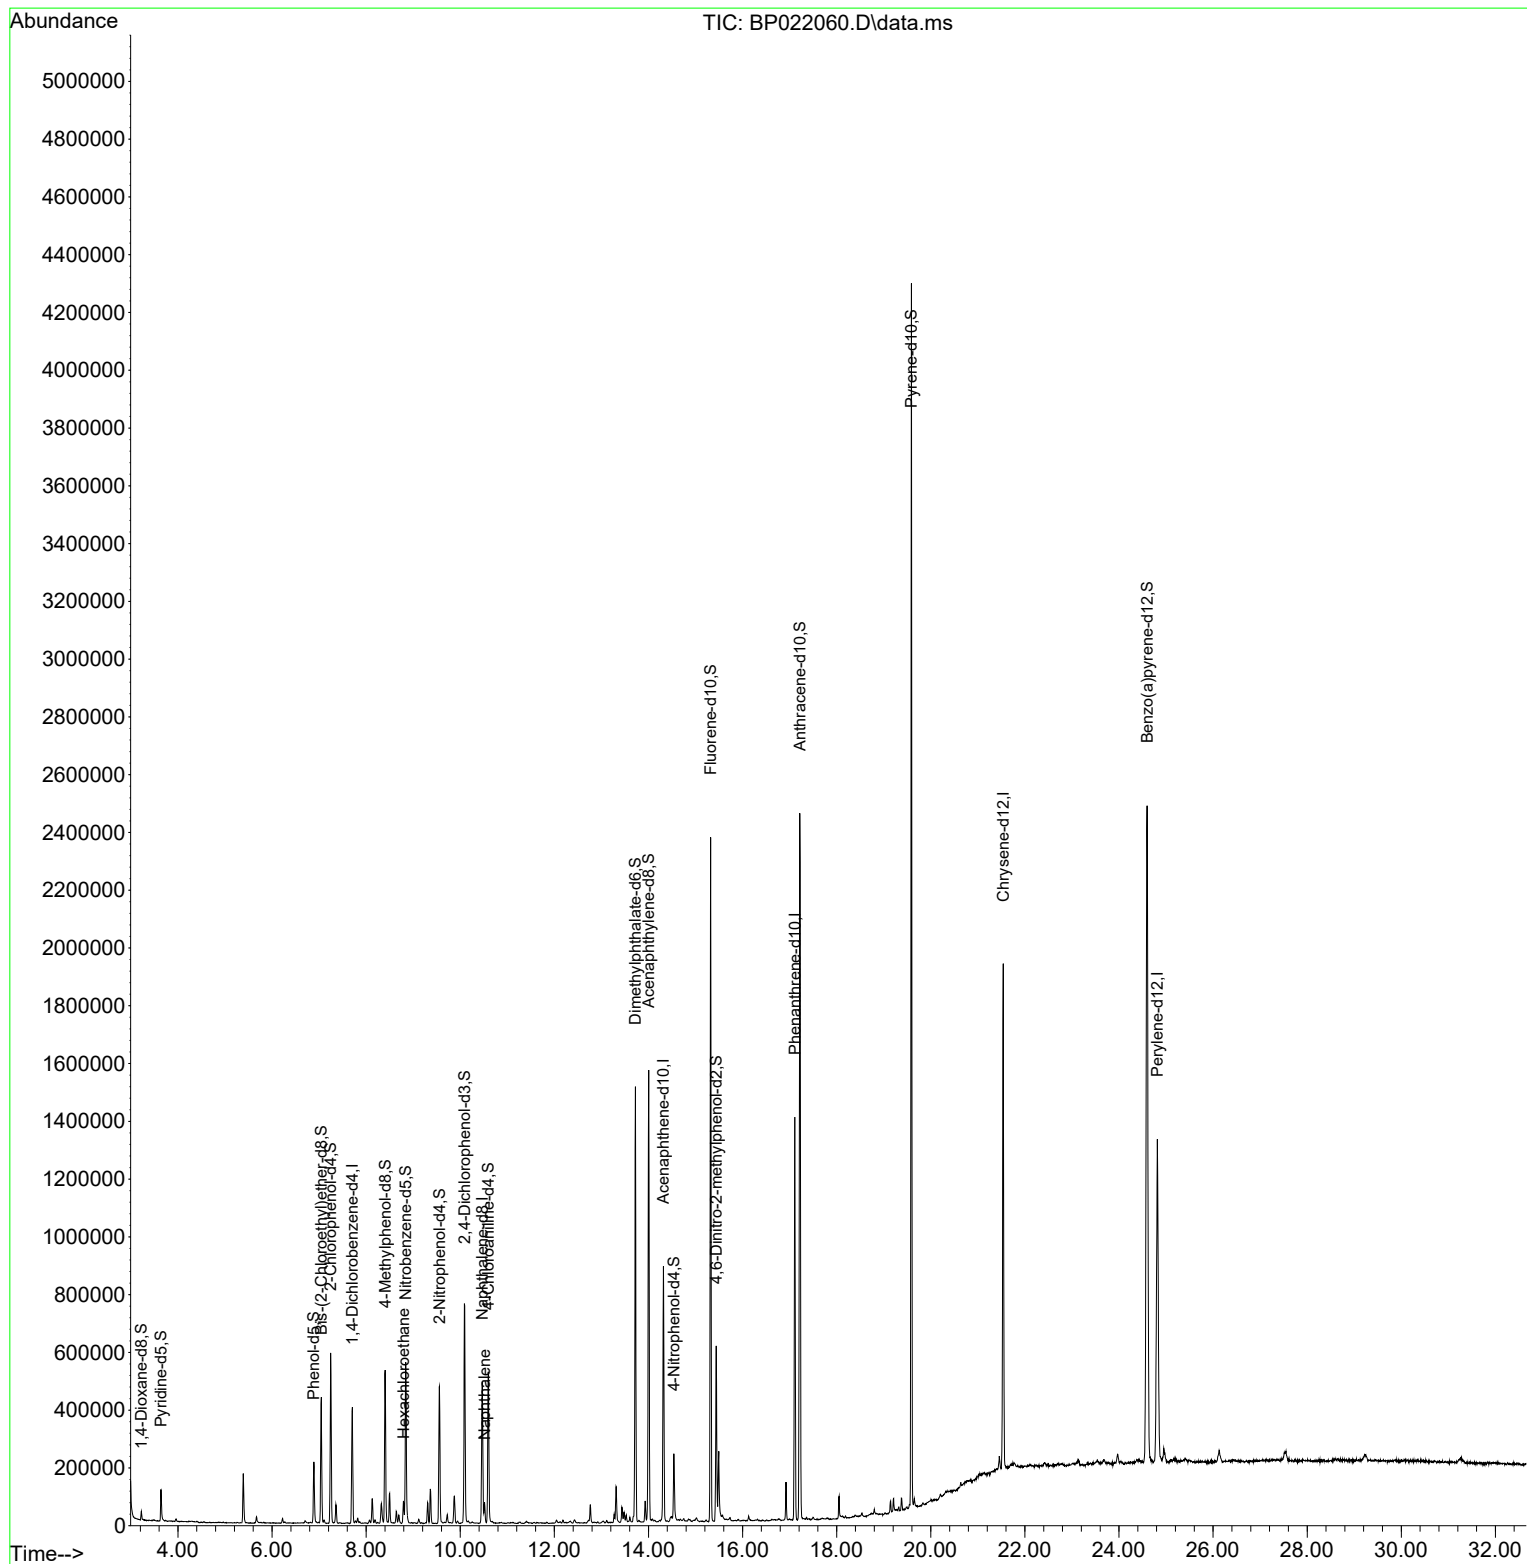


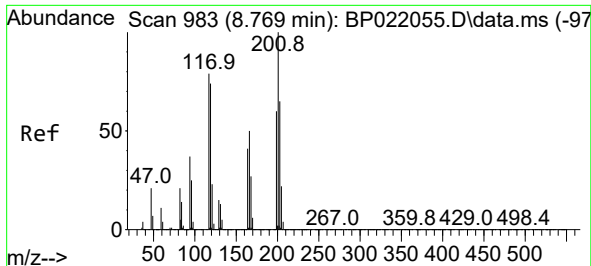

#19
Hexachloroethane
Concen: 2.157 ng/ul
RT: 8.793 min Scan# 91
Delta R.T. 0.018 min
Lab File: BP022060.D
Acq: 26 Sep 2024 13:08

Instrument :
BNA_P
ClientSampleId :
C0AP5

Tgt Ion:117 Resp: 6610
Ion Ratio Lower Upper
117 100
201 0.4 110.2 165.4#
199 0.3 67.9 101.9#

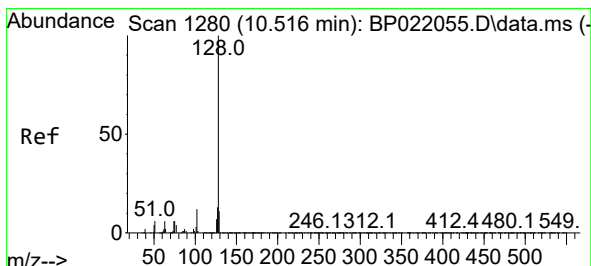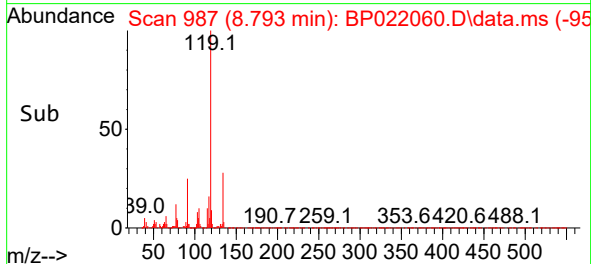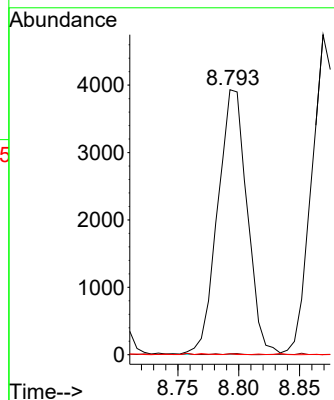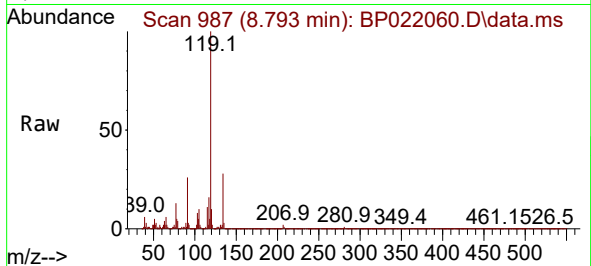

#30
Naphthalene
Concen: 2.304 ng/ul
RT: 10.516 min Scan# 1280
Delta R.T. -0.006 min
Lab File: BP022060.D
Acq: 26 Sep 2024 13:08

Tgt Ion:128 Resp: 47965
Ion Ratio Lower Upper
128 100
129 11.8 8.9 13.3
127 11.8 10.9 16.3

