

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022070.D
 Acq On : 26 Sep 2024 19:57
 Operator : RC/JU
 Sample : P4106-04DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0SX9DL

Quant Time: Sep 27 01:20:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	92010	20.000	ng/u1	0.01
20) Naphthalene-d8	10.469	136	305905	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.316	164	231101	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.104	188	598676	20.000	ng/u1	-0.01
79) Chrysene-d12	21.533	240	728811	20.000	ng/u1	0.00
88) Perylene-d12	24.827	264	855925	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	2177	0.927	ng/uL	0.00
4) Pyridine-d5	3.646	84	12557	1.870	ng/u1	0.01
7) Phenol-d5	6.887	99	12080	1.605	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	30248	6.527	ng/u1	0.00
11) 2-Chlorophenol-d4	7.246	132	32461	5.961	ng/u1	0.00
15) 4-Methylphenol-d8	8.405	113	23974	4.020	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	16684	7.287	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	18556	7.148	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	38497	6.828	ng/u1	0.00
31) 4-Chloroaniline-d4	10.599	131	19421	2.887	ng/u1	0.00
46) Dimethylphthalate-d6	13.722	166	142010	7.949	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	134870	7.131	ng/u1	0.00
54) 4-Nitrophenol-d4	14.510	143	94	0.031	ng/u1	-0.02
60) Fluorene-d10	15.322	176	126240	7.989	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.440	200	16720	4.498	ng/u1	0.00
73) Anthracene-d10	17.204	188	219462	7.852	ng/u1	-0.01
81) Pyrene-d10	19.586	212	302086	8.001	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.598	264	350208	7.779	ng/u1	-0.01
Target Compounds						
13) 2-Methylphenol	8.093	108	164443	28.867	ng/u1	93
22) Nitrobenzene	8.887	77	145050	20.721	ng/u1	99
39) 1,2,4,5-Tetrachloroben...	12.499	216	123080	14.365	ng/u1#	95
75) 1,2,3,4-Tetrachloroben...	13.104	216	293652	32.687	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022070.D
Acq On : 26 Sep 2024 19:57
Operator : RC/JU
Sample : P4106-04DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SX9DL

Quant Time: Sep 27 01:20:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

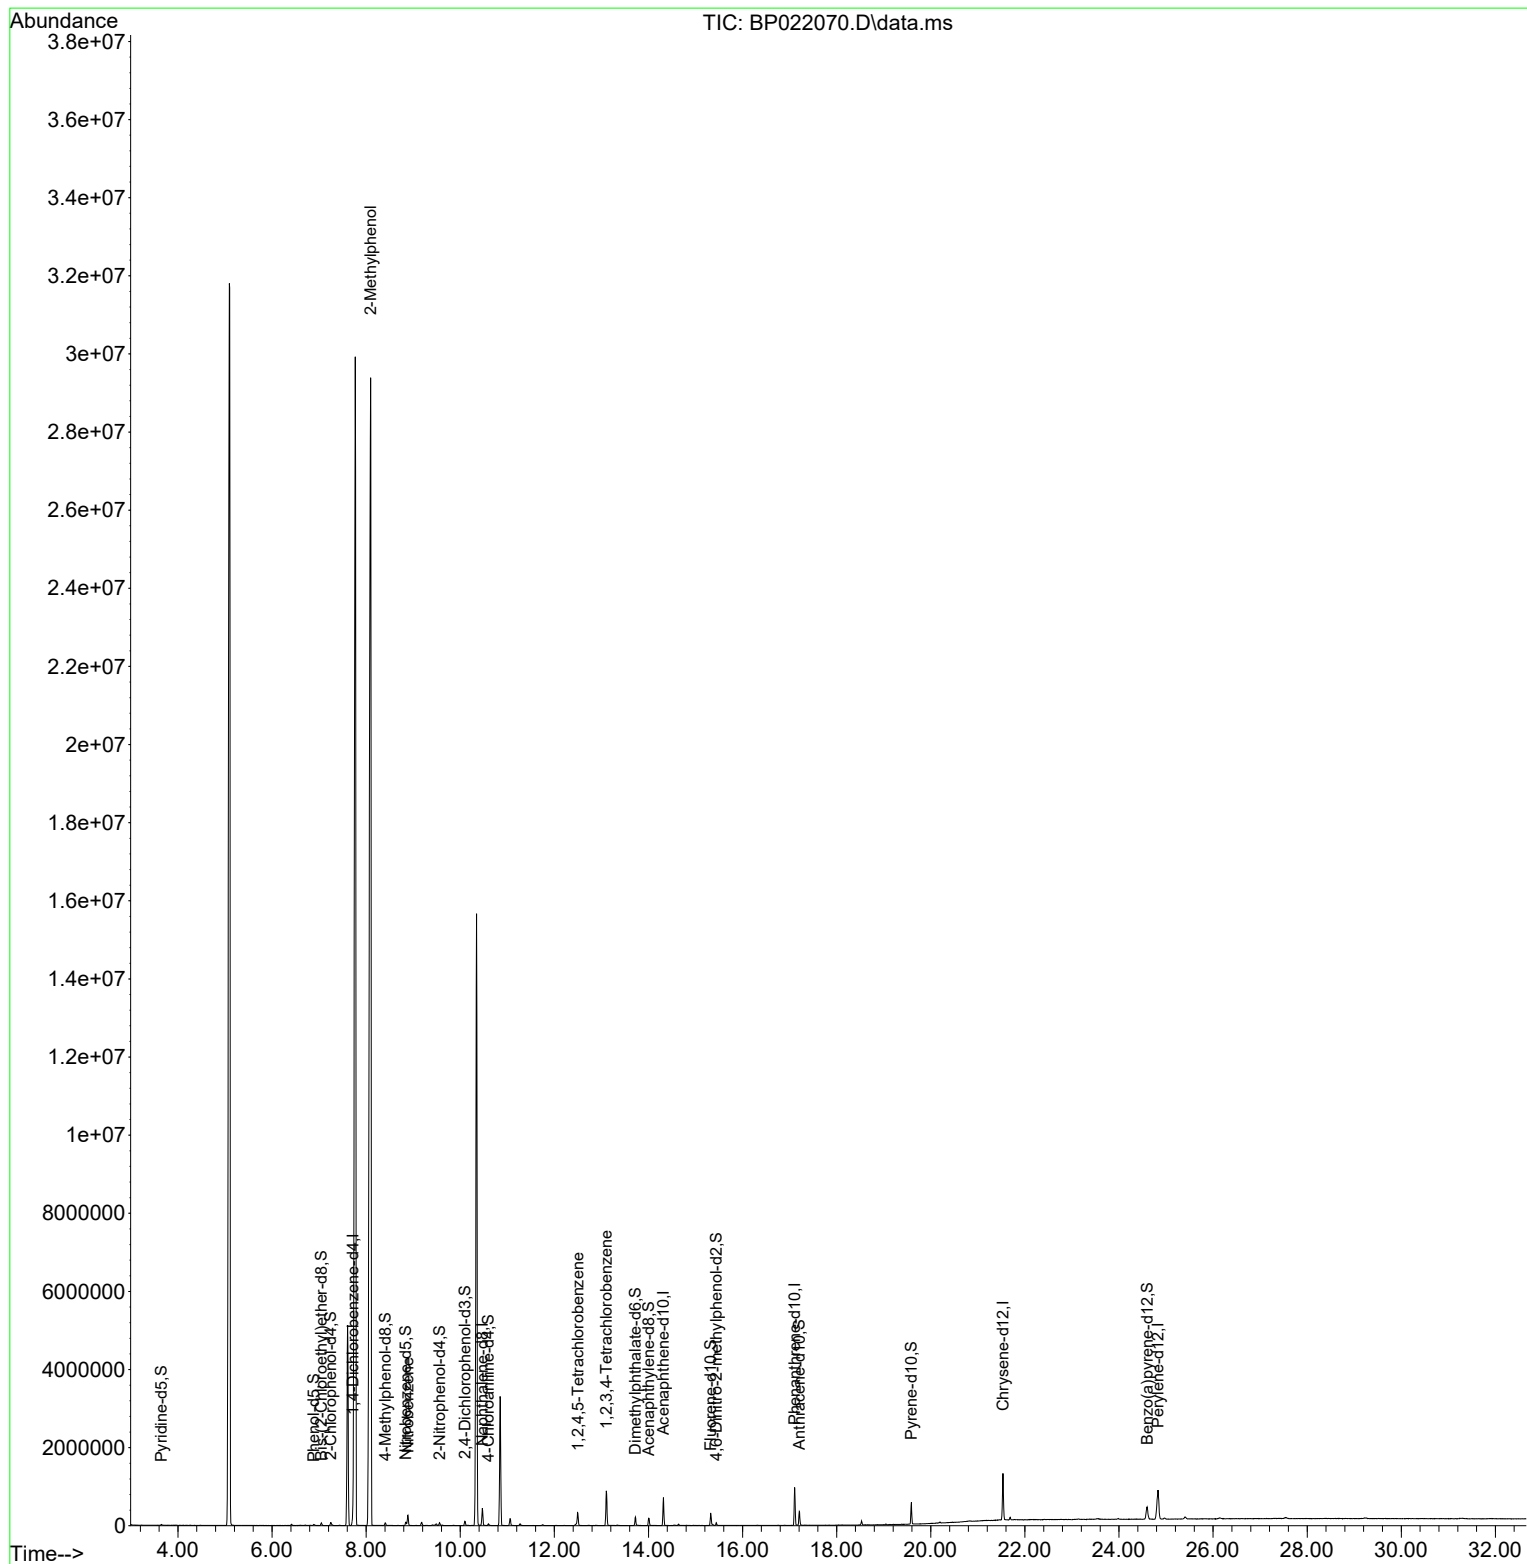

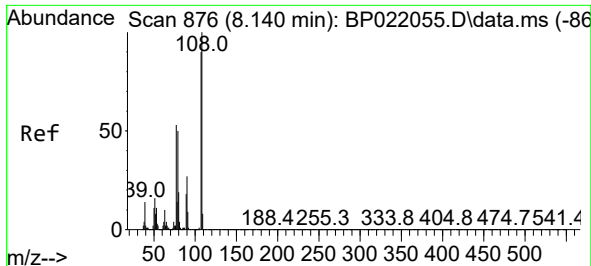

#13

2-Methylphenol

Concen: 28.867 ng/ul

RT: 8.093 min Scan# 8

Delta R.T. -0.053 min

Lab File: BP022070.D

Acq: 26 Sep 2024 19:57

Instrument :

BNA_P

ClientSampleId :





C0SX9DL

Tgt Ion:108 Resp: 164443

Ion Ratio Lower Upper

108 100

107 96.0 71.3 106.9

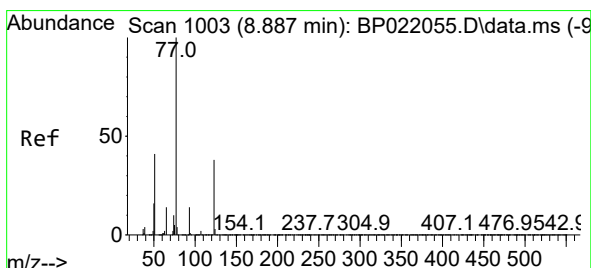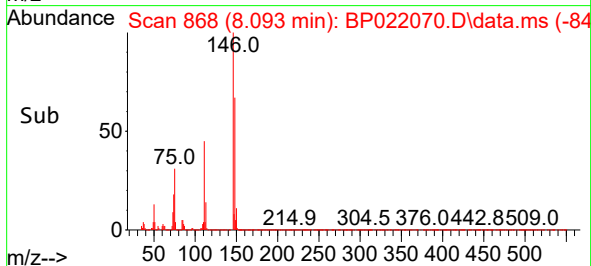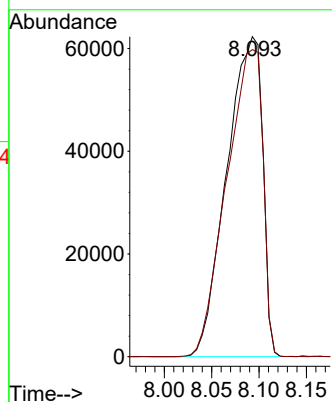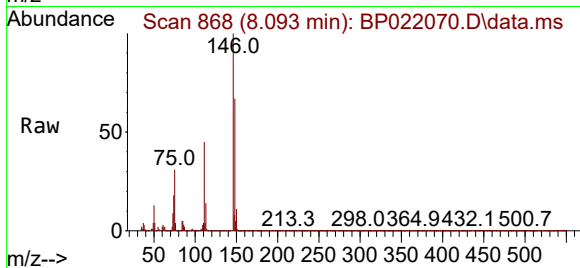

#22

Nitrobenzene

Concen: 20.721 ng/ul

RT: 8.887 min Scan# 1003

Delta R.T. 0.000 min

Lab File: BP022070.D

Acq: 26 Sep 2024 19:57




Tgt Ion: 77 Resp: 145050


Ion Ratio Lower Upper

77 100

123 36.2 29.8 44.8

65 13.9 11.3 16.9

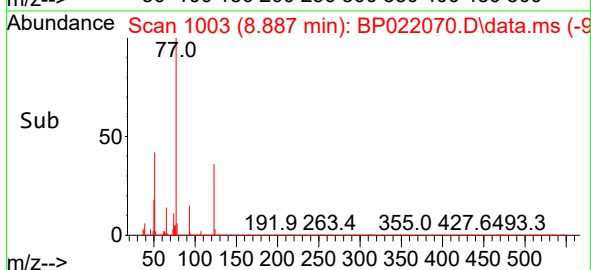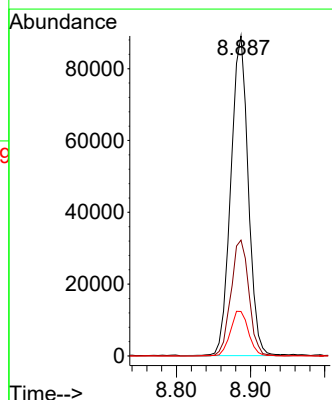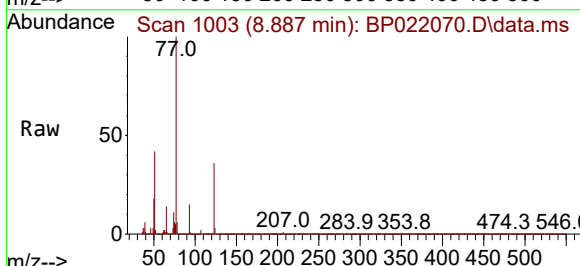

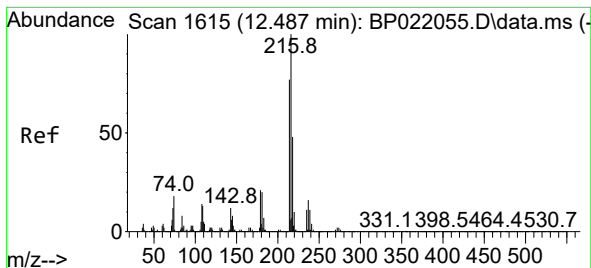

#39

1,2,4,5-Tetrachlorobenzene

Concen: 14.365 ng/ul

RT: 12.499 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP022070.D

Acq: 26 Sep 2024 19:57

Instrument :

BNA_P

ClientSampleId :

C0SX9DL

Tgt Ion:216 Resp: 123080





Ion Ratio Lower Upper

216 100

214 75.1 62.8 94.2

179 20.9 17.9 26.9

108 13.6 14.1 21.1#

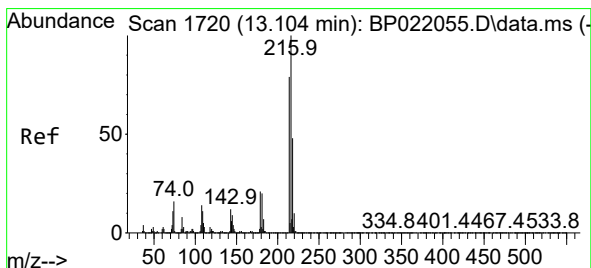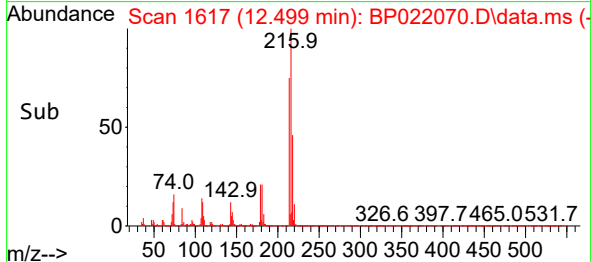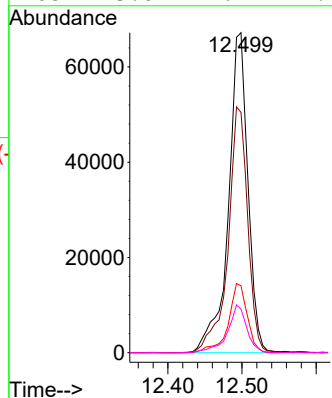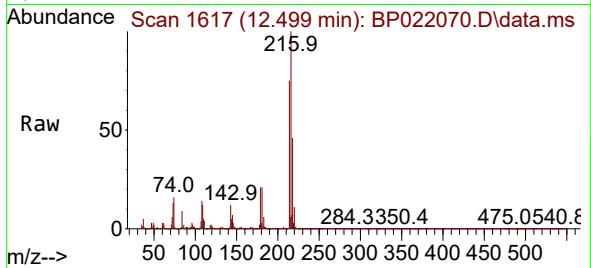

#75

1,2,3,4-Tetrachlorobenzene

Concen: 32.687 ng/uL

RT: 13.104 min Scan# 1720

Delta R.T. -0.012 min

Lab File: BP022070.D

Acq: 26 Sep 2024 19:57

Tgt Ion:216 Resp: 293652

Ion Ratio Lower Upper

216 100

214 76.4 60.6 90.8

218 47.7 38.1 57.1

