




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022005.D
Acq On : 24 Sep 2024 21:45
Operator : RC/JU
Sample : P4092-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B37

Manual IntegrationsAPPROVED

Quant Time: Sep 24 23:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/28/2024

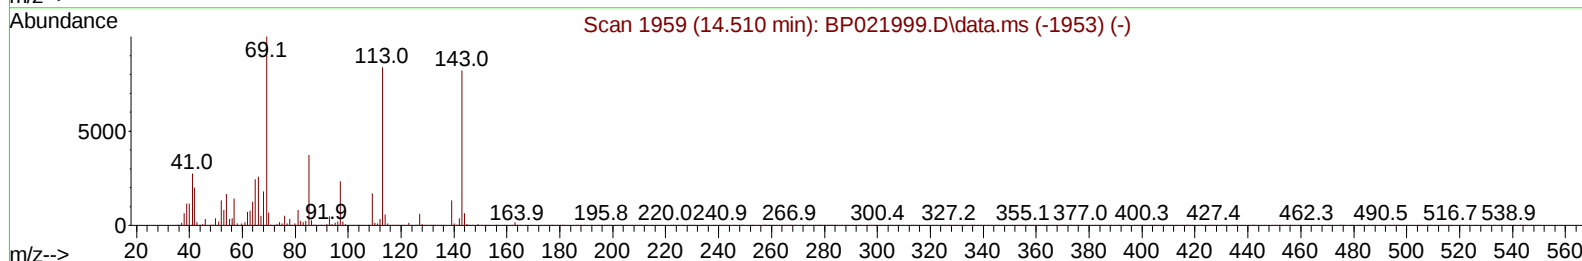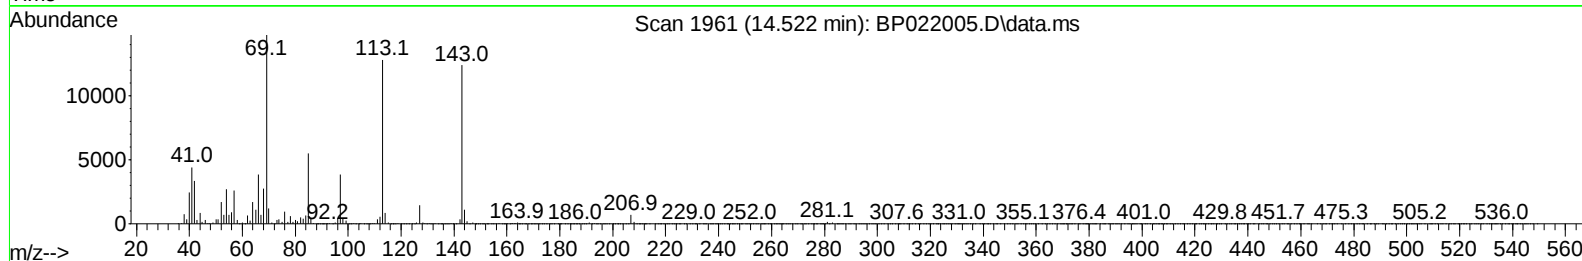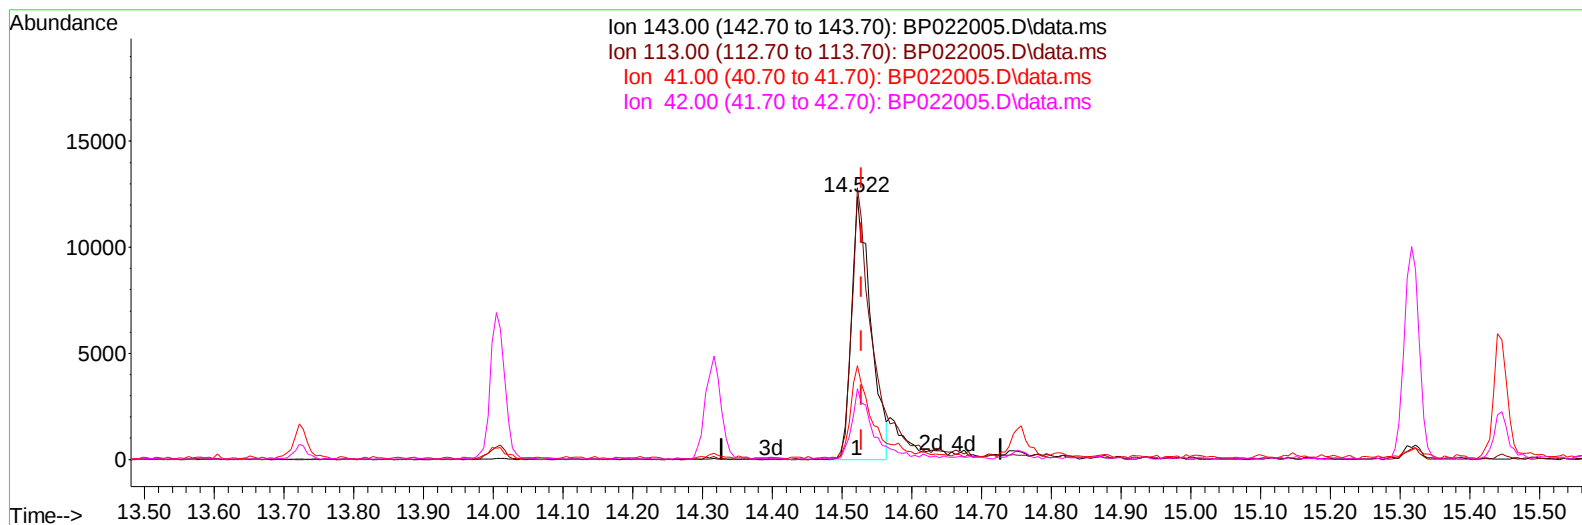

TIC: BP022005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (-0.006) 6.83 ng/u1

response 23671

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.70	103.37
41.00	35.80	35.61
42.00	26.20	26.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022005.D
 Acq On : 24 Sep 2024 21:45
 Operator : RC/JU
 Sample : P4092-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B37

Manual IntegrationsAPPROVED

Quant Time: Sep 24 23:32:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/28/2024

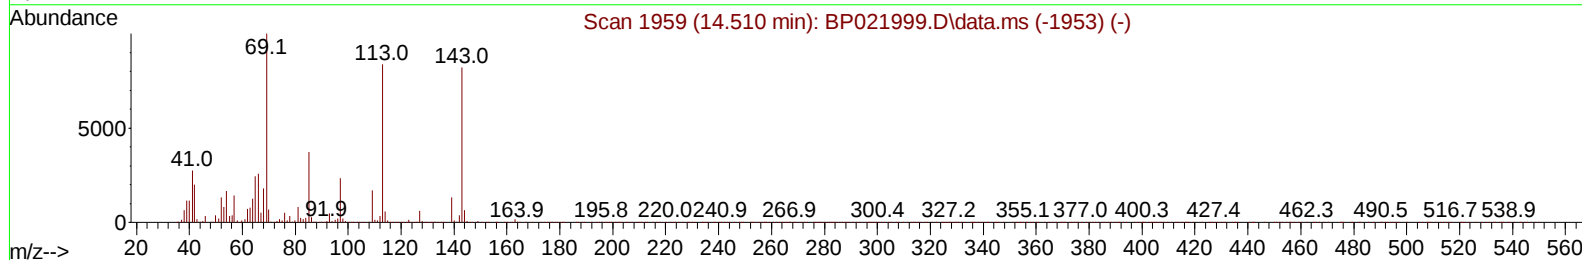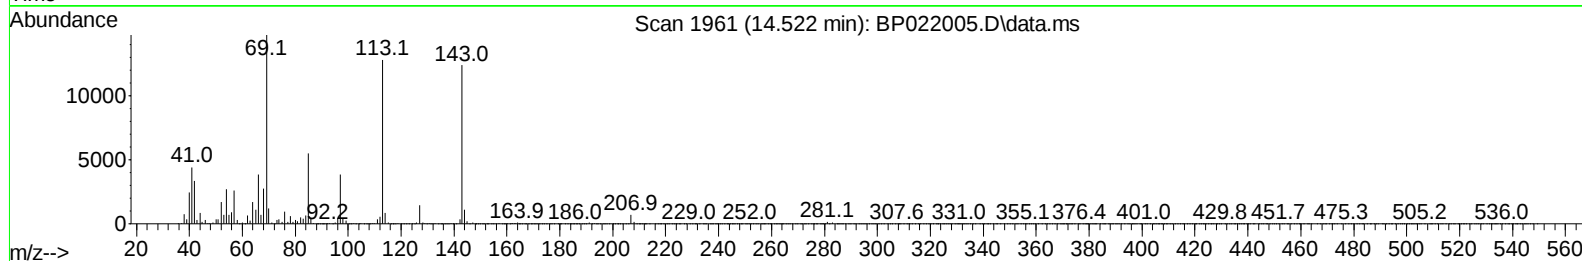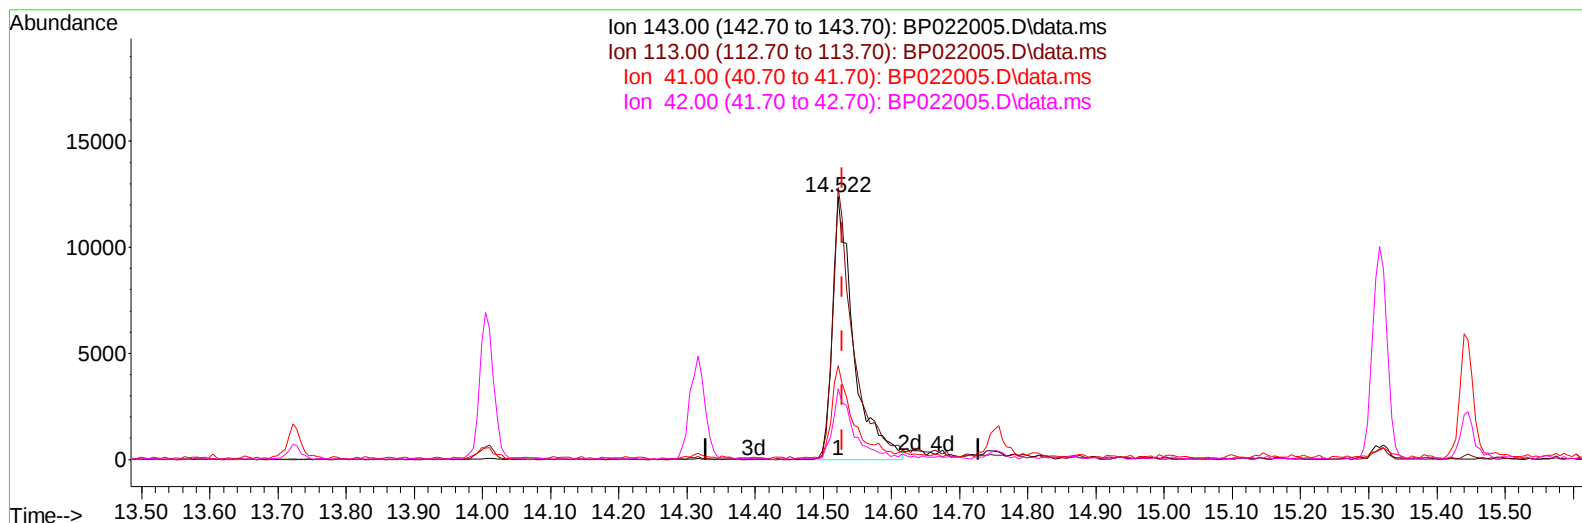

TIC: BP022005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (-0.006) 7.76 ng/u1 m

response 26880

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.70	103.37
41.00	35.80	35.61
42.00	26.20	26.99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022005.D
 Acq On : 24 Sep 2024 21:45
 Operator : RC/JU
 Sample : P4092-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B37

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 24 23:50:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	88176	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	338392	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	262013	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	638578	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	792281	20.000	ng/ul	0.00
88) Perylene-d12	24.821	264	944667	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	11883	5.279	ng/uL	0.00
4) Pyridine-d5	3.640	84	71340	11.087	ng/ul	0.00
7) Phenol-d5	6.893	99	66607	9.234	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	156353	35.203	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	168859	32.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.405	113	123648	21.634	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	91425	36.097	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	109972	38.295	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	217427	34.864	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	220160	29.587	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	783268	38.672	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	796431	37.140	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	26880m	7.759	ng/ul	0.00
60) Fluorene-d10	15.316	176	678346	37.863	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	133188	33.594	ng/ul	0.00
73) Anthracene-d10	17.216	188	1149479	38.558	ng/ul	0.00
81) Pyrene-d10	19.586	212	1588934	38.711	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.592	264	1985798	39.967	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.264	88	2663	1.092	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022005.D
Acq On : 24 Sep 2024 21:45
Operator : RC/JU
Sample : P4092-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B37

Manual IntegrationsAPPROVED

Quant Time: Sep 24 23:50:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/28/2024

