




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022044.D
Acq On : 26 Sep 2024 02:17
Operator : RC/JU
Sample : P4084-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYM4

Manual IntegrationsAPPROVED

Quant Time: Sep 26 03:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/26/2024
Supervised By :mohammad ahmed 09/28/2024

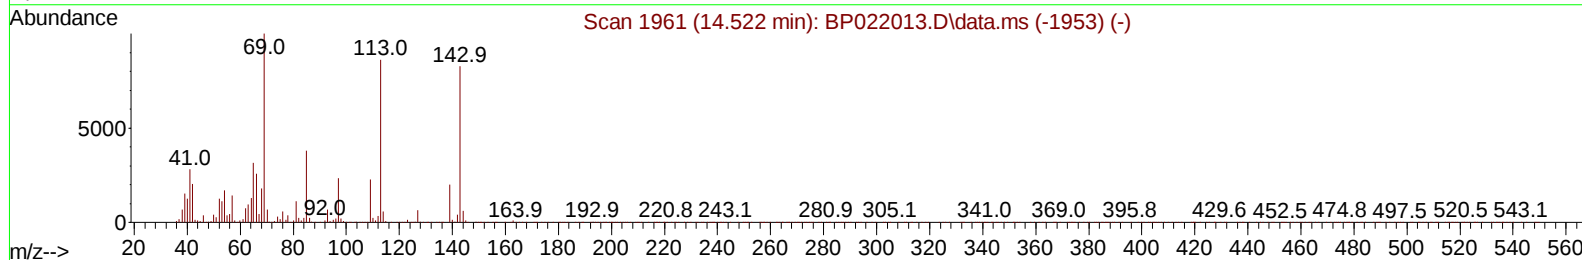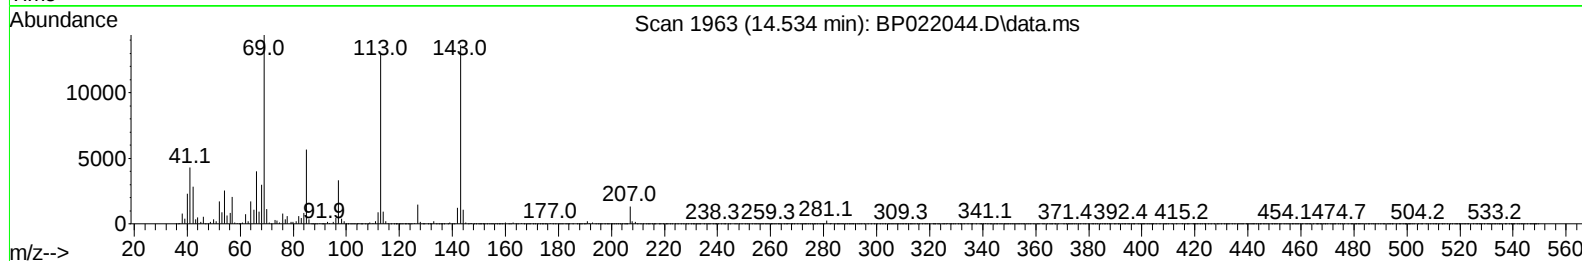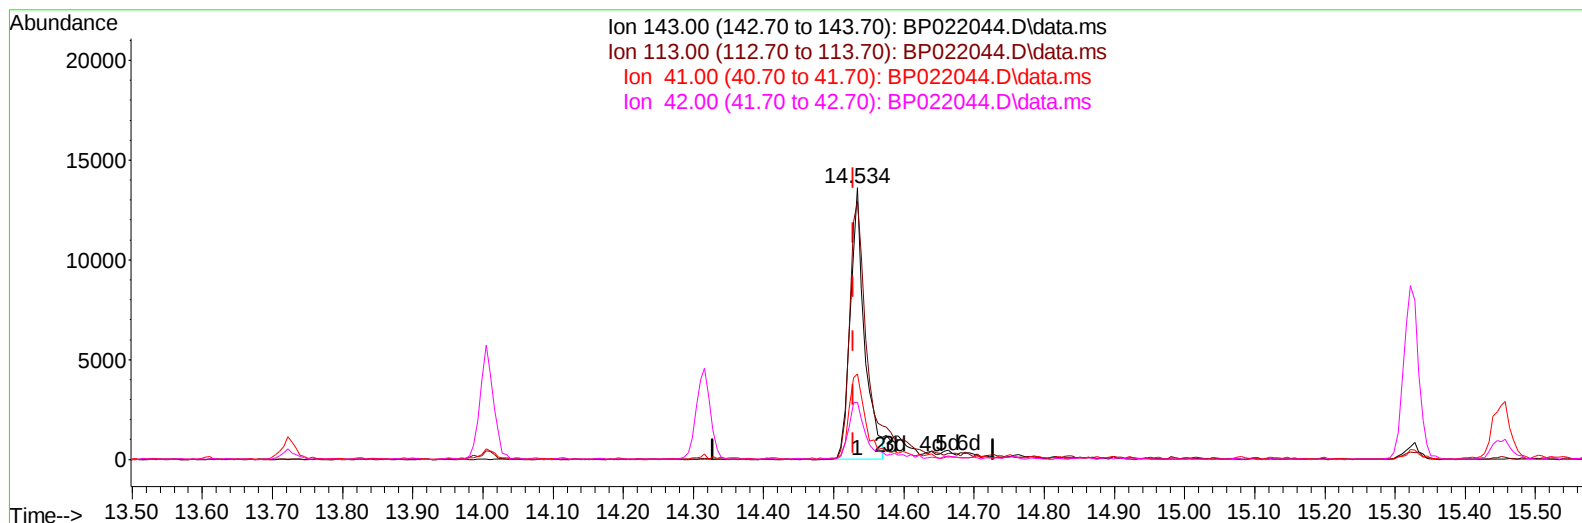

TIC: BP022044.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (+ 0.006) 7.51 ng/u1

response 19357

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.70	95.16
41.00	35.80	31.43
42.00	26.20	21.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022044.D
 Acq On : 26 Sep 2024 02:17
 Operator : RC/JU
 Sample : P4084-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYM4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/26/2024
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 26 03:22:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	67292	20.000	ng/ul	0.00
20) Naphthalene-d8	10.463	136	249404	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	195039	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	482522	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.539	240	562747	20.000	ng/ul	# 0.00
88) Perylene-d12	24.827	264	683759	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8761	5.100	ng/uL	0.00
4) Pyridine-d5	3.640	84	25529	5.199	ng/ul	0.00
7) Phenol-d5	6.887	99	55494	10.081	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	109279	32.240	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	125143	31.422	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	95137	21.811	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	64743	34.683	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	73206	34.587	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.093	165	153045	33.296	ng/ul	0.00
31) 4-Chloroaniline-d4	10.599	131	124103	22.629	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	573946	38.068	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	531448	33.294	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143	21995m	8.529	ng/ul	0.00
60) Fluorene-d10	15.322	176	491597	36.862	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	90832	30.321	ng/ul	0.00
73) Anthracene-d10	17.216	188	940403	41.747	ng/ul	0.00
81) Pyrene-d10	19.586	212	1232652	42.280	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.604	264	1488814	41.398	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022044.D
Acq On : 26 Sep 2024 02:17
Operator : RC/JU
Sample : P4084-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYM4

Manual IntegrationsAPPROVED

Quant Time: Sep 26 03:22:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/26/2024
Supervised By :mohammad ahmed 09/28/2024

