

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022051.D
 Acq On : 26 Sep 2024 07:02
 Operator : RC/JU
 Sample : P4107-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B30

Quant Time: Sep 26 07:40:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	103586	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	371622	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.316	164	281925	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.104	188	699996	20.000	ng/u1	-0.01
79) Chrysene-d12	21.539	240	837262	20.000	ng/u1	0.00
88) Perylene-d12	24.821	264	981285	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	11100	4.197	ng/uL	0.00
4) Pyridine-d5	3.640	84	61651	8.156	ng/u1	0.00
7) Phenol-d5	6.887	99	66226	7.816	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	140168	26.864	ng/u1	0.00
11) 2-Chlorophenol-d4	7.246	132	164749	26.873	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	126754	18.878	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	82619	29.703	ng/u1	0.00
24) 2-Nitrophenol-d4	9.552	143	94723	30.035	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.093	165	200071	29.212	ng/u1	0.00
31) 4-Chloroaniline-d4	10.599	131	239189	29.270	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	686452	31.499	ng/u1	0.00
49) Acenaphthylene-d8	13.998	160	665704	28.851	ng/u1	0.00
54) 4-Nitrophenol-d4	14.528	143	23498	6.304	ng/u1	0.00
60) Fluorene-d10	15.322	176	582132	30.198	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	114013	26.235	ng/u1	-0.01
73) Anthracene-d10	17.204	188	1023214	31.311	ng/u1	-0.01
81) Pyrene-d10	19.592	212	1353714	31.208	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.604	264	1616310	31.316	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.258	88	2912	1.017 ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022051.D
Acq On : 26 Sep 2024 07:02
Operator : RC/JU
Sample : P4107-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B30


Quant Time: Sep 26 07:40:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

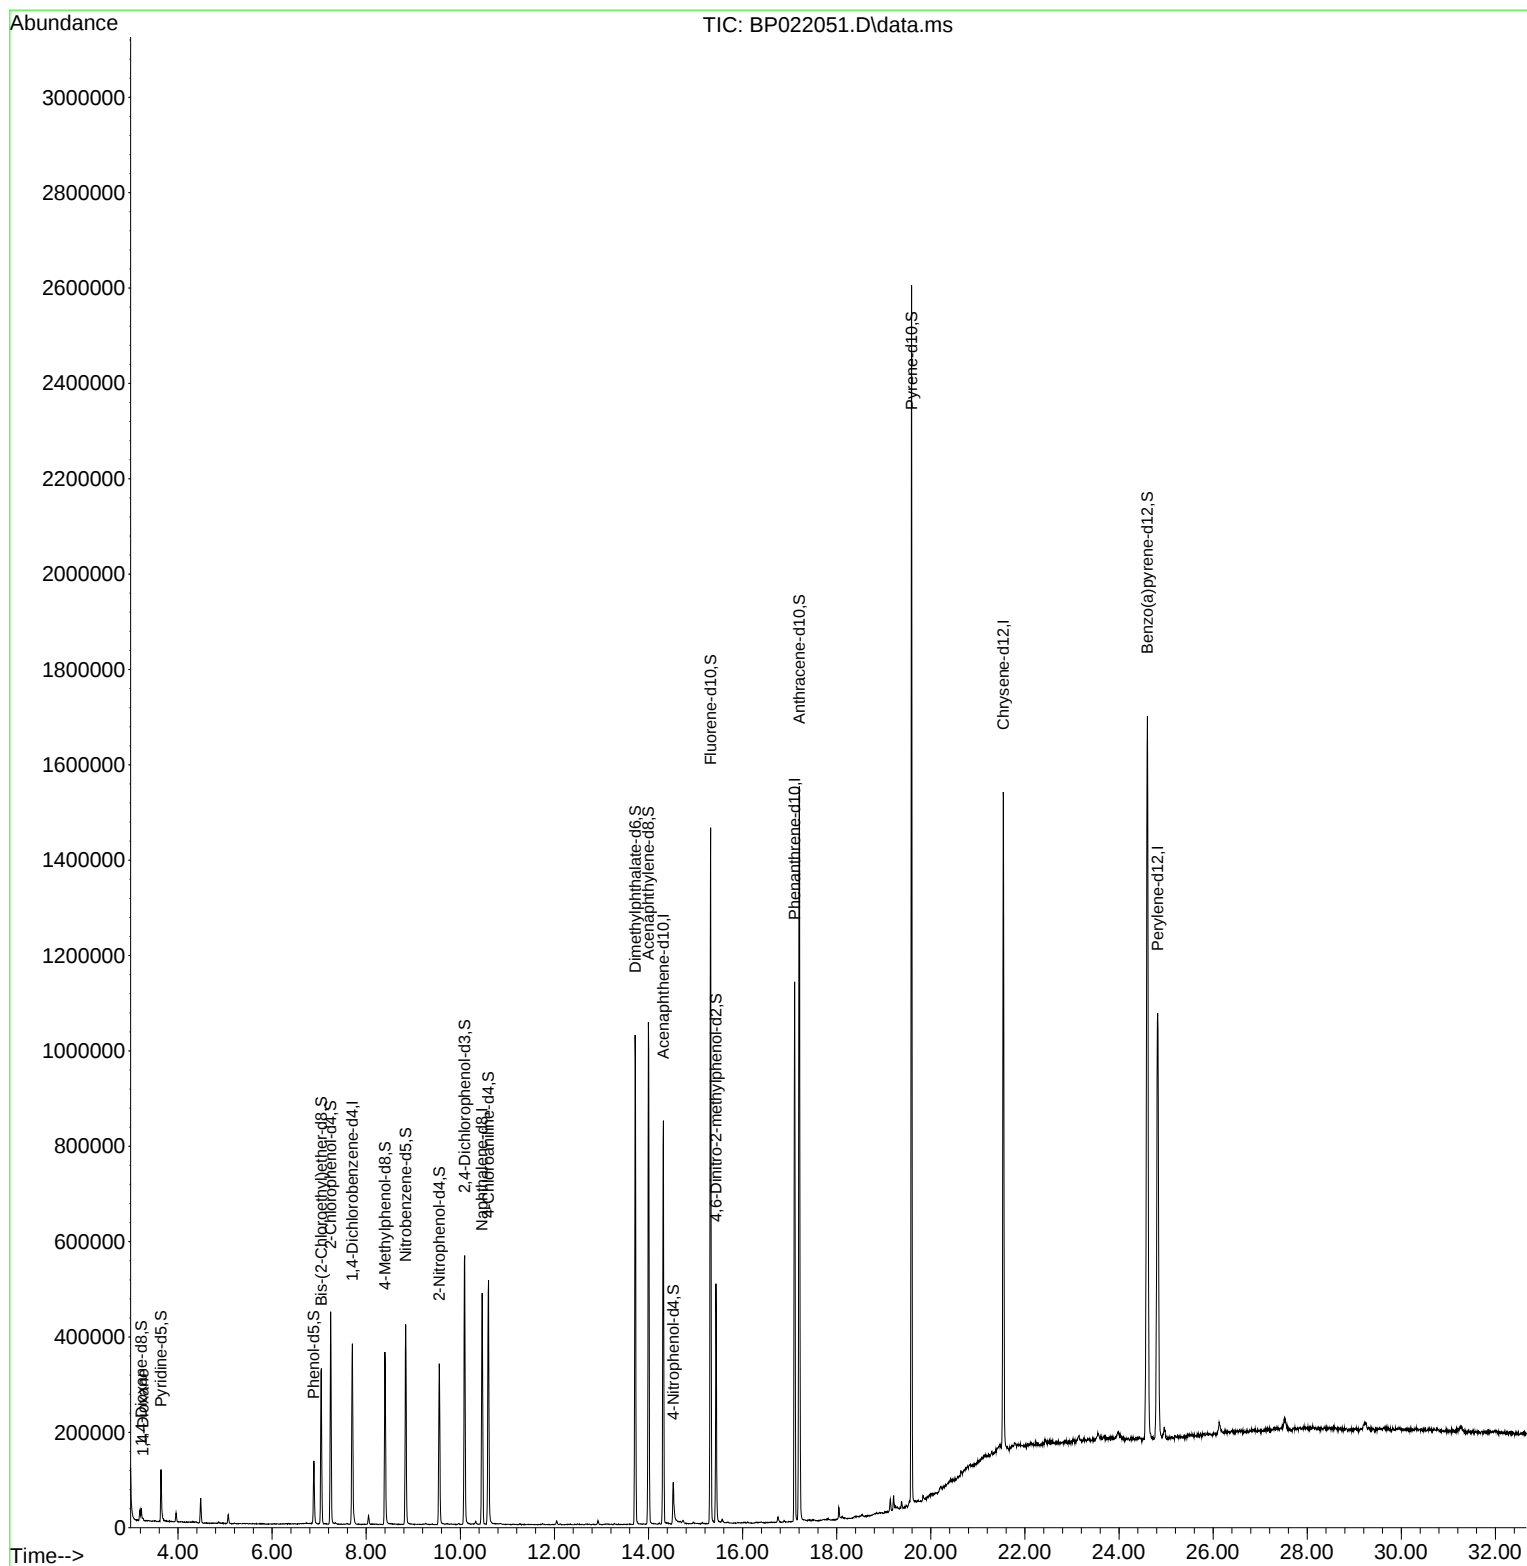

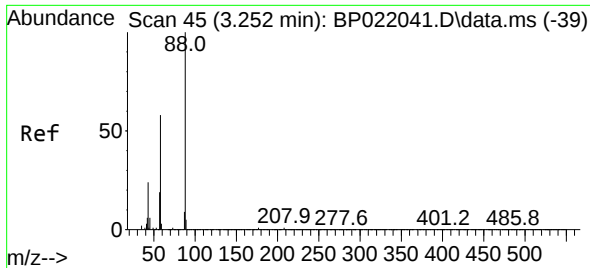

#2
 1,4-Dioxane
 Concen: 1.017 ng/uL
 RT: 3.258 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP022051.D
 Acq: 26 Sep 2024 07:02

Instrument :
 BNA_P
 ClientSampleId :
 C0B30

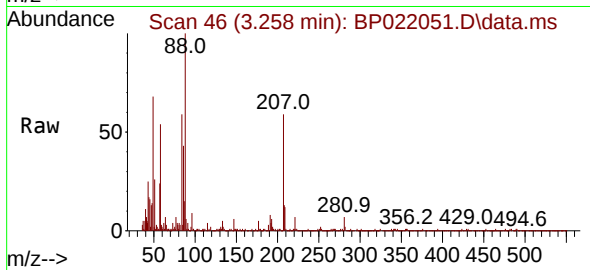

Tgt Ion: 88 Resp: 2912

Ion	Ratio	Lower	Upper
88	100		
43	25.1	22.1	33.1
58	54.1	49.3	73.9

