

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP021997.D
 Acq On : 24 Sep 2024 16:18
 Operator : RC/JU
 Sample : PB163502BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	31	36	41	rBV	27817	36680	1.04%	0.106%
2	3.605	101	105	121	rBV	370110	561752	15.88%	1.624%
3	3.928	156	160	164	rBV2	8184	11051	0.31%	0.032%
4	6.834	646	654	671	rBV	462133	713440	20.17%	2.062%
5	6.999	676	682	693	rVB	344734	531956	15.04%	1.537%
6	7.087	693	697	707	rVB3	5156	8904	0.25%	0.026%
7	7.193	707	715	726	rBV	445500	717238	20.28%	2.073%
8	7.663	787	795	805	rBV	422266	735891	20.80%	2.127%
9	8.005	849	853	856	rBV5	2337	3798	0.11%	0.011%
10	8.105	864	870	877	rBV5	7169	12081	0.34%	0.035%
11	8.175	877	882	888	rBV6	5958	9588	0.27%	0.028%
12	8.358	906	913	921	rBV	494073	853812	24.14%	2.468%
13	8.463	928	931	943	rVB4	12270	22405	0.63%	0.065%
14	8.728	971	976	981	rBV9	6440	10490	0.30%	0.030%
15	8.799	981	988	1001	rBV	437125	708950	20.04%	2.049%
16	9.369	1080	1085	1091	rBV2	8476	13046	0.37%	0.038%
17	9.510	1101	1109	1120	rBV	345279	593919	16.79%	1.716%
18	9.605	1122	1125	1134	rVB4	8593	15981	0.45%	0.046%
19	9.846	1161	1166	1173	rVB3	6494	10199	0.29%	0.029%
20	10.063	1193	1203	1213	rBV	541752	940216	26.58%	2.717%
21	10.293	1236	1242	1249	rVB9	2707	5990	0.17%	0.017%
22	10.434	1258	1266	1273	rBV	545716	978662	27.67%	2.828%
23	10.557	1280	1287	1307	rBV	540200	907392	25.65%	2.622%
24	10.775	1318	1324	1329	rVB5	11286	18196	0.51%	0.053%
25	11.399	1426	1430	1433	rBV6	2637	4379	0.12%	0.013%
26	11.728	1480	1486	1494	rVB9	4717	11551	0.33%	0.033%
27	12.028	1532	1537	1543	rVB2	8535	14196	0.40%	0.041%
28	12.093	1543	1548	1555	rBV2	11435	18208	0.51%	0.053%
29	12.328	1582	1588	1592	rBV	13183	21866	0.62%	0.063%
30	12.463	1603	1611	1622	rBV4	13842	30407	0.86%	0.088%
31	12.722	1648	1655	1660	rBV8	5982	11890	0.34%	0.034%
32	12.810	1663	1670	1675	rVV8	5235	10604	0.30%	0.031%
33	13.081	1711	1716	1720	rBV	14752	22467	0.64%	0.065%
34	13.128	1720	1724	1726	rVV	12459	21239	0.60%	0.061%
35	13.151	1726	1728	1738	rVB2	13531	22153	0.63%	0.064%
36	13.369	1760	1765	1777	rVB2	3156	9438	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP021997.D
 Acq On : 24 Sep 2024 16:18
 Operator : RC/JU
 Sample : PB163502BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	13.710	1815	1823	1828	rBV	1126600	1637996	46.30%	4.734%
38	13.757	1828	1831	1835	rVV2	17059	24644	0.70%	0.071%
39	13.822	1839	1842	1846	rVV6	3100	4434	0.13%	0.013%
40	13.869	1846	1850	1855	rVB4	8063	11014	0.31%	0.032%
41	13.993	1860	1871	1883	rBV	1163535	1745470	49.34%	5.045%
42	14.210	1903	1908	1914	rBV7	3884	7473	0.21%	0.022%
43	14.304	1917	1924	1930	rVV	1176110	1505954	42.57%	4.352%
44	14.363	1930	1934	1939	rVB	18643	26498	0.75%	0.077%
45	14.522	1954	1961	1970	rBV	515446	753596	21.30%	2.178%
46	14.628	1975	1979	1983	rVV2	27035	42477	1.20%	0.123%
47	14.693	1983	1990	1999	rVB3	16282	50429	1.43%	0.146%
48	14.869	2015	2020	2025	rBV6	5384	7457	0.21%	0.022%
49	14.945	2027	2033	2039	rBV7	8804	15330	0.43%	0.044%
50	15.151	2063	2068	2074	rBV	16690	25712	0.73%	0.074%
51	15.310	2086	2095	2101	rBV	1484079	2305162	65.16%	6.662%
52	15.363	2101	2104	2109	rVV2	40061	67221	1.90%	0.194%
53	15.428	2109	2115	2133	rVV	415563	733737	20.74%	2.121%
54	15.563	2134	2138	2140	rVV4	9360	15555	0.44%	0.045%
55	15.592	2140	2143	2151	rVB	23975	29422	0.83%	0.085%
56	15.663	2151	2155	2158	rBV2	6558	7829	0.22%	0.023%
57	16.287	2256	2261	2268	rBV4	16859	26779	0.76%	0.077%
58	16.392	2275	2279	2284	rBV2	19752	28098	0.79%	0.081%
59	16.569	2306	2309	2313	rBV5	10572	13629	0.39%	0.039%
60	16.757	2335	2341	2346	rBV9	9145	18967	0.54%	0.055%
61	17.104	2394	2400	2407	rBV	1331543	1998298	56.49%	5.775%
62	17.216	2412	2419	2432	rVV2	1784388	2693409	76.14%	7.784%
63	17.534	2468	2473	2478	rVB3	8765	14623	0.41%	0.042%
64	18.122	2569	2573	2577	rBV	15846	21557	0.61%	0.062%
65	19.145	2744	2747	2753	rVB2	20223	27722	0.78%	0.080%
66	19.216	2756	2759	2761	rVV	29582	32367	0.91%	0.094%
67	19.245	2762	2764	2770	rVB2	26118	35900	1.01%	0.104%
68	19.592	2818	2823	2833	rBV	2441873	3439099	97.22%	9.939%
69	21.551	3149	3156	3162	rBV	1557395	2529581	71.51%	7.311%
70	24.610	3667	3676	3687	rBV2	1423998	3537536	100.00%	10.224%
71	24.839	3707	3715	3729	rVB	908514	2545970	71.97%	7.358%




Sum of corrected areas: 34600980

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP021997.D
Acq On : 24 Sep 2024 16:18
Operator : RC/JU
Sample : PB163502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

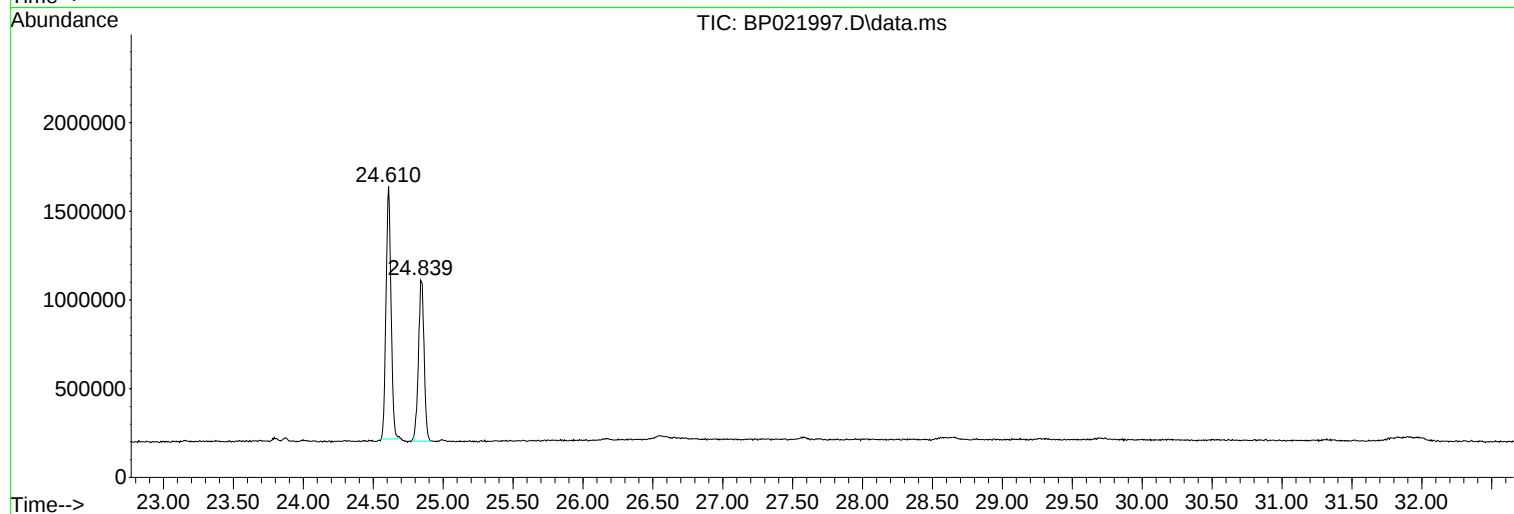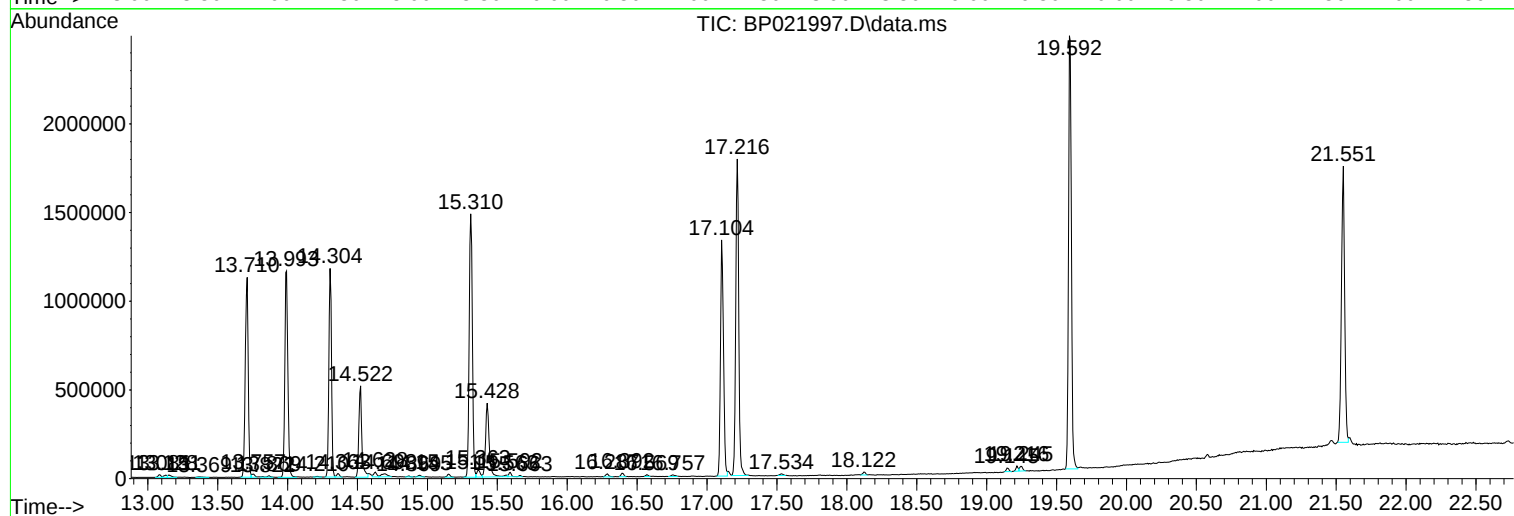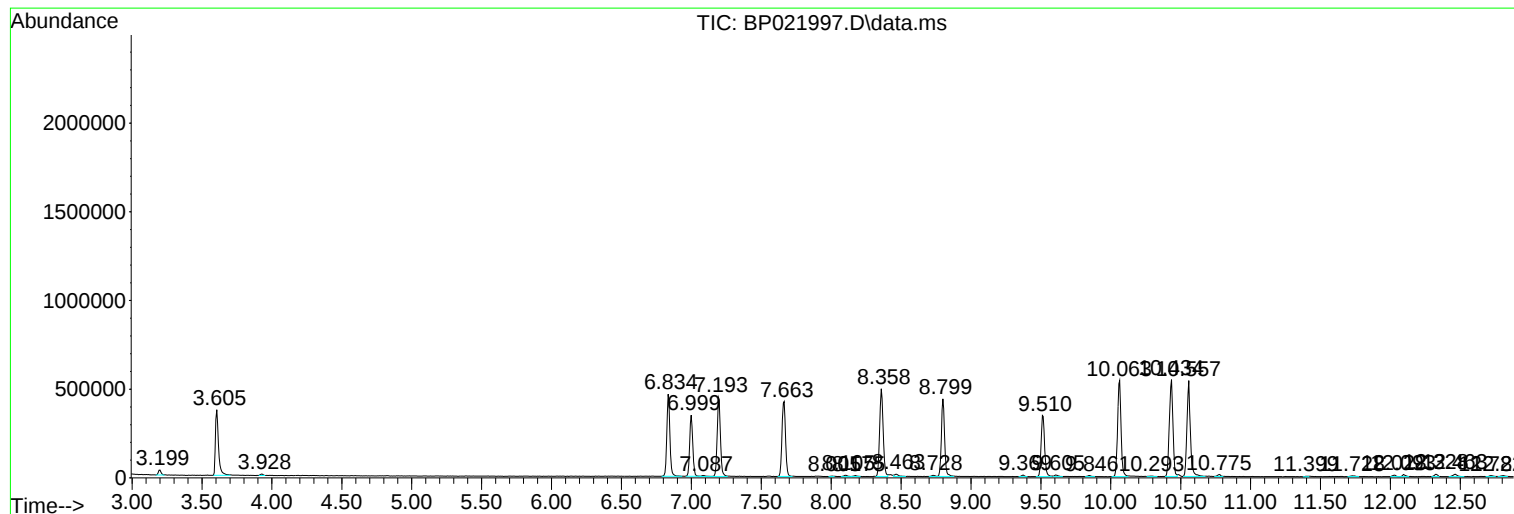

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP021997.D
Acq On : 24 Sep 2024 16:18
Operator : RC/JU
Sample : PB163502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP021997.D
Acq On : 24 Sep 2024 16:18
Operator : RC/JU
Sample : PB163502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------