

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022001.D
 Acq On : 24 Sep 2024 19:01
 Operator : RC/JU
 Sample : PB163472BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK472

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	44	rBV	23962	29967	1.05%	0.119%
2	3.634	106	110	126	rBV	285934	425165	14.90%	1.690%
3	3.964	162	166	169	rBV2	7628	11171	0.39%	0.044%
4	6.887	656	663	675	rBV	327214	533501	18.69%	2.121%
5	7.046	682	690	700	rBV	253610	393617	13.79%	1.565%
6	7.252	717	725	736	rBV	333298	551502	19.32%	2.192%
7	7.705	796	802	811	rVB	349885	556389	19.49%	2.212%
8	8.405	913	921	936	rBV	410096	653252	22.89%	2.597%
9	8.846	987	996	1009	rBV	316757	527082	18.47%	2.095%
10	9.563	1111	1118	1128	rBV	253209	430678	15.09%	1.712%
11	10.099	1199	1209	1224	rBV	413968	701076	24.56%	2.787%
12	10.475	1265	1273	1285	rVB	400402	697272	24.43%	2.772%
13	10.599	1286	1294	1308	rBV	365566	658912	23.08%	2.619%
14	12.057	1537	1542	1548	rBV2	5616	10930	0.38%	0.043%
15	12.634	1635	1640	1645	rBV3	19199	38500	1.35%	0.153%
16	12.698	1645	1651	1660	rVV2	52934	110807	3.88%	0.440%
17	13.116	1713	1722	1731	rBV7	14375	43029	1.51%	0.171%
18	13.234	1736	1742	1749	rVV2	12095	26099	0.91%	0.104%
19	13.310	1750	1755	1761	rVV	32647	56825	1.99%	0.226%
20	13.369	1761	1765	1775	rVB2	21245	46362	1.62%	0.184%
21	13.728	1818	1826	1838	rBV	715476	1146793	40.18%	4.559%
22	14.010	1866	1874	1885	rBV	789561	1190835	41.72%	4.734%
23	14.316	1918	1926	1933	rBV	666657	1000265	35.04%	3.976%
24	14.381	1933	1937	1942	rVB8	2478	3959	0.14%	0.016%
25	14.445	1942	1948	1952	rBV4	7090	17339	0.61%	0.069%
26	14.522	1955	1961	1978	rBV	328348	549216	19.24%	2.183%
27	14.734	1995	1997	2009	rVB	4086	8975	0.31%	0.036%
28	15.145	2063	2067	2075	rBV7	3256	5602	0.20%	0.022%
29	15.328	2089	2098	2105	rBV	984794	1595396	55.89%	6.342%
30	15.381	2105	2107	2113	rVV7	7561	11912	0.42%	0.047%
31	15.451	2113	2119	2131	rVV	363265	516661	18.10%	2.054%
32	15.569	2134	2139	2149	rVB6	7136	17464	0.61%	0.069%
33	16.281	2258	2260	2264	rVB5	2398	2921	0.10%	0.012%
34	16.557	2304	2307	2314	rBV8	1893	3836	0.13%	0.015%
35	16.792	2340	2347	2350	rVB9	2406	4696	0.16%	0.019%
36	16.898	2363	2365	2371	rVB6	3262	3902	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022001.D
Acq On : 24 Sep 2024 19:01
Operator : RC/JU
Sample : PB163472BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	17.122	2394	2403	2413	rBV	885568	1360710	47.67%	5.409%
38	17.216	2413	2419	2430	rVV	1427822	1895452	66.41%	7.535%
39	18.133	2571	2575	2579	rVB6	3600	5144	0.18%	0.020%
40	19.139	2742	2746	2752	rVB5	16724	26048	0.91%	0.104%
41	19.210	2755	2758	2763	rBV	14793	21912	0.77%	0.087%
42	19.592	2817	2823	2833	rBV	1840033	2435398	85.32%	9.682%
43	21.539	3148	3154	3167	rBV	1274430	1924925	67.44%	7.652%
44	24.598	3664	3674	3686	rVB	1089456	2854347	100.00%	11.347%
45	24.810	3702	3710	3725	rVB	794536	2049267	71.79%	8.147%




Sum of corrected areas: 25155111

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022001.D
Acq On : 24 Sep 2024 19:01
Operator : RC/JU
Sample : PB163472BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

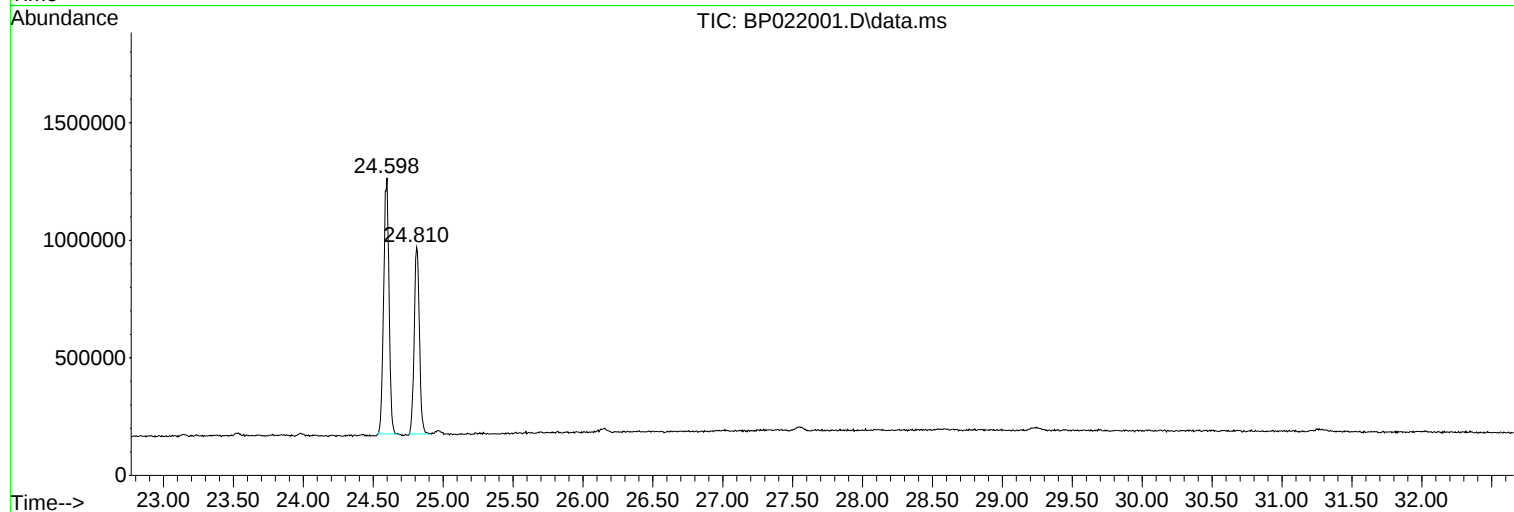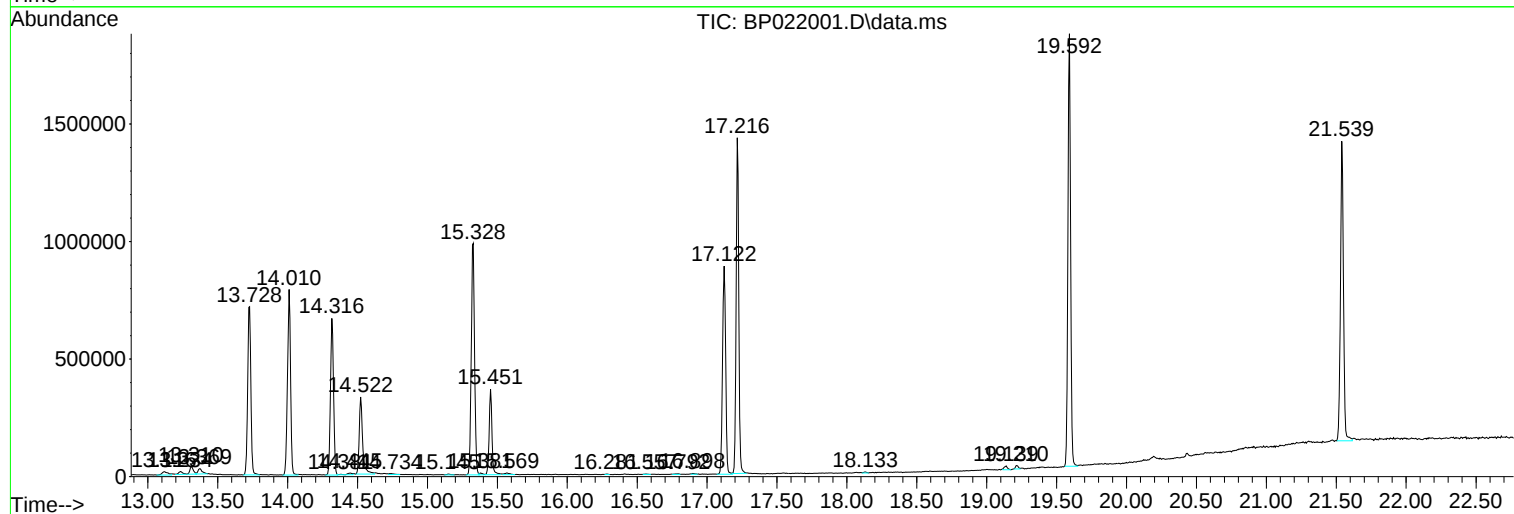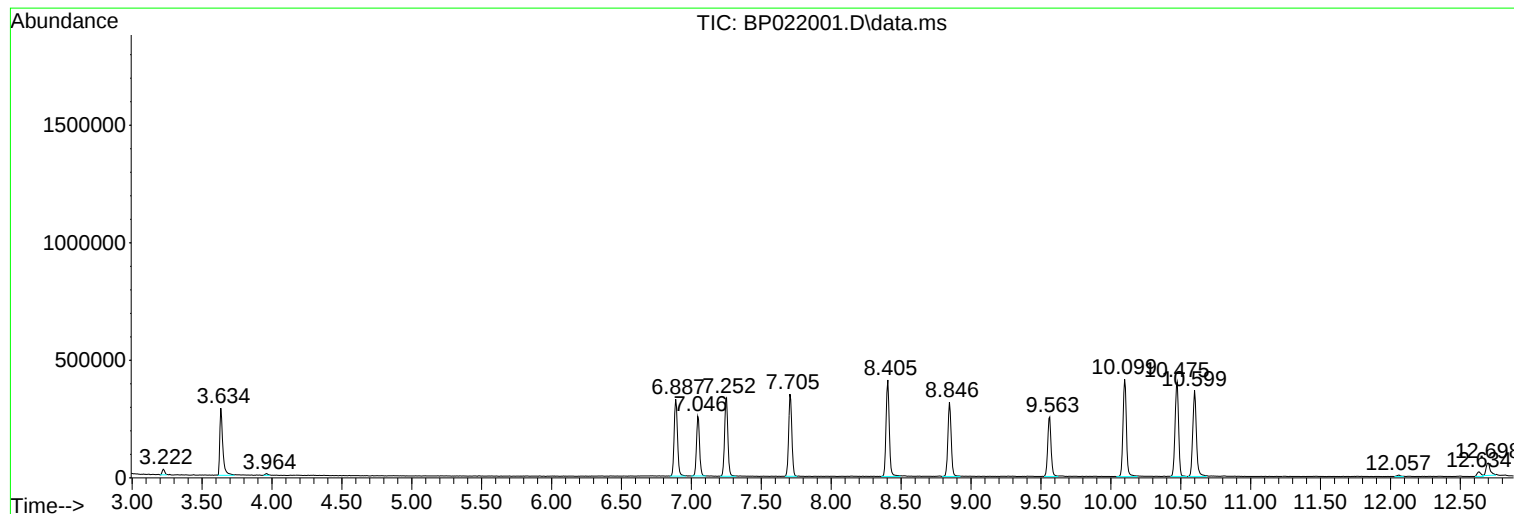

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022001.D
Acq On : 24 Sep 2024 19:01
Operator : RC/JU
Sample : PB163472BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 2,4-diisocyanato-1... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.698	2.22 ng/ul	110807	Acenaphthene-d10	14.316

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 2,4-diisocyanato-1-methyl-	174	C9H6N2O2	000584-84-9	97
2			Benzene, 2,4-diisocyanato-1-methyl-	174	C9H6N2O2	000584-84-9	97
3			Benzene, 2,4-diisocyanato-1-methyl-	174	C9H6N2O2	000584-84-9	95
4			Benzene, 2,4-diisocyanato-1-methyl-	174	C9H6N2O2	000584-84-9	93
5			Benzene, 2,4-diisocyanato-1-methyl-	174	C9H6N2O2	000584-84-9	93

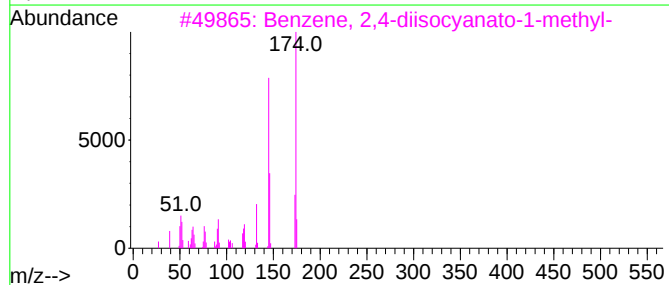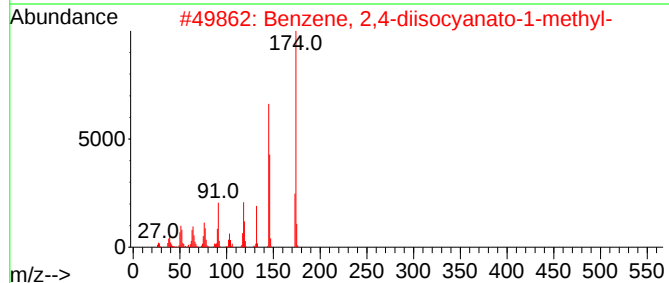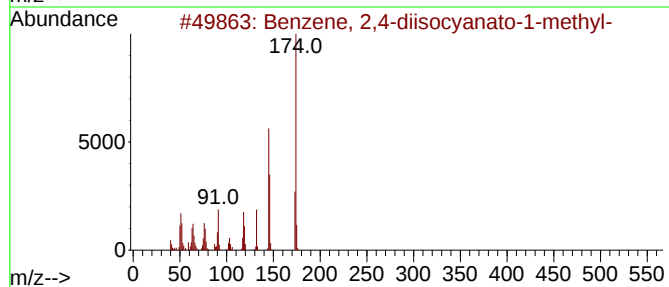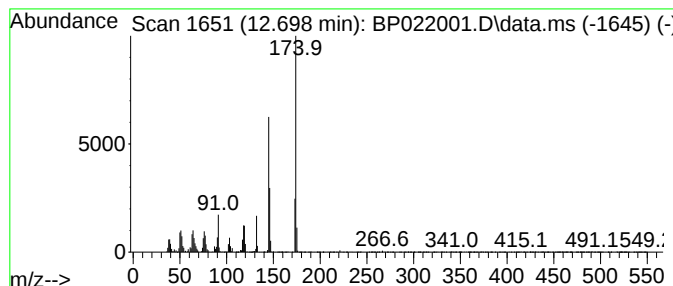

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022001.D
Acq On : 24 Sep 2024 19:01
Operator : RC/JU
Sample : PB163472BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 2,4-di...	12.698	2.2	ng/u1	110807	3	14.316	1000270	20.0