

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022008.D
 Acq On : 24 Sep 2024 23:47
 Operator : RC/JU
 Sample : P4092-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	45	rBV2	352136	527286	11.85%	1.448%
2	3.499	85	87	97	rVB10	3165	7194	0.16%	0.020%
3	3.640	107	111	126	rBV	101945	149648	3.36%	0.411%
4	3.964	162	166	170	rVB2	9873	12540	0.28%	0.034%
5	4.487	249	255	263	rVB	114031	161044	3.62%	0.442%
6	4.869	314	320	323	rBV4	3185	5488	0.12%	0.015%
7	5.264	383	387	392	rVB5	3735	5576	0.13%	0.015%
8	5.399	405	410	418	rBV3	9045	18162	0.41%	0.050%
9	5.758	467	471	476	rVB	8900	12391	0.28%	0.034%
10	6.705	626	632	641	rBV	163905	259315	5.83%	0.712%
11	6.893	656	664	671	rBV	137772	226088	5.08%	0.621%
12	7.052	683	691	700	rBV	387850	644522	14.49%	1.770%
13	7.252	717	725	734	rBV	499029	784201	17.63%	2.154%
14	7.369	737	745	751	rVB4	7860	18113	0.41%	0.050%
15	7.711	797	803	812	rBV	403482	664231	14.93%	1.824%
16	7.822	818	822	827	rVB2	6540	9493	0.21%	0.026%
17	8.340	906	910	914	rBV6	4186	6478	0.15%	0.018%
18	8.405	914	921	932	rVV	391159	651490	14.64%	1.789%
19	8.499	935	937	946	rVB10	2422	5697	0.13%	0.016%
20	8.846	989	996	1011	rVB	493176	866549	19.48%	2.380%
21	9.281	1062	1070	1073	rBV8	2949	5673	0.13%	0.016%
22	9.563	1108	1118	1126	rBV	439434	749068	16.84%	2.057%
23	9.793	1153	1157	1164	rBV10	2269	4563	0.10%	0.013%
24	10.093	1200	1208	1219	rBV	707899	1173343	26.37%	3.223%
25	10.469	1264	1272	1281	rVB	507241	890289	20.01%	2.445%
26	10.604	1286	1295	1306	rBV	518123	846083	19.02%	2.324%
27	11.269	1402	1408	1412	rBV9	2639	6105	0.14%	0.017%
28	11.757	1486	1491	1496	rVB9	2560	5581	0.13%	0.015%
29	12.051	1536	1541	1550	rVB4	9235	19104	0.43%	0.052%
30	13.722	1818	1825	1838	rBV	1383924	1864306	41.91%	5.120%
31	14.010	1865	1874	1883	rBV	1343380	2027831	45.58%	5.569%
32	14.322	1920	1927	1937	rBV	963045	1366231	30.71%	3.752%
33	14.534	1956	1963	1979	rBV	85891	213059	4.79%	0.585%
34	14.757	1994	2001	2007	rBV	74264	123145	2.77%	0.338%
35	15.145	2062	2067	2073	rVB10	4355	7707	0.17%	0.021%
36	15.328	2090	2098	2108	rBV	2030085	2704814	60.80%	7.429%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022008.D
 Acq On : 24 Sep 2024 23:47
 Operator : RC/JU
 Sample : P4092-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.440	2111	2117	2128	rVV	666819	845457	19.00%	2.322%
38	15.569	2134	2139	2147	rVB3	8201	15194	0.34%	0.042%
39	15.704	2157	2162	2167	rVB	21646	28687	0.64%	0.079%
40	15.904	2192	2196	2202	rVB9	2790	5675	0.13%	0.016%
41	15.969	2202	2207	2208	rBV5	3229	4581	0.10%	0.013%
42	16.116	2230	2232	2237	rVB6	3453	4473	0.10%	0.012%
43	16.239	2250	2253	2259	rBV8	5279	11117	0.25%	0.031%
44	16.516	2294	2300	2305	rBV8	3869	7590	0.17%	0.021%
45	17.110	2395	2401	2411	rBV	1345913	1818058	40.87%	4.993%
46	17.216	2412	2419	2430	rVV2	1947577	3117115	70.07%	8.561%
47	17.410	2450	2452	2458	rBV7	3346	5275	0.12%	0.014%
48	17.486	2462	2465	2466	rBV3	4971	5220	0.12%	0.014%
49	17.810	2518	2520	2527	rVB8	5322	7324	0.16%	0.020%
50	18.051	2557	2561	2568	rBV3	34375	53478	1.20%	0.147%
51	18.498	2634	2637	2640	rBV5	5579	7586	0.17%	0.021%
52	19.139	2742	2746	2752	rBV2	32155	50364	1.13%	0.138%
53	19.216	2754	2759	2763	rBV	36406	54447	1.22%	0.150%
54	19.380	2784	2787	2790	rVB3	20517	21525	0.48%	0.059%
55	19.592	2817	2823	2829	rBV	3366474	4147001	93.22%	11.390%
56	21.539	3147	3154	3163	rBV2	1429310	2315954	52.06%	6.361%
57	24.604	3665	3675	3691	rVB	1732043	4448793	100.00%	12.219%
58	24.827	3703	3713	3725	rVB2	823658	2392890	53.79%	6.572%




Sum of corrected areas: 36410212

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022008.D
Acq On : 24 Sep 2024 23:47
Operator : RC/JU
Sample : P4092-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

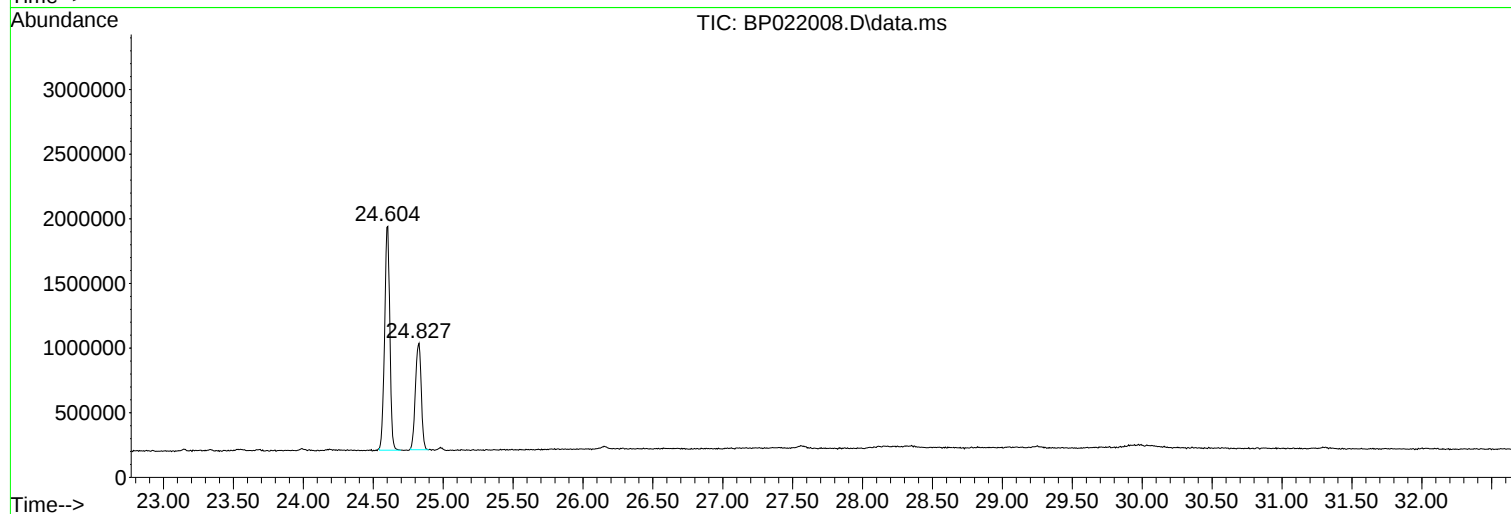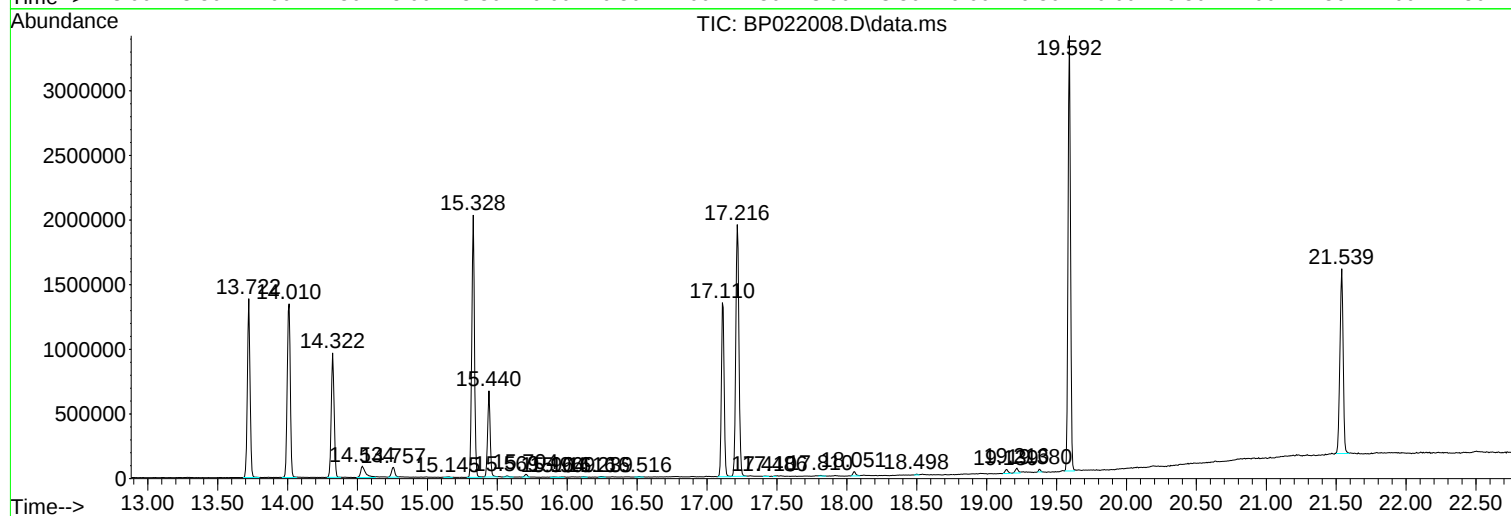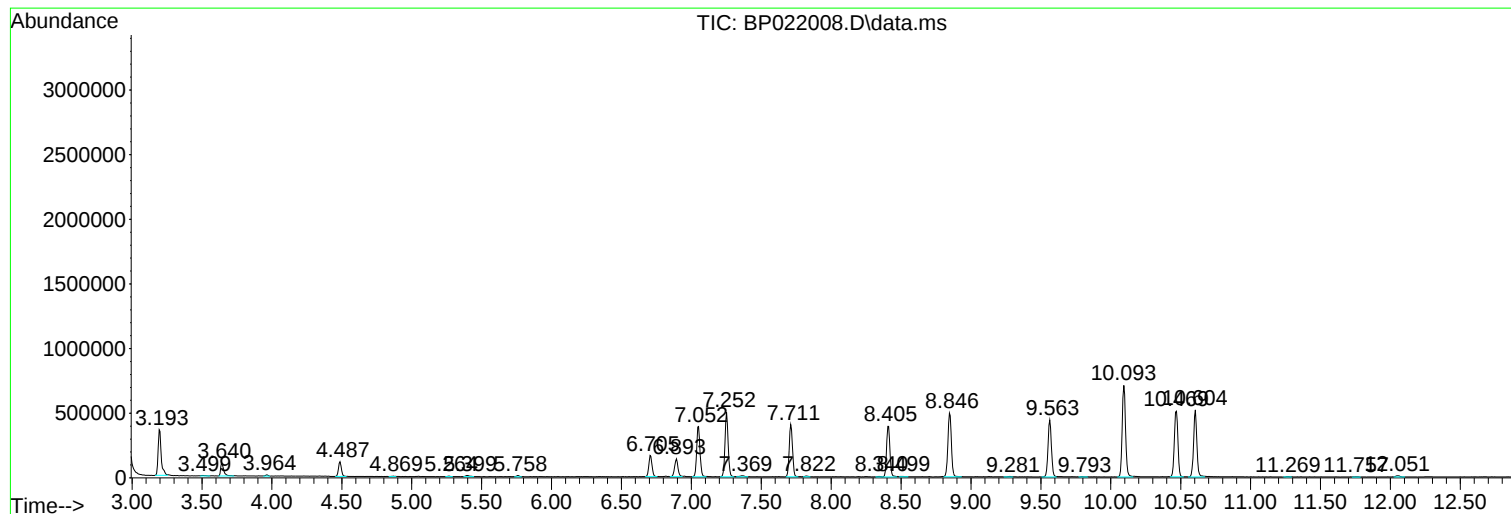

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022008.D
Acq On : 24 Sep 2024 23:47
Operator : RC/JU
Sample : P4092-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B15










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1-chloro-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.705	7.81 ng/ul	259315	1,4-Dichlorobenzene-d4	7.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-chloro-2-methyl-	126	C7H7Cl	000095-49-8	96
2			Benzene, 1-chloro-3-methyl-	126	C7H7Cl	000108-41-8	95
3			Benzene, 1-chloro-2-methyl-	126	C7H7Cl	000095-49-8	94
4			Benzene, 1-chloro-2-methyl-	126	C7H7Cl	000095-49-8	90
5			Benzene, 1-chloro-2-methyl-	126	C7H7Cl	000095-49-8	90

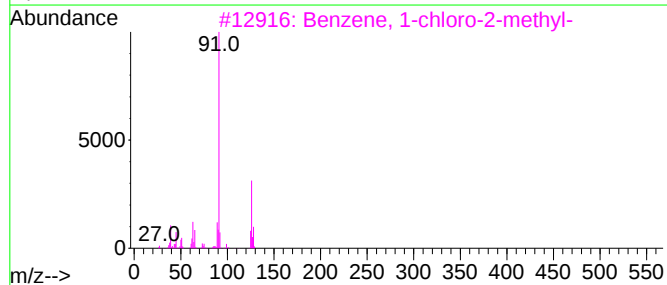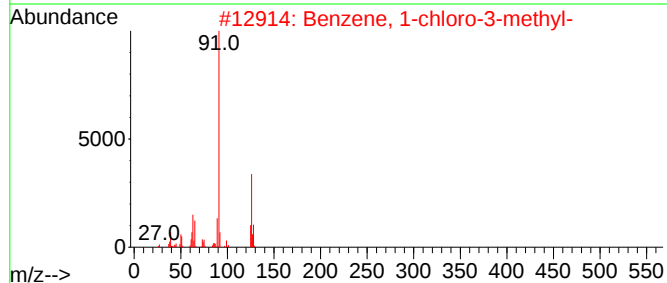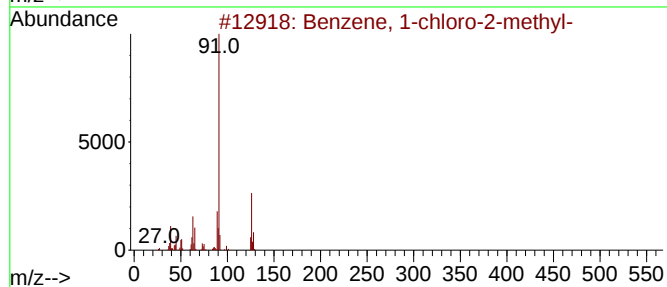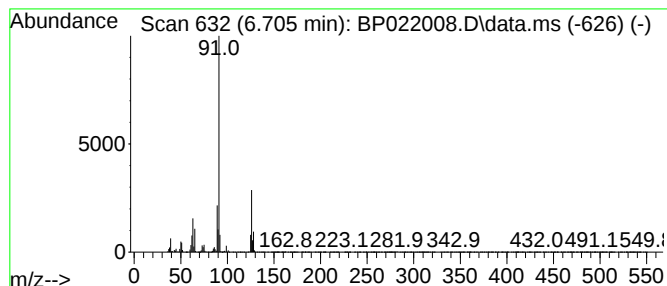

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022008.D
Acq On : 24 Sep 2024 23:47
Operator : RC/JU
Sample : P4092-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1-chlo...	6.705	7.8	ng/u1	259315	1	7.710	664231	20.0