

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022014.D
 Acq On : 25 Sep 2024 04:32
 Operator : RC/JU
 Sample : PB163539BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	45	rBV	34630	42391	0.98%	0.107%
2	3.634	106	110	126	rBV	422071	620009	14.35%	1.571%
3	3.958	162	165	170	rVB	10862	13507	0.31%	0.034%
4	6.887	653	663	675	rBV	496716	828389	19.18%	2.099%
5	7.046	684	690	699	rVV	369841	604058	13.98%	1.531%
6	7.140	703	706	712	rVB5	3660	6016	0.14%	0.015%
7	7.246	717	724	734	rBV	497192	812271	18.80%	2.058%
8	7.705	794	802	810	rBV	469976	732223	16.95%	1.855%
9	8.146	871	877	882	rVB7	4387	6978	0.16%	0.018%
10	8.222	887	890	895	rVB7	3345	5600	0.13%	0.014%
11	8.405	912	921	935	rBV	621317	1026138	23.75%	2.600%
12	8.511	936	939	948	rVB7	8149	17080	0.40%	0.043%
13	8.769	979	983	988	rBV7	3975	5610	0.13%	0.014%
14	8.846	988	996	1008	rBV	487400	820331	18.99%	2.079%
15	9.410	1086	1092	1098	rBV3	5427	7864	0.18%	0.020%
16	9.563	1109	1118	1128	rBV	433313	714155	16.53%	1.810%
17	9.652	1129	1133	1140	rVB5	6454	11736	0.27%	0.030%
18	10.099	1200	1209	1220	rBV	622277	1144224	26.49%	2.899%
19	10.469	1264	1272	1279	rBV	615531	1028303	23.80%	2.606%
20	10.516	1279	1280	1286	rVB2	7450	8152	0.19%	0.021%
21	10.599	1286	1294	1307	rBV	617835	1084593	25.11%	2.748%
22	10.805	1325	1329	1337	rVB9	8019	14457	0.33%	0.037%
23	11.763	1488	1492	1497	rVB7	4354	6710	0.16%	0.017%
24	12.063	1538	1543	1549	rVB3	10857	19239	0.45%	0.049%
25	12.128	1549	1554	1560	rBV2	8317	14584	0.34%	0.037%
26	12.351	1587	1592	1598	rVB2	9021	14861	0.34%	0.038%
27	12.499	1609	1617	1623	rBV7	9132	20759	0.48%	0.053%
28	12.740	1654	1658	1666	rVB9	4758	7707	0.18%	0.020%
29	12.822	1669	1672	1676	rVV5	3444	5275	0.12%	0.013%
30	13.110	1714	1721	1724	rBV6	9607	16214	0.38%	0.041%
31	13.146	1724	1727	1731	rVV2	10795	17407	0.40%	0.044%
32	13.187	1731	1734	1742	rVV	9173	18184	0.42%	0.046%
33	13.281	1745	1750	1755	rVB7	2744	4963	0.11%	0.013%
34	13.728	1818	1826	1833	rVV	1266432	1922196	44.49%	4.871%
35	13.775	1833	1834	1841	rVB	13242	15688	0.36%	0.040%
36	13.893	1848	1854	1857	rBV8	4915	8447	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022014.D
 Acq On : 25 Sep 2024 04:32
 Operator : RC/JU
 Sample : PB163539BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	14.010	1866	1874	1890	rBV	1304908	2103520	48.69%	5.330%
38	14.234	1907	1912	1916	rBV7	4085	5859	0.14%	0.015%
39	14.322	1919	1927	1934	rBV	1047000	1616183	37.41%	4.095%
40	14.387	1934	1938	1942	rVB2	12129	18378	0.43%	0.047%
41	14.528	1956	1962	1978	rBV	582658	948219	21.95%	2.403%
42	14.640	1978	1981	1986	rVB	14837	22260	0.52%	0.056%
43	14.687	1986	1989	1992	rBV4	5284	8653	0.20%	0.022%
44	14.722	1992	1995	2000	rVB	8299	11996	0.28%	0.030%
45	14.957	2029	2035	2040	rBV8	6940	12999	0.30%	0.033%
46	15.163	2064	2070	2074	rBV	12575	16952	0.39%	0.043%
47	15.328	2090	2098	2104	rBV	1678937	2739860	63.42%	6.943%
48	15.387	2104	2108	2113	rVB3	22199	36668	0.85%	0.093%
49	15.457	2113	2120	2128	rBV	557524	808750	18.72%	2.049%
50	15.587	2134	2142	2149	rVB4	16459	36971	0.86%	0.094%
51	16.140	2230	2236	2241	rBV6	5627	9478	0.22%	0.024%
52	16.287	2256	2261	2268	rBV4	10728	17902	0.41%	0.045%
53	16.410	2274	2282	2288	rBV7	13292	23805	0.55%	0.060%
54	16.569	2306	2309	2315	rVB5	6892	10317	0.24%	0.026%
55	16.763	2338	2342	2345	rBV5	6155	9990	0.23%	0.025%
56	16.904	2362	2366	2369	rBV4	4283	6360	0.15%	0.016%
57	17.116	2394	2402	2409	rBV	1253884	2148698	49.74%	5.445%
58	17.222	2414	2420	2432	rVV	2384461	3258168	75.42%	8.256%
59	17.539	2470	2474	2482	rVB	9344	16060	0.37%	0.041%
60	17.816	2518	2521	2525	rVB6	5086	7510	0.17%	0.019%
61	18.051	2557	2561	2567	rBV7	6312	10329	0.24%	0.026%
62	18.122	2570	2573	2577	rVB	12611	14362	0.33%	0.036%
63	19.133	2741	2745	2751	rBV3	31096	39467	0.91%	0.100%
64	19.204	2754	2757	2761	rBV2	21786	38365	0.89%	0.097%
65	19.586	2815	2822	2832	rVB	2612051	4065655	94.11%	10.302%
66	21.533	3147	3153	3160	rBV2	1609498	2709491	62.72%	6.866%
67	24.592	3663	3673	3687	rVB2	1680060	4320037	100.00%	10.947%
68	24.816	3703	3711	3724	rVB	1039903	2724784	63.07%	6.904%




Sum of corrected areas: 39464365

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022014.D
Acq On : 25 Sep 2024 04:32
Operator : RC/JU
Sample : PB163539BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK539

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

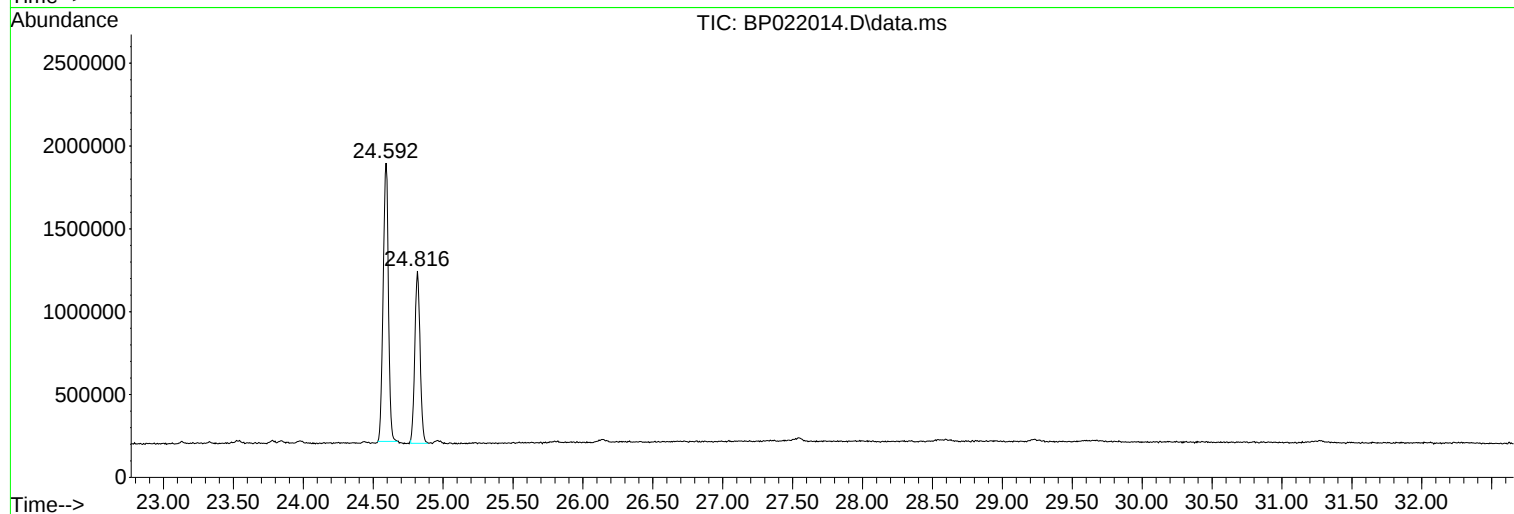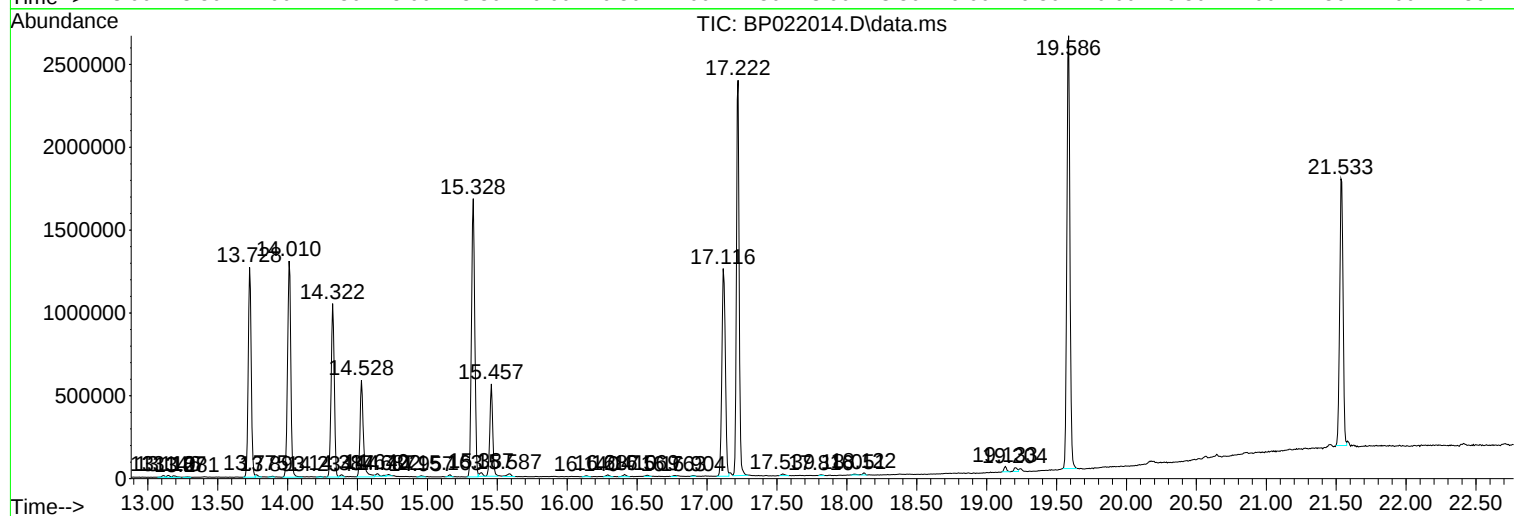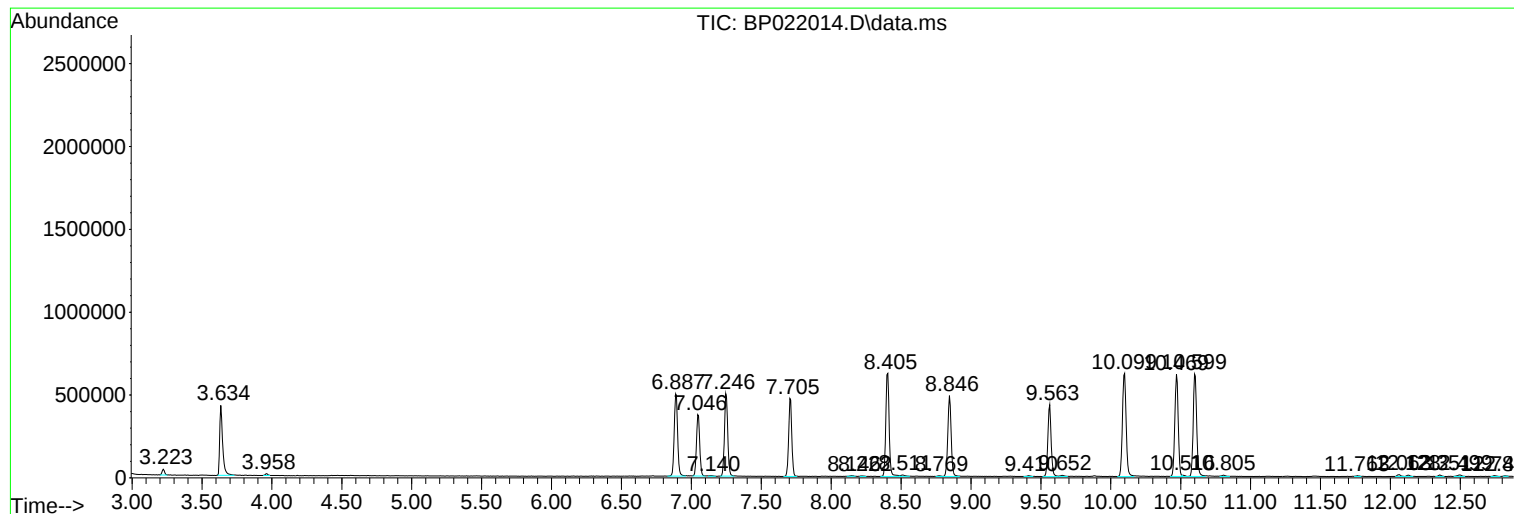

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022014.D
Acq On : 25 Sep 2024 04:32
Operator : RC/JU
Sample : PB163539BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK539

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022014.D
Acq On : 25 Sep 2024 04:32
Operator : RC/JU
Sample : PB163539BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK539

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------