

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022015.D
 Acq On : 25 Sep 2024 05:13
 Operator : RC/JU
 Sample : PB163586BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	45	rBV	31580	37141	1.00%	0.119%
2	3.634	106	110	132	rBV	364982	543188	14.65%	1.734%
3	3.958	161	165	171	rVB2	8559	12041	0.32%	0.038%
4	6.893	654	664	677	rBV	449244	716920	19.33%	2.289%
5	7.046	684	690	700	rVB	328557	523585	14.12%	1.671%
6	7.246	715	724	735	rBV	434221	722248	19.47%	2.306%
7	7.716	797	804	811	rBV	367232	605880	16.34%	1.934%
8	8.405	914	921	931	rBV	510555	865232	23.33%	2.762%
9	8.852	989	997	1009	rBV	416640	702680	18.95%	2.243%
10	9.563	1110	1118	1132	rBV	365237	611694	16.49%	1.953%
11	10.099	1202	1209	1223	rBV	553753	956068	25.78%	3.052%
12	10.475	1265	1273	1284	rVB	501994	781586	21.07%	2.495%
13	10.604	1287	1295	1310	rBV	507625	893263	24.08%	2.852%
14	12.057	1536	1542	1548	rBV3	7989	15296	0.41%	0.049%
15	13.722	1817	1825	1842	rBV	1001771	1510608	40.73%	4.822%
16	14.004	1865	1873	1888	rBV2	966359	1617977	43.62%	5.165%
17	14.322	1915	1927	1937	rBV	784557	1172925	31.62%	3.744%
18	14.528	1954	1962	1977	rBV	433480	761041	20.52%	2.430%
19	14.740	1997	1998	2005	rVB7	3257	4043	0.11%	0.013%
20	15.322	2089	2097	2105	rBV	1449280	2201020	59.34%	7.027%
21	15.445	2110	2118	2132	rVV	442744	653895	17.63%	2.087%
22	15.569	2135	2139	2147	rVB7	7078	15487	0.42%	0.049%
23	16.122	2227	2233	2239	rBV10	4255	7691	0.21%	0.025%
24	16.287	2256	2261	2267	rBV10	1891	4971	0.13%	0.016%
25	16.781	2340	2345	2348	rBV7	2632	4401	0.12%	0.014%
26	16.886	2360	2363	2366	rBV4	2909	4262	0.11%	0.014%
27	17.110	2394	2401	2408	rBV	994050	1576678	42.51%	5.033%
28	17.216	2411	2419	2433	rVV	1623979	2571622	69.34%	8.210%
29	18.051	2558	2561	2563	rBV4	4282	5018	0.14%	0.016%
30	19.133	2741	2745	2750	rVB3	20749	31505	0.85%	0.101%
31	19.216	2755	2759	2764	rVB2	18452	28683	0.77%	0.092%
32	19.598	2817	2824	2834	rBV	2451839	3249117	87.60%	10.373%
33	21.545	3149	3155	3165	rBV	1419963	2056912	55.46%	6.567%
34	24.610	3664	3676	3691	rVB	1298167	3708904	100.00%	11.840%
35	24.827	3705	3713	3728	rVB	843755	2150732	57.99%	6.866%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022015.D
Acq On : 25 Sep 2024 05:13
Operator : RC/JU
Sample : PB163586BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 31324314

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022015.D
Acq On : 25 Sep 2024 05:13
Operator : RC/JU
Sample : PB163586BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

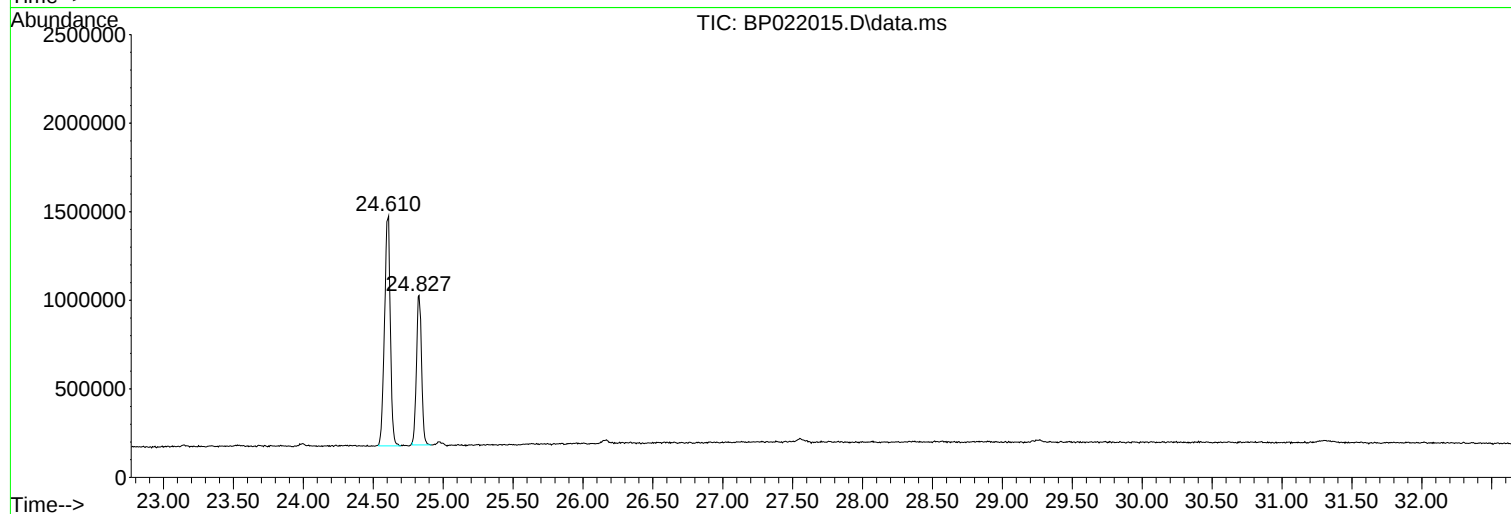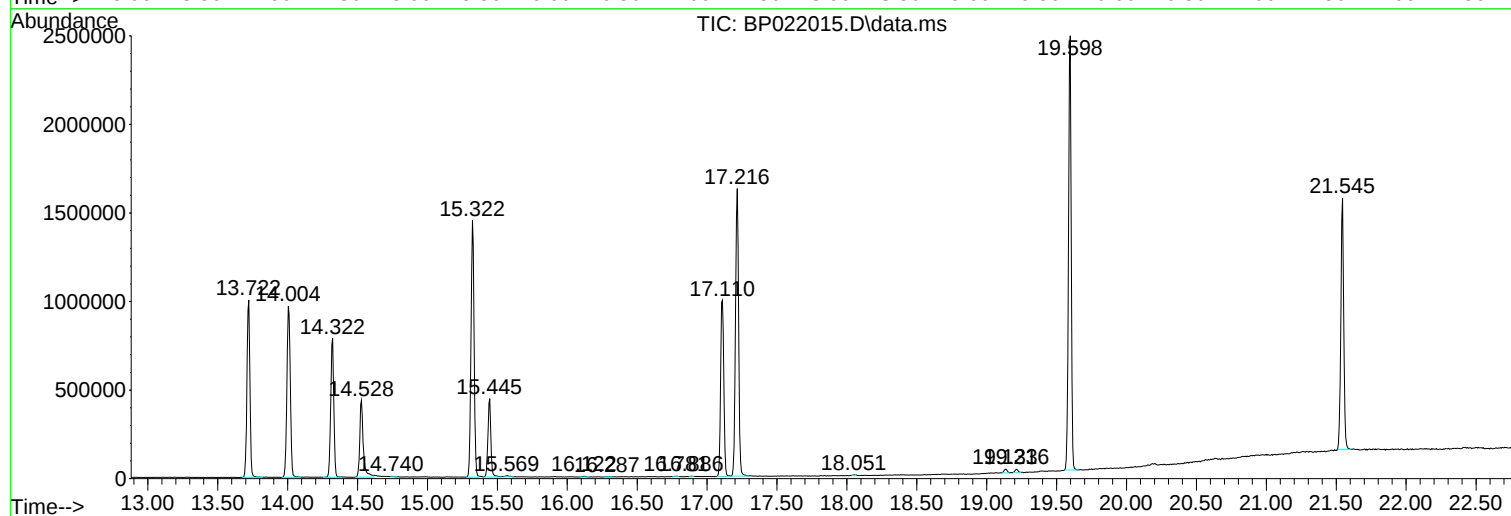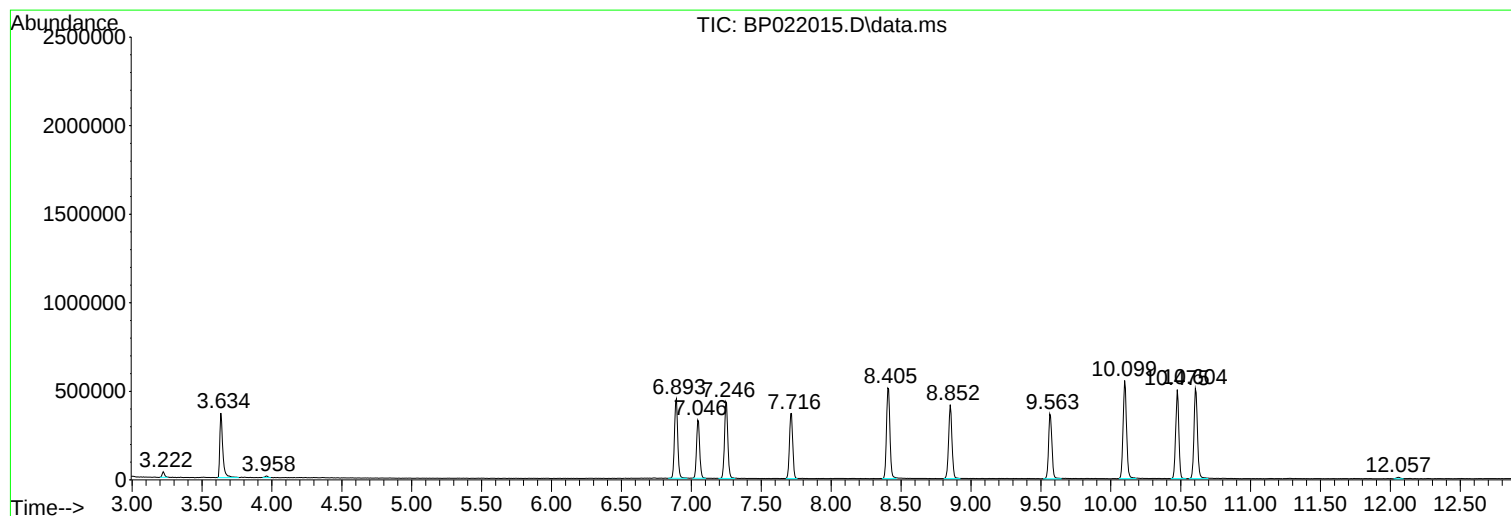

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022015.D
Acq On : 25 Sep 2024 05:13
Operator : RC/JU
Sample : PB163586BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022015.D
Acq On : 25 Sep 2024 05:13
Operator : RC/JU
Sample : PB163586BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------