

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022017.D
 Acq On : 25 Sep 2024 06:34
 Operator : RC/JU
 Sample : P4080-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	47	rBV	31061	42532	0.74%	0.103%
2	3.640	107	111	125	rBV	162852	253907	4.44%	0.617%
3	3.964	161	166	171	rVB2	15479	21909	0.38%	0.053%
4	6.893	657	664	673	rBV	173180	279743	4.89%	0.680%
5	7.052	685	691	700	rBV	468069	706133	12.35%	1.716%
6	7.252	715	725	736	rBV	561824	905188	15.83%	2.200%
7	7.711	795	803	810	rBV	447281	683184	11.94%	1.660%
8	8.405	914	921	934	rBV	486562	802316	14.03%	1.950%
9	8.846	988	996	1009	rBV	587735	959097	16.77%	2.331%
10	9.558	1110	1117	1127	rBV	516336	837132	14.64%	2.034%
11	10.099	1199	1209	1220	rBV	805220	1356441	23.72%	3.296%
12	10.469	1261	1272	1283	rBV	525234	918001	16.05%	2.231%
13	10.599	1285	1294	1304	rBV	628998	1082445	18.93%	2.630%
14	11.257	1400	1406	1410	rBV8	4846	9240	0.16%	0.022%
15	12.052	1534	1541	1546	rBV2	12059	21173	0.37%	0.051%
16	12.234	1567	1572	1578	rBV9	2879	6654	0.12%	0.016%
17	13.275	1744	1749	1752	rBV5	4099	6594	0.12%	0.016%
18	13.722	1818	1825	1834	rBV	1558291	2120266	37.07%	5.152%
19	14.010	1864	1874	1884	rBV	1518682	2259219	39.50%	5.490%
20	14.316	1915	1926	1936	rBV	991770	1395908	24.41%	3.392%
21	14.528	1954	1962	1980	rBV	141448	288097	5.04%	0.700%
22	14.740	1992	1998	2005	rVB6	21443	31917	0.56%	0.078%
23	15.069	2049	2054	2058	rBV	14147	18879	0.33%	0.046%
24	15.328	2090	2098	2105	rBV	2098532	3103484	54.26%	7.542%
25	15.440	2110	2117	2133	rVV	792974	1043739	18.25%	2.536%
26	15.569	2134	2139	2144	rVB3	8986	15596	0.27%	0.038%
27	15.704	2157	2162	2167	rBV9	3259	6065	0.11%	0.015%
28	16.110	2228	2231	2236	rBV3	5525	8137	0.14%	0.020%
29	16.322	2264	2267	2272	rBV2	4719	7309	0.13%	0.018%
30	16.757	2337	2341	2343	rBV5	6361	8526	0.15%	0.021%
31	16.781	2343	2345	2349	rVB4	5302	5999	0.10%	0.015%
32	17.110	2393	2401	2410	rBV	1262674	1872339	32.74%	4.550%
33	17.210	2411	2418	2428	rVV	2627915	3851116	67.33%	9.358%
34	17.316	2432	2436	2439	rVV6	4939	7394	0.13%	0.018%
35	17.357	2440	2443	2448	rVV2	5917	7534	0.13%	0.018%
36	17.804	2517	2519	2524	rVB5	5054	5961	0.10%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022017.D
Acq On : 25 Sep 2024 06:34
Operator : RC/JU
Sample : P4080-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	18.051	2557	2561	2569	rBV	87236	123338	2.16%	0.300%
38	18.798	2686	2688	2694	rBV	10469	11055	0.19%	0.027%
39	19.139	2742	2746	2751	rVB2	42084	57387	1.00%	0.139%
40	19.210	2754	2758	2763	rBV	38238	60550	1.06%	0.147%
41	19.386	2784	2788	2794	rBV3	76159	110019	1.92%	0.267%
42	19.534	2811	2813	2816	rBV3	10219	12002	0.21%	0.029%
43	19.586	2816	2822	2833	rVB	3786593	4989447	87.24%	12.124%
44	21.539	3148	3154	3162	rBV	1586279	2454783	42.92%	5.965%
45	24.592	3663	3673	3685	rVB	2055672	5719434	100.00%	13.898%
46	24.816	3701	3711	3723	rVB	990693	2664604	46.59%	6.475%




Sum of corrected areas: 41151793

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022017.D
Acq On : 25 Sep 2024 06:34
Operator : RC/JU
Sample : P4080-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

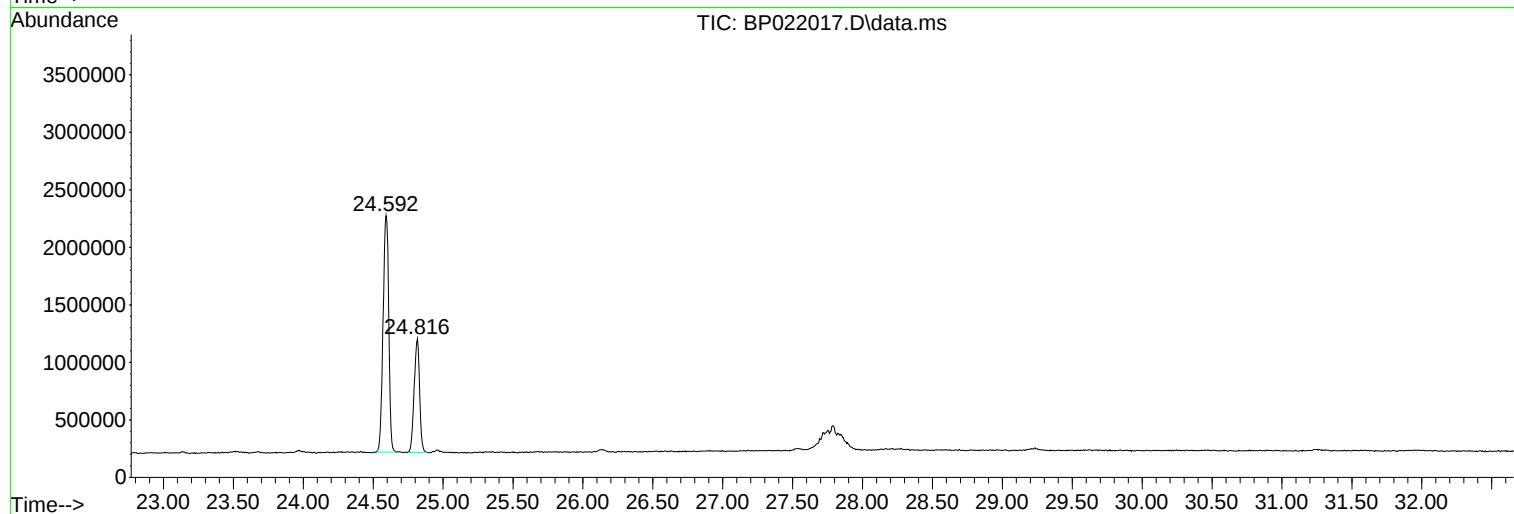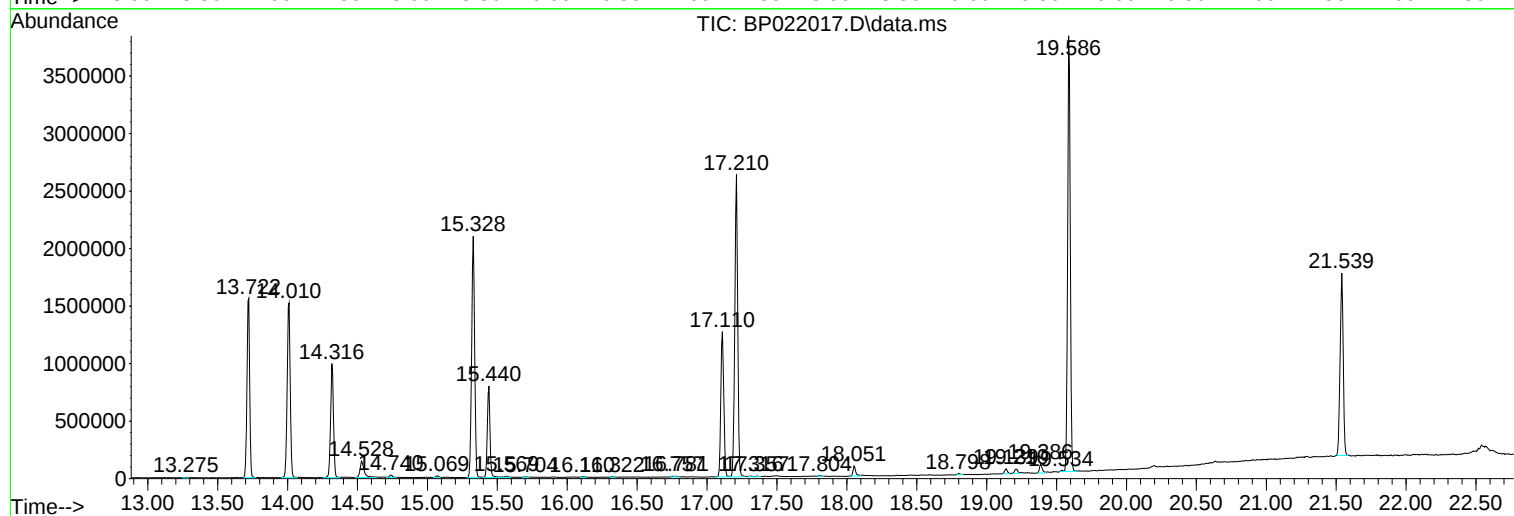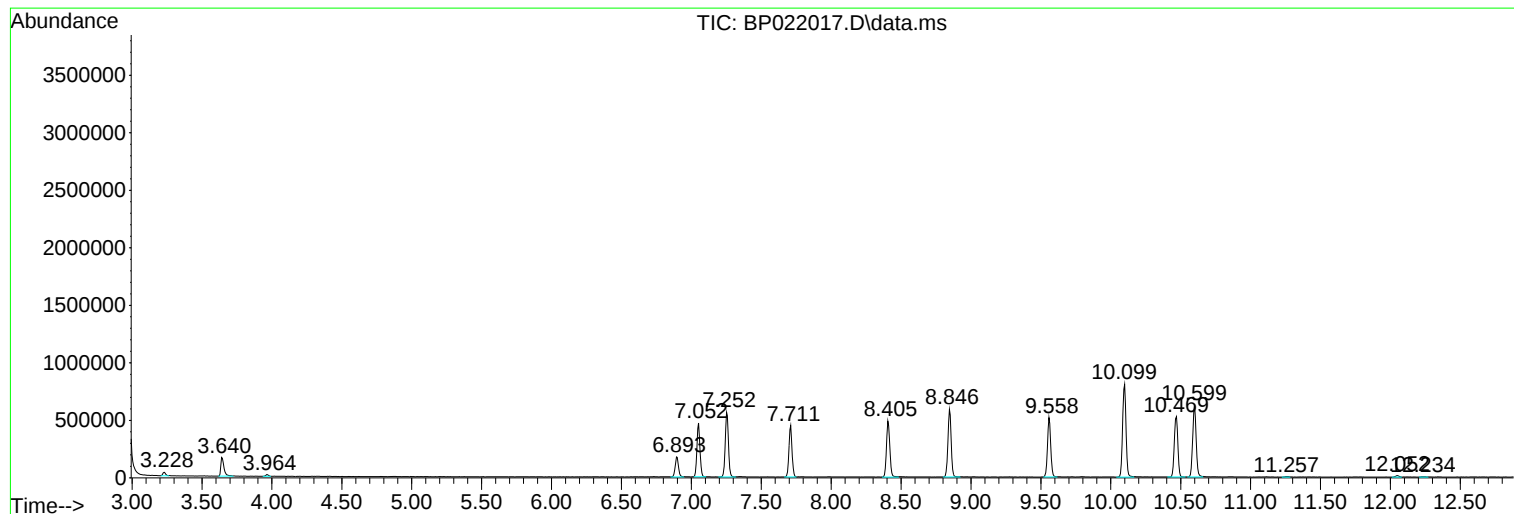

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022017.D
Acq On : 25 Sep 2024 06:34
Operator : RC/JU
Sample : P4080-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022017.D
Acq On : 25 Sep 2024 06:34
Operator : RC/JU
Sample : P4080-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------