

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022028.D
 Acq On : 25 Sep 2024 14:43
 Operator : RC/JU
 Sample : PB163543BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	36	39	47	rVB	30864	43503	1.04%	0.113%
2	3.634	105	110	127	rBV	383411	584558	14.04%	1.515%
3	3.958	160	165	172	rVB2	12166	20168	0.48%	0.052%
4	6.893	653	664	674	rBV	539474	856408	20.57%	2.219%
5	7.046	684	690	700	rVB	414664	608731	14.62%	1.577%
6	7.246	716	724	735	rBV	538166	833844	20.03%	2.160%
7	7.705	793	802	813	rBV	419231	697906	16.76%	1.808%
8	8.152	871	878	883	rBV6	4903	9040	0.22%	0.023%
9	8.228	883	891	896	rVB9	4081	8688	0.21%	0.023%
10	8.410	912	922	931	rBV	608614	1064036	25.56%	2.757%
11	8.510	937	939	944	rVB5	6015	8817	0.21%	0.023%
12	8.775	980	984	988	rBV7	3171	4902	0.12%	0.013%
13	8.846	988	996	1012	rVV	495259	837268	20.11%	2.169%
14	9.416	1089	1093	1097	rBV2	3910	6296	0.15%	0.016%
15	9.557	1108	1117	1128	rBV	429262	729862	17.53%	1.891%
16	9.652	1129	1133	1140	rVB8	5721	11078	0.27%	0.029%
17	9.887	1169	1173	1178	rVB5	4922	7289	0.18%	0.019%
18	10.093	1201	1208	1222	rBV	690200	1190968	28.60%	3.086%
19	10.469	1264	1272	1278	rBV	554622	954580	22.93%	2.473%
20	10.516	1278	1280	1285	rVB4	6729	8333	0.20%	0.022%
21	10.599	1286	1294	1311	rBV	660213	1108856	26.63%	2.873%
22	10.804	1321	1329	1335	rVB10	5364	12367	0.30%	0.032%
23	11.446	1428	1438	1439	rBV10	2682	5612	0.13%	0.015%
24	11.763	1484	1492	1497	rBV10	4005	9972	0.24%	0.026%
25	12.046	1535	1540	1546	rBV2	11322	19240	0.46%	0.050%
26	12.128	1548	1554	1559	rVB4	6416	12212	0.29%	0.032%
27	12.346	1584	1591	1595	rVB5	6901	12261	0.29%	0.032%
28	12.487	1609	1615	1620	rBV6	7033	15054	0.36%	0.039%
29	12.746	1653	1659	1665	rVV9	4114	8374	0.20%	0.022%
30	12.816	1667	1671	1679	rVB9	4426	9190	0.22%	0.024%
31	13.104	1714	1720	1723	rBV4	8430	14256	0.34%	0.037%
32	13.140	1723	1726	1730	rVV3	9965	15219	0.37%	0.039%
33	13.181	1730	1733	1738	rVB3	8052	12116	0.29%	0.031%
34	13.387	1764	1768	1774	rBV9	2447	5258	0.13%	0.014%
35	13.716	1816	1824	1830	rBV	1302148	1926459	46.27%	4.991%
36	13.763	1830	1832	1839	rVB2	13251	17569	0.42%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022028.D
 Acq On : 25 Sep 2024 14:43
 Operator : RC/JU
 Sample : PB163543BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	13.881	1849	1852	1858	rVB7	4499	6690	0.16%	0.017%
38	13.998	1865	1872	1886	rBV2	1332055	2097718	50.38%	5.435%
39	14.222	1907	1910	1915	rBV7	3046	5381	0.13%	0.014%
40	14.310	1917	1925	1933	rBV	979241	1494038	35.88%	3.871%
41	14.375	1933	1936	1944	rVB2	10833	16131	0.39%	0.042%
42	14.522	1953	1961	1977	rBV	541140	962483	23.12%	2.494%
43	14.634	1977	1980	1985	rVV2	18497	32543	0.78%	0.084%
44	14.675	1985	1987	1990	rVV4	9387	14001	0.34%	0.036%
45	14.716	1990	1994	2006	rVB	12889	32097	0.77%	0.083%
46	14.951	2028	2034	2037	rBV7	6679	11094	0.27%	0.029%
47	15.151	2062	2068	2071	rBV3	10654	15566	0.37%	0.040%
48	15.322	2089	2097	2103	rBV	1901213	2804212	67.35%	7.266%
49	15.375	2103	2106	2111	rVV3	23316	35459	0.85%	0.092%
50	15.445	2111	2118	2127	rVV	520726	752330	18.07%	1.949%
51	15.581	2135	2141	2146	rVB4	12835	27146	0.65%	0.070%
52	16.116	2228	2232	2241	rBV4	5406	9026	0.22%	0.023%
53	16.281	2256	2260	2266	rVB4	10142	14844	0.36%	0.038%
54	16.398	2277	2280	2288	rVB6	11398	19104	0.46%	0.049%
55	16.563	2304	2308	2313	rBV8	7332	11581	0.28%	0.030%
56	16.763	2336	2342	2353	rBV8	7271	21949	0.53%	0.057%
57	16.898	2361	2365	2366	rBV4	3565	5076	0.12%	0.013%
58	17.116	2392	2402	2408	rBV	1277010	1993959	47.89%	5.166%
59	17.216	2412	2419	2432	rVB	2440577	3270277	78.55%	8.473%
60	17.533	2470	2473	2481	rVB2	9839	14759	0.35%	0.038%
61	17.816	2517	2521	2526	rBV7	6398	11442	0.27%	0.030%
62	18.057	2558	2562	2564	rBV5	7428	9471	0.23%	0.025%
63	18.128	2571	2574	2578	rBV2	12477	13593	0.33%	0.035%
64	19.139	2742	2746	2753	rVB3	28536	46582	1.12%	0.121%
65	19.216	2755	2759	2761	rBV	29598	40155	0.96%	0.104%
66	19.592	2817	2823	2832	rBV	2948924	4163523	100.00%	10.788%
67	21.545	3149	3155	3162	rBV	1440271	2422117	58.17%	6.276%
68	24.604	3666	3675	3686	rBV2	1734812	4141878	99.48%	10.731%
69	24.833	3705	3714	3725	rVB	917421	2389060	57.38%	6.190%




Sum of corrected areas: 38595575

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022028.D
Acq On : 25 Sep 2024 14:43
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

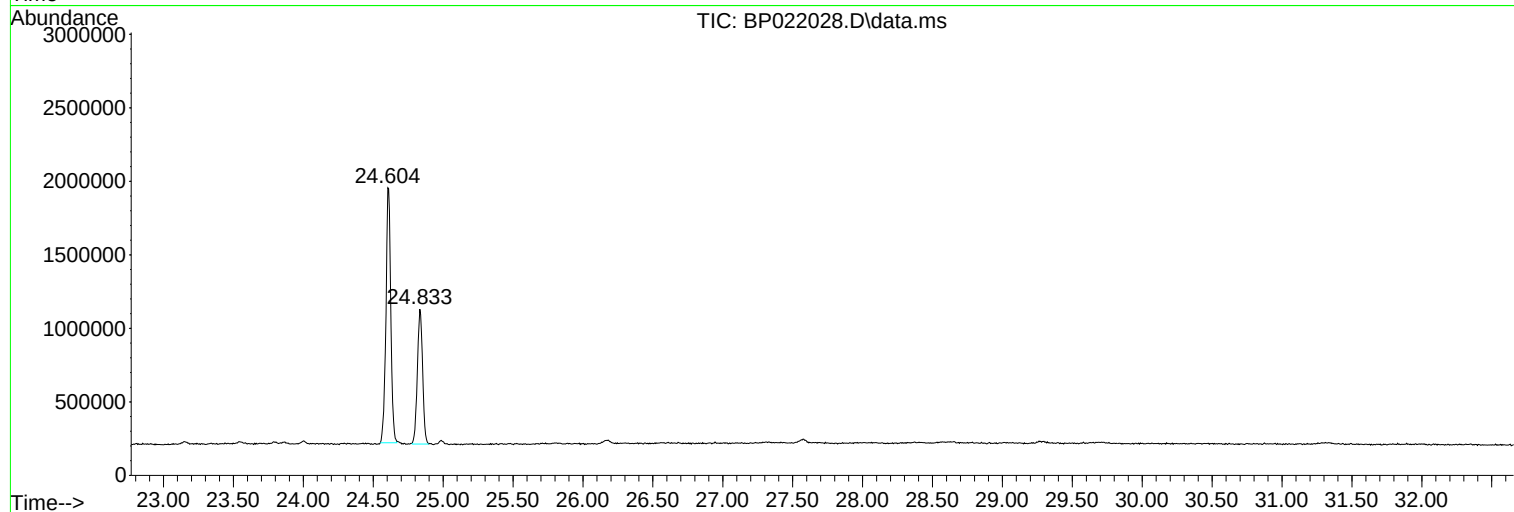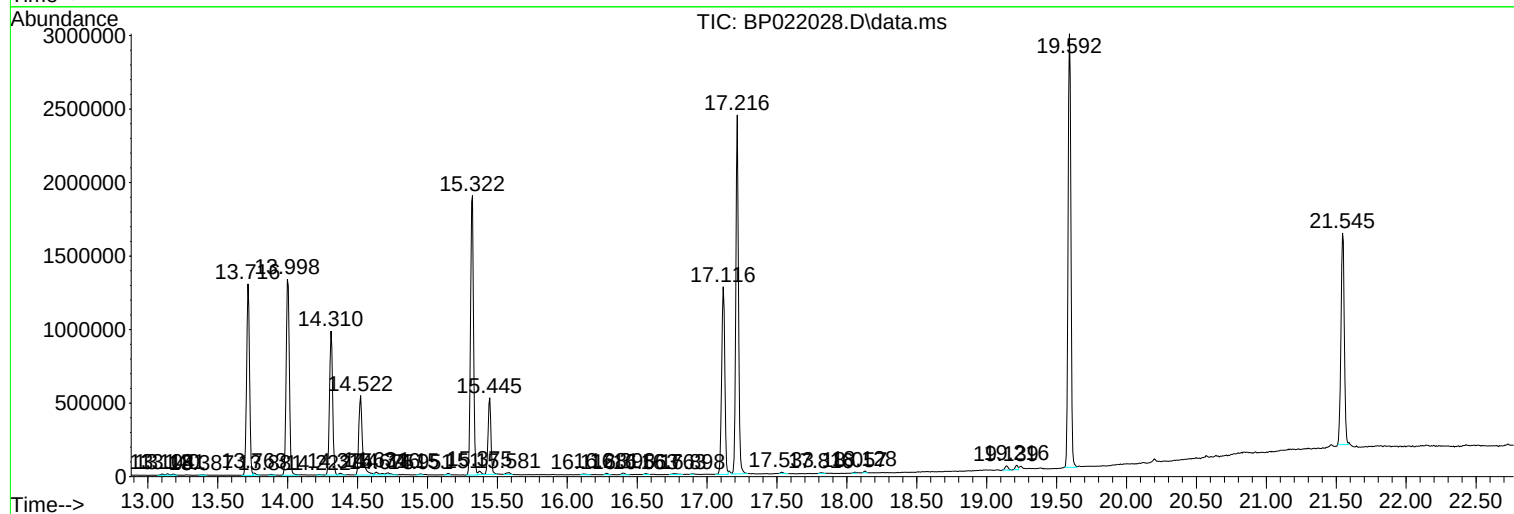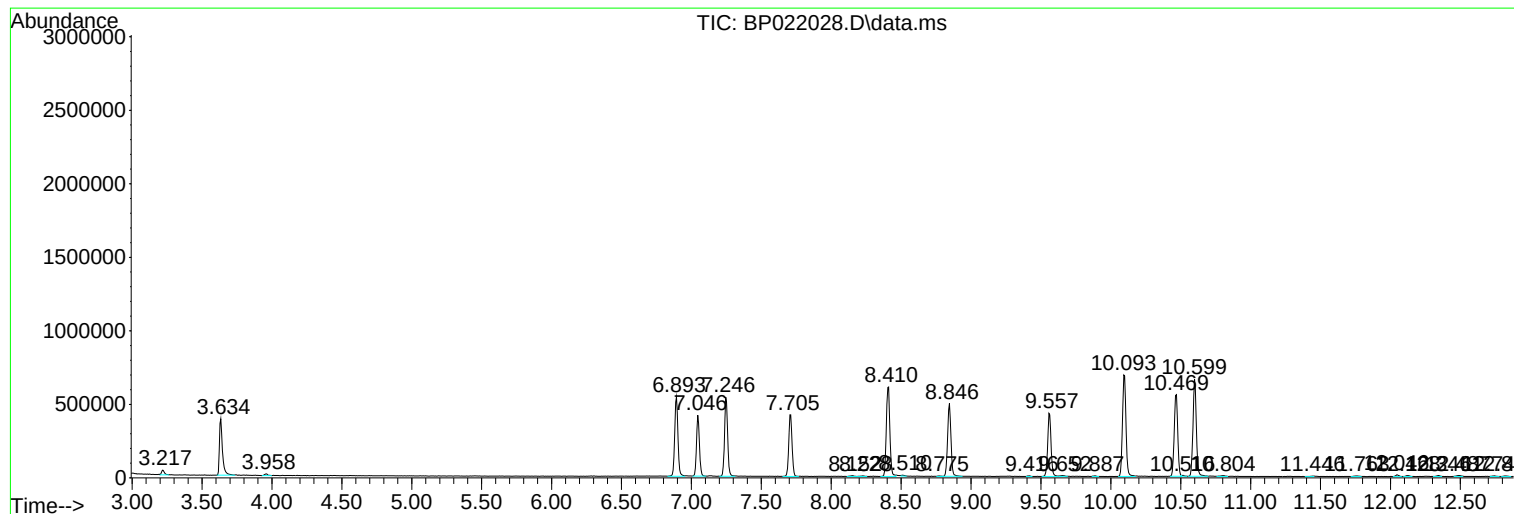

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022028.D
Acq On : 25 Sep 2024 14:43
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022028.D
Acq On : 25 Sep 2024 14:43
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc