

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022031.D
 Acq On : 25 Sep 2024 16:45
 Operator : RC/JU
 Sample : P4107-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	37	rBV4	4430	6860	0.17%	0.022%
2	3.223	37	40	48	rVB	25848	35977	0.88%	0.114%
3	3.499	83	87	91	rBV7	3440	7145	0.18%	0.023%
4	3.640	107	111	121	rBV	82534	124967	3.07%	0.397%
5	3.958	160	165	173	rVB	12259	17765	0.44%	0.056%
6	4.481	249	254	262	rVB2	23595	35668	0.88%	0.113%
7	4.870	315	320	328	rVB2	16890	28058	0.69%	0.089%
8	5.417	409	413	417	rVB6	2755	4300	0.11%	0.014%
9	6.893	656	664	672	rBV	178124	292278	7.18%	0.928%
10	7.046	681	690	699	rBV	342352	554054	13.62%	1.759%
11	7.246	714	724	735	rBV	457206	739573	18.18%	2.348%
12	7.705	793	802	811	rBV	384850	597886	14.70%	1.898%
13	8.405	913	921	933	rBV	463422	744002	18.29%	2.362%
14	8.846	987	996	1006	rBV	440629	757878	18.63%	2.406%
15	9.275	1064	1069	1074	rVB8	2238	4432	0.11%	0.014%
16	9.558	1109	1117	1129	rBV	385522	656638	16.14%	2.085%
17	10.093	1200	1208	1224	rBV	610175	1064236	26.16%	3.379%
18	10.463	1263	1271	1280	rBV	454094	782090	19.22%	2.483%
19	10.599	1286	1294	1305	rBV	375850	669758	16.46%	2.126%
20	11.263	1402	1407	1414	rVB10	2845	5928	0.15%	0.019%
21	11.746	1485	1489	1496	rBV10	2620	4277	0.11%	0.014%
22	12.052	1536	1541	1548	rVB	8602	15516	0.38%	0.049%
23	12.234	1561	1572	1580	rBV5	5872	15173	0.37%	0.048%
24	13.716	1816	1824	1837	rBV	1197321	1656339	40.71%	5.258%
25	13.998	1864	1872	1882	rBV	1219299	1712556	42.09%	5.437%
26	14.310	1917	1925	1933	rBV	743248	1169688	28.75%	3.713%
27	14.528	1955	1962	1978	rBV	127694	275959	6.78%	0.876%
28	14.751	1993	2000	2007	rBV	48972	78429	1.93%	0.249%
29	15.145	2060	2067	2071	rBV7	1904	4146	0.10%	0.013%
30	15.316	2087	2096	2109	rBV	1412805	2348170	57.72%	7.455%
31	15.445	2110	2118	2131	rVV	494842	743595	18.28%	2.361%
32	15.563	2134	2138	2146	rVB3	9705	19102	0.47%	0.061%
33	16.134	2228	2235	2237	rVB8	2466	4877	0.12%	0.015%
34	16.792	2343	2347	2352	rBV7	3734	5981	0.15%	0.019%
35	16.892	2363	2364	2372	rVB8	3249	5732	0.14%	0.018%
36	17.116	2394	2402	2412	rBV	972067	1555125	38.23%	4.937%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022031.D
Acq On : 25 Sep 2024 16:45
Operator : RC/JU
Sample : P4107-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B43

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	17.222	2413	2420	2433	rVV	2013171	2772238	68.14%	8.801%
38	17.710	2498	2503	2505	rBV5	2564	5054	0.12%	0.016%
39	17.816	2519	2521	2526	rBV5	3498	5805	0.14%	0.018%
40	18.051	2556	2561	2568	rBV7	21623	33207	0.82%	0.105%
41	18.634	2658	2660	2664	rBV5	4073	6536	0.16%	0.021%
42	19.133	2741	2745	2751	rBV	25899	36621	0.90%	0.116%
43	19.210	2754	2758	2762	rBV2	28411	44640	1.10%	0.142%
44	19.375	2784	2786	2792	rVB7	13997	20481	0.50%	0.065%
45	19.592	2816	2823	2830	rBV	2594009	3568162	87.71%	11.328%
46	21.533	3147	3153	3165	rVB2	1225892	1985709	48.81%	6.304%
47	24.598	3664	3674	3686	rVB	1407749	4068316	100.00%	12.915%
48	24.816	3702	3711	3725	rVB	814564	2208613	54.29%	7.012%




Sum of corrected areas: 31499540

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022031.D
Acq On : 25 Sep 2024 16:45
Operator : RC/JU
Sample : P4107-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

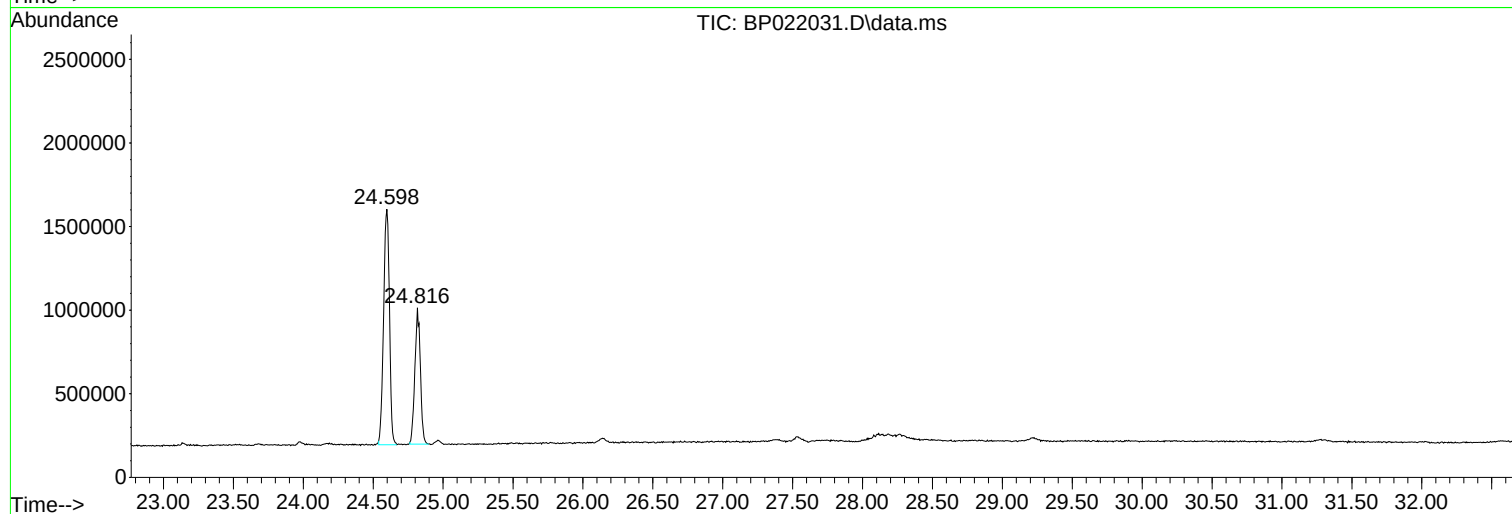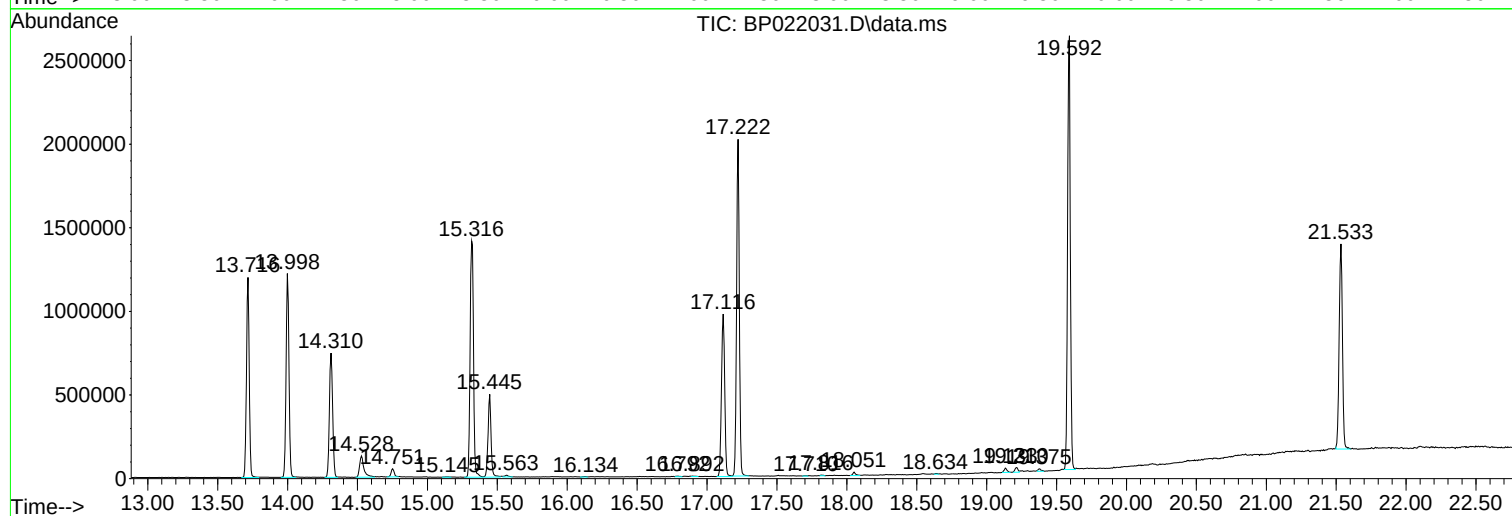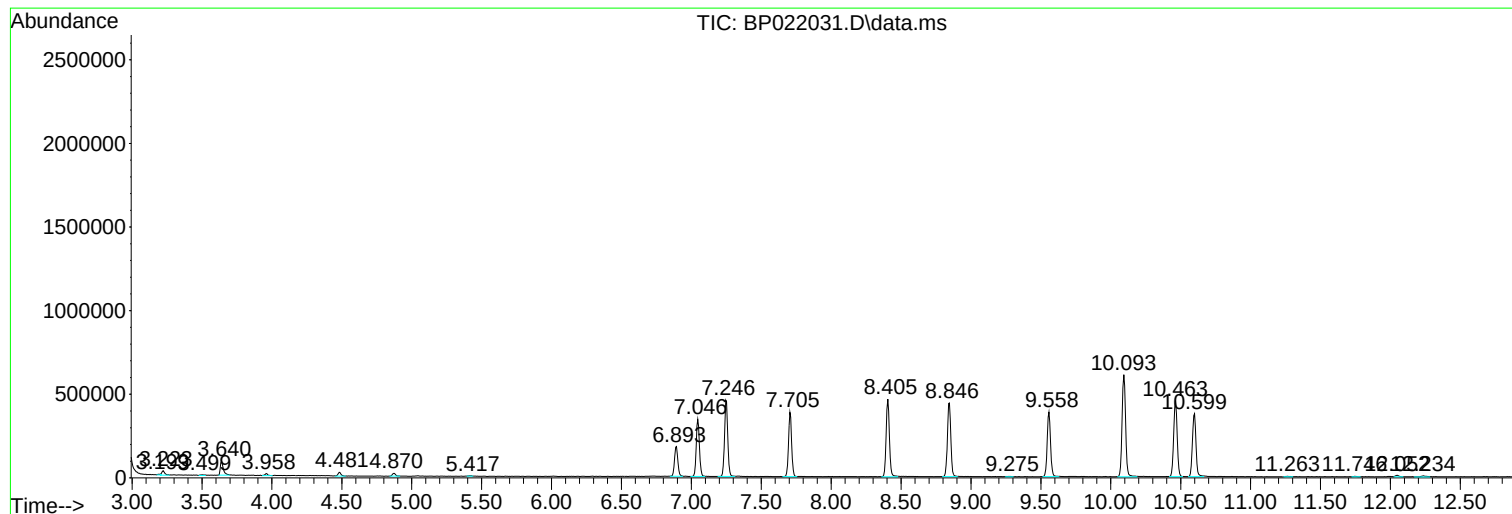

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022031.D
Acq On : 25 Sep 2024 16:45
Operator : RC/JU
Sample : P4107-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022031.D
Acq On : 25 Sep 2024 16:45
Operator : RC/JU
Sample : P4107-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------