

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022034.D
 Acq On : 25 Sep 2024 18:48
 Operator : RC/JU
 Sample : P4013-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	44	rVB	21156	25098	0.81%	0.103%
2	3.640	108	111	122	rVB	64553	99968	3.23%	0.410%
3	3.963	161	166	169	rBV3	4831	7278	0.24%	0.030%
4	6.887	656	663	674	rVB	101195	169327	5.47%	0.695%
5	7.046	683	690	699	rBV	287584	416770	13.47%	1.710%
6	7.245	717	724	731	rBV	347260	531199	17.17%	2.179%
7	7.340	739	740	749	rVB9	2887	4496	0.15%	0.018%
8	7.704	795	802	810	rBV	309658	493946	15.97%	2.026%
9	8.404	913	921	934	rBV	257212	458225	14.81%	1.880%
10	8.781	981	985	989	rBV3	9265	15140	0.49%	0.062%
11	8.845	989	996	1007	rVB	348395	561466	18.15%	2.303%
12	9.275	1064	1069	1077	rVB10	2365	5446	0.18%	0.022%
13	9.557	1108	1117	1125	rBV	305856	488380	15.79%	2.004%
14	9.722	1142	1145	1153	rBV10	1598	4314	0.14%	0.018%
15	10.098	1201	1209	1221	rBV	416311	785380	25.39%	3.222%
16	10.369	1250	1255	1262	rBV3	10186	20670	0.67%	0.085%
17	10.469	1264	1272	1279	rVV	378673	638940	20.66%	2.621%
18	10.522	1279	1281	1287	rVB6	3919	5604	0.18%	0.023%
19	10.598	1287	1294	1304	rBV	48255	87606	2.83%	0.359%
20	11.245	1401	1404	1406	rBV4	2386	3156	0.10%	0.013%
21	11.757	1485	1491	1497	rVB4	3743	7434	0.24%	0.030%
22	12.045	1537	1540	1545	rBV3	6397	11850	0.38%	0.049%
23	12.104	1545	1550	1560	rVV3	11368	30721	0.99%	0.126%
24	12.298	1580	1583	1587	rVB5	2573	3160	0.10%	0.013%
25	13.722	1817	1825	1839	rBV	845753	1260147	40.74%	5.170%
26	14.010	1865	1874	1888	rBV2	861811	1331517	43.05%	5.463%
27	14.322	1918	1927	1935	rBV	671996	961870	31.10%	3.946%
28	14.545	1959	1965	1986	rBV	87204	179431	5.80%	0.736%
29	14.680	1986	1988	1995	rVV8	2700	5761	0.19%	0.024%
30	14.757	1995	2001	2008	rVB8	5557	10170	0.33%	0.042%
31	15.004	2036	2043	2045	rBV7	4394	6801	0.22%	0.028%
32	15.151	2063	2068	2074	rBV4	3984	8524	0.28%	0.035%
33	15.327	2091	2098	2111	rBV	1237731	1798604	58.15%	7.379%
34	15.439	2111	2117	2133	rVV	320778	507345	16.40%	2.081%
35	15.574	2135	2140	2145	rVB6	6612	9710	0.31%	0.040%
36	16.039	2215	2219	2226	rBV8	4742	9922	0.32%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022034.D
Acq On : 25 Sep 2024 18:48
Operator : RC/JU
Sample : P4013-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	16.610	2312	2316	2326	rBV	27761	49753	1.61%	0.204%
38	16.774	2338	2344	2351	rVB	3817	7338	0.24%	0.030%
39	17.110	2394	2401	2412	rBV	984474	1332807	43.09%	5.468%
40	17.221	2412	2420	2431	rBV2	1264310	2185239	70.65%	8.965%
41	17.416	2451	2453	2459	rVB4	3379	4147	0.13%	0.017%
42	17.816	2516	2521	2526	rVB2	30382	44966	1.45%	0.184%
43	18.057	2557	2562	2569	rBV3	30486	45939	1.49%	0.188%
44	18.121	2570	2573	2580	rVB2	5345	9496	0.31%	0.039%
45	19.151	2742	2748	2753	rBV4	21852	40417	1.31%	0.166%
46	19.215	2755	2759	2763	rBV	24495	37735	1.22%	0.155%
47	19.380	2784	2787	2794	rBV7	23865	30317	0.98%	0.124%
48	19.592	2817	2823	2832	rBV	2266949	2861259	92.50%	11.738%
49	20.662	3002	3005	3010	rVB2	26475	30794	1.00%	0.126%
50	21.545	3148	3155	3163	rVB	1108952	1771062	57.26%	7.266%
51	24.609	3667	3676	3687	rVB	1115013	3093160	100.00%	12.690%
52	24.827	3705	3713	3727	rVB	723674	1865650	60.32%	7.654%




Sum of corrected areas: 24375455

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022034.D
Acq On : 25 Sep 2024 18:48
Operator : RC/JU
Sample : P4013-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

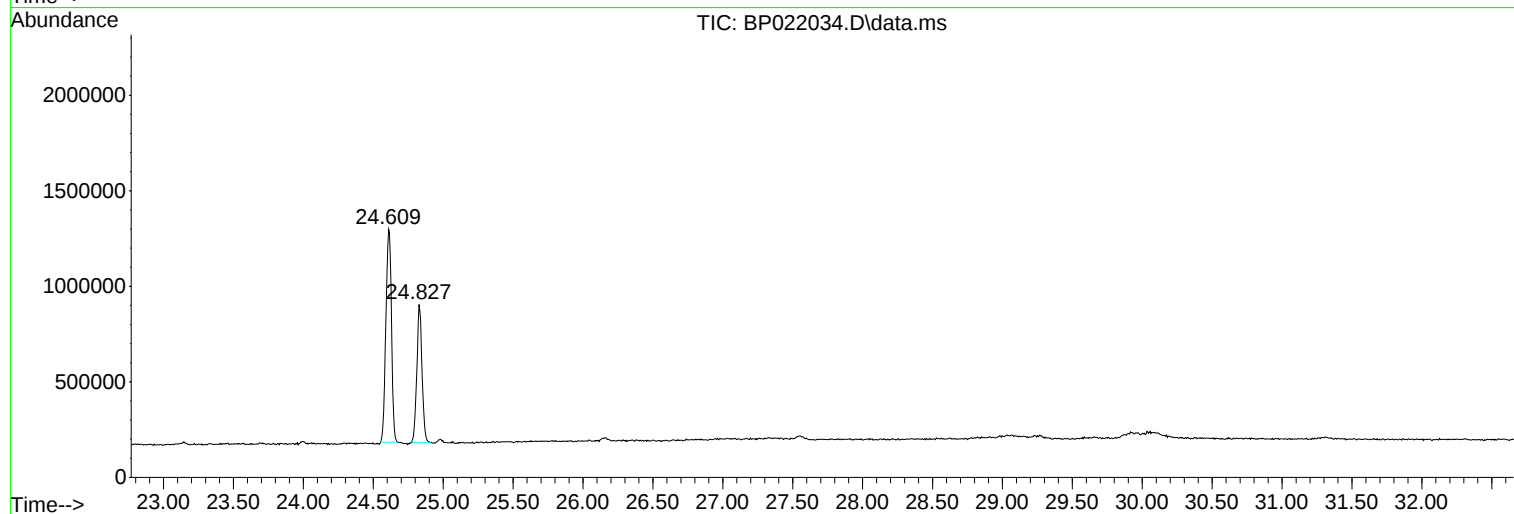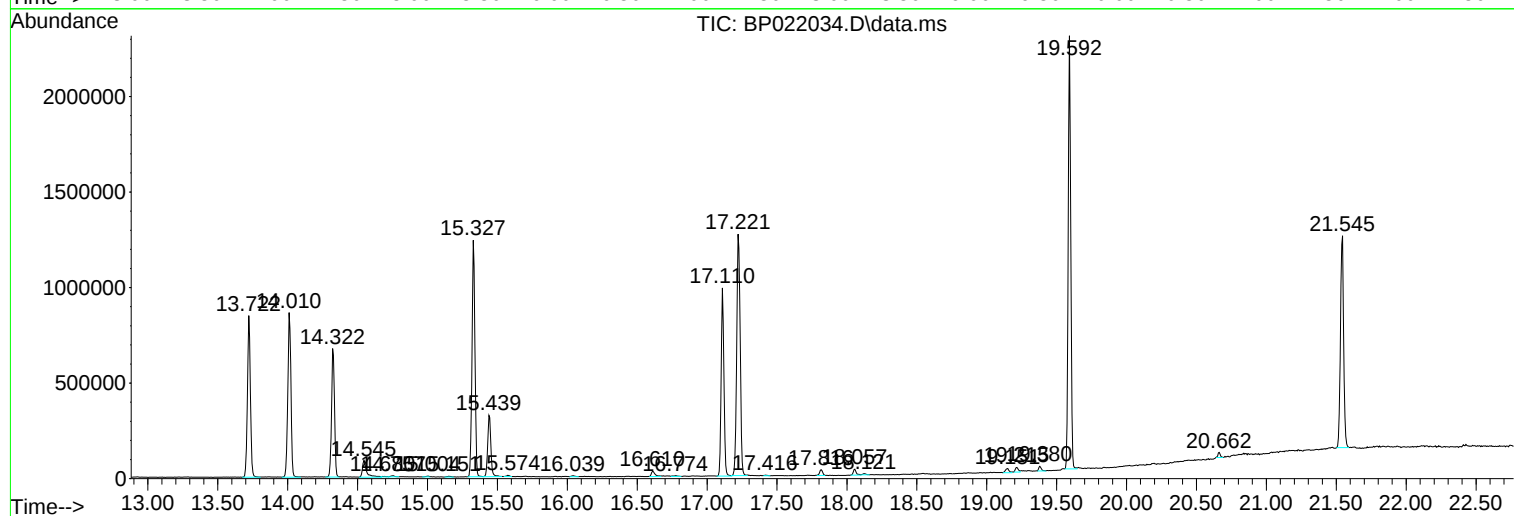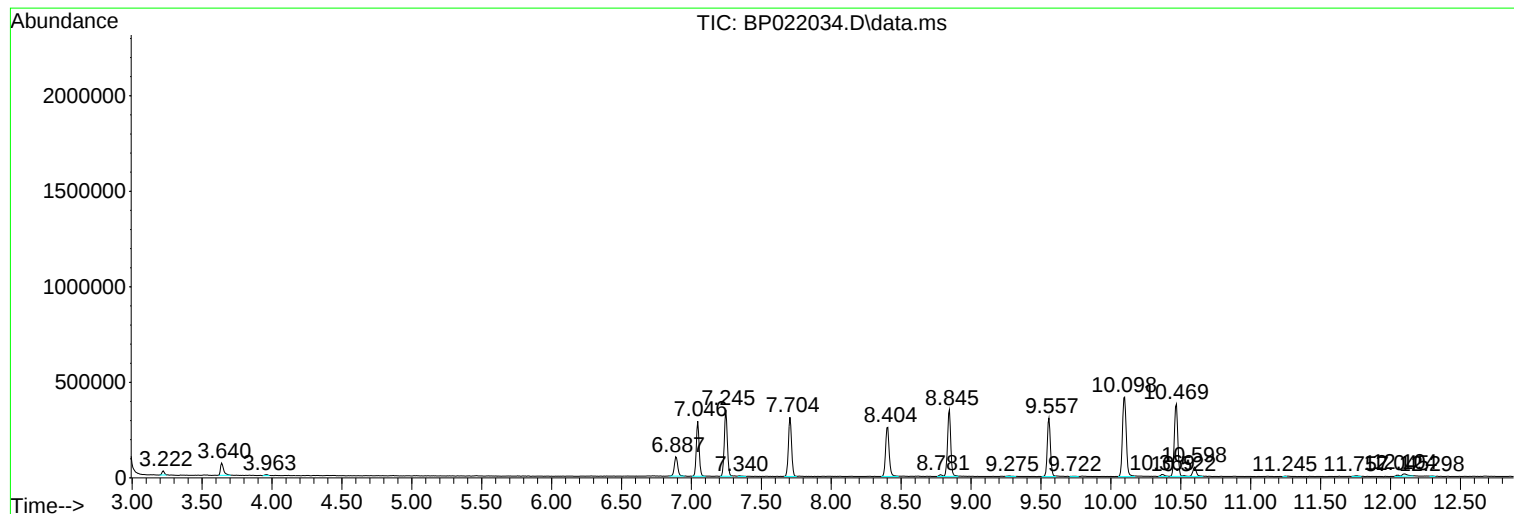

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022034.D
Acq On : 25 Sep 2024 18:48
Operator : RC/JU
Sample : P4013-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022034.D
Acq On : 25 Sep 2024 18:48
Operator : RC/JU
Sample : P4013-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc