

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022036.D
 Acq On : 25 Sep 2024 20:10
 Operator : RC/JU
 Sample : P4013-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	44	rVB	23077	28489	0.80%	0.110%
2	3.640	107	111	124	rVB	62668	101858	2.86%	0.393%
3	3.958	162	165	169	rVB3	4262	5222	0.15%	0.020%
4	5.228	377	381	387	rBV6	2233	4280	0.12%	0.017%
5	6.893	656	664	673	rBV	122213	207241	5.82%	0.799%
6	7.046	683	690	698	rBV	333231	501234	14.07%	1.933%
7	7.252	718	725	734	rBV	391693	648810	18.21%	2.503%
8	7.334	736	739	745	rVB8	2796	4422	0.12%	0.017%
9	7.711	794	803	812	rBV	277994	445578	12.50%	1.719%
10	8.405	912	921	932	rBV	339629	555014	15.58%	2.141%
11	8.846	987	996	1005	rBV	417733	686027	19.25%	2.646%
12	9.558	1109	1117	1130	rBV	402541	611274	17.16%	2.358%
13	9.810	1155	1160	1162	rBV6	3323	4796	0.13%	0.018%
14	10.099	1200	1209	1223	rBV	539999	945325	26.53%	3.646%
15	10.469	1263	1272	1281	rBV	321074	583757	16.38%	2.252%
16	10.599	1289	1294	1306	rBV	32880	56958	1.60%	0.220%
17	11.269	1403	1408	1411	rBV6	3768	6474	0.18%	0.025%
18	12.051	1535	1541	1550	rVB4	7313	14834	0.42%	0.057%
19	12.675	1642	1647	1650	rBV7	2454	3852	0.11%	0.015%
20	13.722	1818	1825	1836	rBV	1002118	1465878	41.14%	5.654%
21	14.010	1865	1874	1884	rBV	807823	1318107	36.99%	5.084%
22	14.322	1919	1927	1936	rBV	542299	854558	23.98%	3.296%
23	14.534	1955	1963	1975	rBV	93061	193699	5.44%	0.747%
24	14.740	1994	1998	2006	rBV3	20667	29443	0.83%	0.114%
25	15.140	2062	2066	2073	rVB6	4032	6741	0.19%	0.026%
26	15.322	2089	2097	2105	rBV	1376689	2123867	59.61%	8.192%
27	15.434	2111	2116	2128	rBV	500345	646923	18.16%	2.495%
28	15.563	2134	2138	2145	rVB5	7241	11425	0.32%	0.044%
29	16.045	2214	2220	2226	rBV3	10278	19210	0.54%	0.074%
30	16.787	2341	2346	2349	rBV7	2453	4436	0.12%	0.017%
31	16.892	2360	2364	2367	rVB5	2972	4513	0.13%	0.017%
32	17.110	2395	2401	2411	rBV	896091	1183054	33.20%	4.563%
33	17.216	2412	2419	2433	rVB	1517854	2469895	69.32%	9.527%
34	17.410	2449	2452	2454	rBV4	3604	4229	0.12%	0.016%
35	17.816	2517	2521	2523	rBV5	6075	7469	0.21%	0.029%
36	18.057	2558	2562	2568	rBV5	17457	24404	0.68%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022036.D
Acq On : 25 Sep 2024 20:10
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	18.122	2570	2573	2579	rVV	7669	10967	0.31%	0.042%
38	19.139	2741	2746	2753	rVB3	22410	37833	1.06%	0.146%
39	19.216	2755	2759	2763	rBV2	23848	32684	0.92%	0.126%
40	19.386	2785	2788	2793	rVB6	12929	15684	0.44%	0.060%
41	19.592	2817	2823	2831	rBV	2370247	3175077	89.11%	12.247%
42	21.539	3148	3154	3162	rVB2	963029	1534196	43.06%	5.918%
43	24.586	3663	3672	3688	rVB2	1163828	3563211	100.00%	13.744%
44	24.816	3702	3711	3723	rBV	706590	1771870	49.73%	6.835%




Sum of corrected areas: 25924818

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022036.D
Acq On : 25 Sep 2024 20:10
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

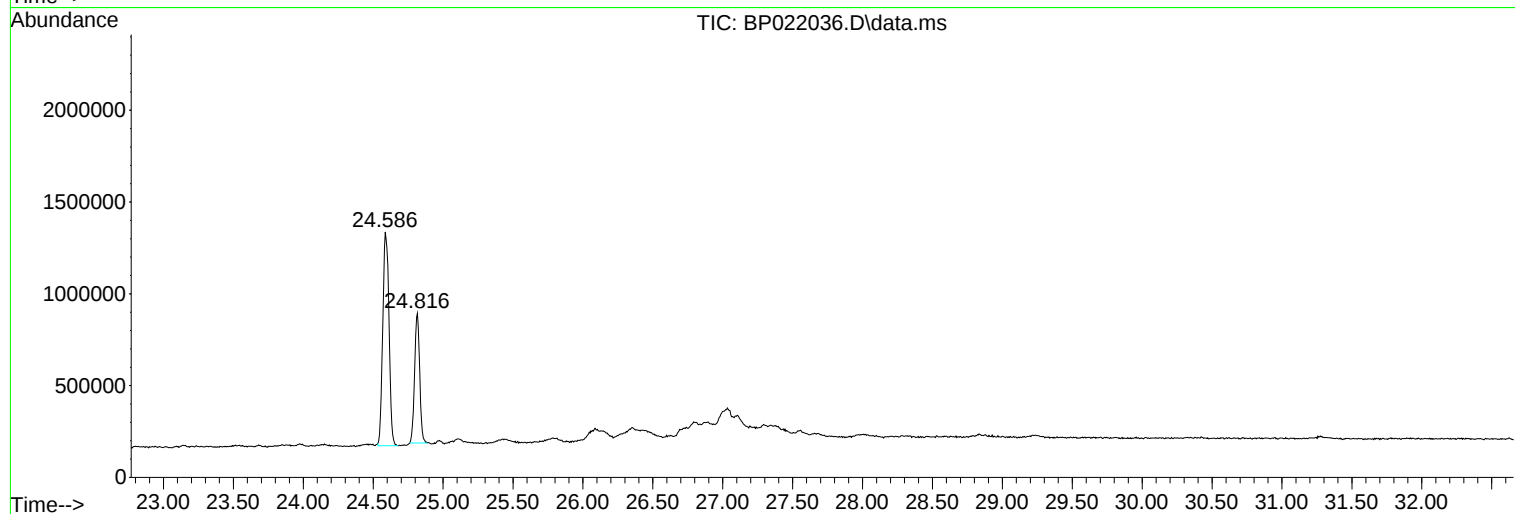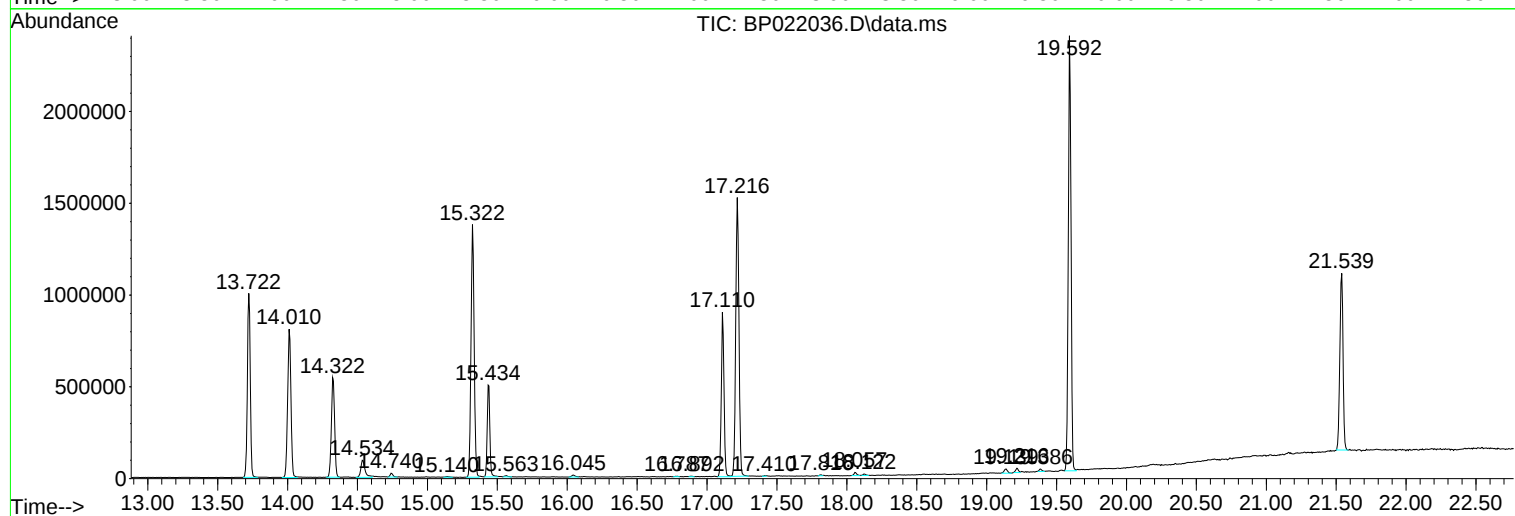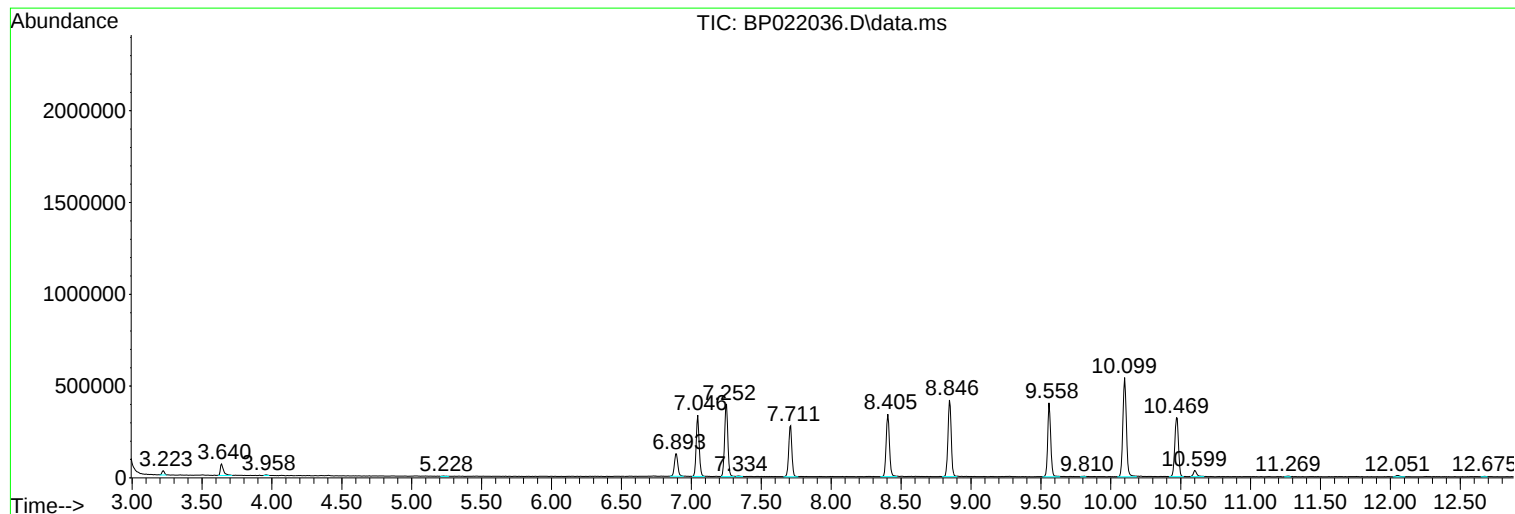

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022036.D
Acq On : 25 Sep 2024 20:10
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022036.D
Acq On : 25 Sep 2024 20:10
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc