

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022037.D
 Acq On : 25 Sep 2024 20:51
 Operator : RC/JU
 Sample : P4013-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	45	rBV	22616	32211	0.92%	0.117%
2	3.640	107	111	120	rBV	57327	85543	2.44%	0.312%
3	3.958	160	165	172	rVB3	7021	11754	0.34%	0.043%
4	4.087	184	187	191	rBV6	4376	6578	0.19%	0.024%
5	4.152	193	198	203	rVV3	7038	10070	0.29%	0.037%
6	4.264	212	217	219	rBV6	2545	3803	0.11%	0.014%
7	4.317	223	226	229	rVB5	4234	4976	0.14%	0.018%
8	5.452	412	419	423	rBV8	1638	3675	0.10%	0.013%
9	5.758	466	471	473	rBV5	3160	4246	0.12%	0.015%
10	5.787	473	476	482	rVB5	4963	7869	0.22%	0.029%
11	6.734	634	637	642	rVB7	2460	3547	0.10%	0.013%
12	6.893	653	664	673	rVB	125416	229825	6.55%	0.837%
13	7.046	682	690	697	rBV	341049	511420	14.58%	1.862%
14	7.105	697	700	705	rVV7	3341	4482	0.13%	0.016%
15	7.246	716	724	736	rBV	417335	653008	18.61%	2.378%
16	7.352	736	742	747	rVB10	2510	6618	0.19%	0.024%
17	7.705	795	802	809	rBV	324665	501530	14.30%	1.826%
18	8.405	914	921	932	rBV	328466	564753	16.10%	2.057%
19	8.846	988	996	1009	rVV	413512	684249	19.50%	2.492%
20	9.005	1020	1023	1031	rVB7	3252	6710	0.19%	0.024%
21	9.557	1105	1117	1124	rBV	357530	593259	16.91%	2.160%
22	9.804	1153	1159	1166	rBV10	3679	9272	0.26%	0.034%
23	10.099	1201	1209	1226	rBV	582332	954523	27.21%	3.476%
24	10.469	1262	1272	1286	rBV	384153	661928	18.87%	2.410%
25	10.599	1286	1294	1305	rBV	256858	465873	13.28%	1.697%
26	11.257	1398	1406	1413	rBV4	18380	36119	1.03%	0.132%
27	12.046	1533	1540	1546	rBV	9361	19240	0.55%	0.070%
28	13.722	1817	1825	1835	rBV	1093855	1494690	42.60%	5.443%
29	14.010	1865	1874	1884	rBV	1040388	1578159	44.98%	5.747%
30	14.316	1919	1926	1934	rBV	703192	974751	27.78%	3.550%
31	14.522	1955	1961	1975	rBV2	81488	177536	5.06%	0.647%
32	14.687	1985	1989	1995	rVB8	3517	6026	0.17%	0.022%
33	14.745	1995	1999	2005	rVB7	10924	16047	0.46%	0.058%
34	15.139	2061	2066	2071	rVB7	4729	9099	0.26%	0.033%
35	15.328	2090	2098	2108	rBV	1394145	2129932	60.71%	7.756%
36	15.451	2111	2119	2132	rVV	477578	636924	18.15%	2.319%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022037.D
 Acq On : 25 Sep 2024 20:51
 Operator : RC/JU
 Sample : P4013-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.569	2134	2139	2144	rVB2	7698	13769	0.39%	0.050%
38	15.704	2159	2162	2168	rVB7	2453	4315	0.12%	0.016%
39	15.904	2194	2196	2201	rVB5	2781	3719	0.11%	0.014%
40	16.039	2215	2219	2224	rBV6	3476	6723	0.19%	0.024%
41	16.792	2342	2347	2352	rBV9	3169	5052	0.14%	0.018%
42	16.886	2360	2363	2368	rVB4	4291	5841	0.17%	0.021%
43	17.122	2396	2403	2410	rBV	900141	1299175	37.03%	4.731%
44	17.216	2413	2419	2433	rVV	1950498	2491099	71.00%	9.072%
45	17.428	2451	2455	2460	rVB4	3548	5361	0.15%	0.020%
46	17.833	2520	2524	2531	rVB9	8281	12279	0.35%	0.045%
47	17.928	2537	2540	2542	rBV4	3522	4189	0.12%	0.015%
48	17.986	2547	2550	2556	rVV7	6907	10182	0.29%	0.037%
49	18.057	2557	2562	2570	rVV3	49013	83625	2.38%	0.305%
50	18.128	2571	2574	2581	rVB	10640	13227	0.38%	0.048%
51	18.539	2641	2644	2645	rBV3	4373	4120	0.12%	0.015%
52	19.133	2741	2745	2751	rVB3	25289	35635	1.02%	0.130%
53	19.216	2755	2759	2763	rVB	19930	30444	0.87%	0.111%
54	19.386	2784	2788	2798	rBV3	49019	79737	2.27%	0.290%
55	19.592	2816	2823	2831	rBV	2026451	3217779	91.72%	11.718%
56	21.539	3148	3154	3163	rBV	1135344	1706941	48.65%	6.216%
57	24.586	3663	3672	3684	rVB	1299085	3508345	100.00%	12.776%
58	24.821	3703	3712	3724	rVB	714682	1818891	51.84%	6.624%




Sum of corrected areas: 27460693

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022037.D
Acq On : 25 Sep 2024 20:51
Operator : RC/JU
Sample : P4013-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

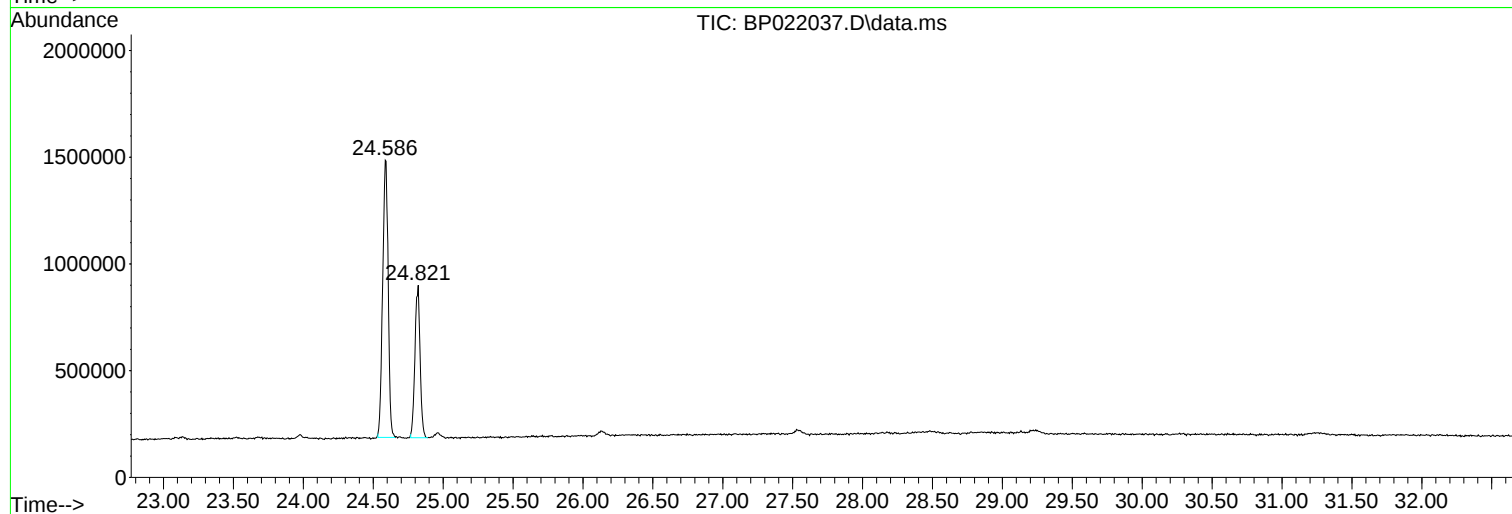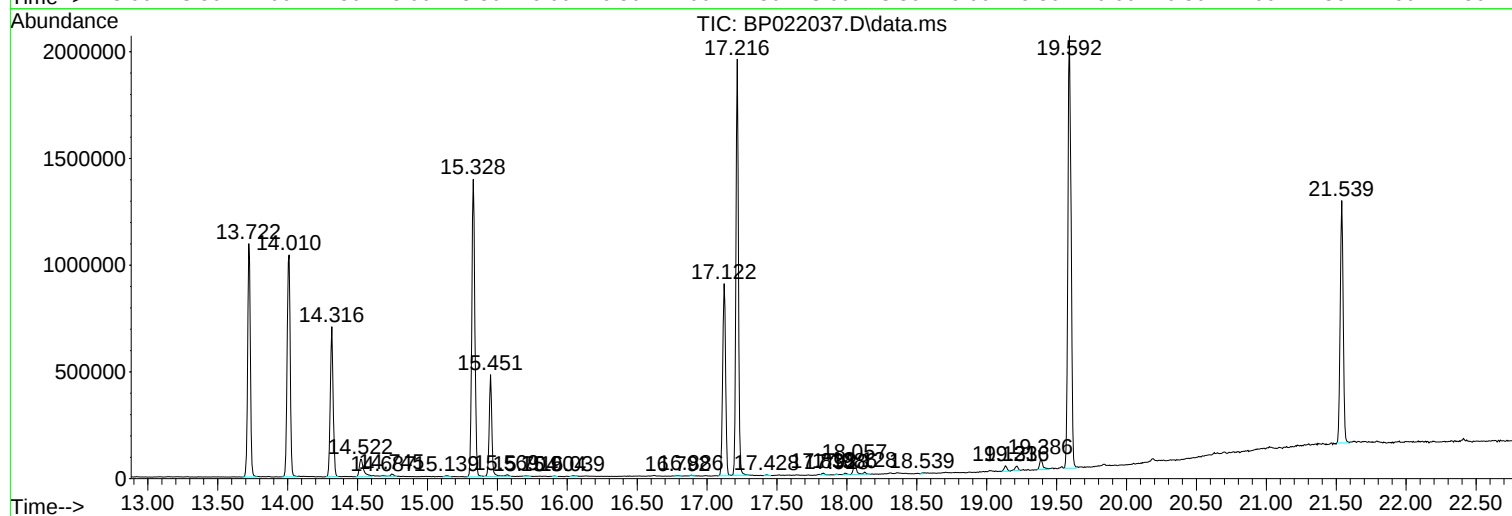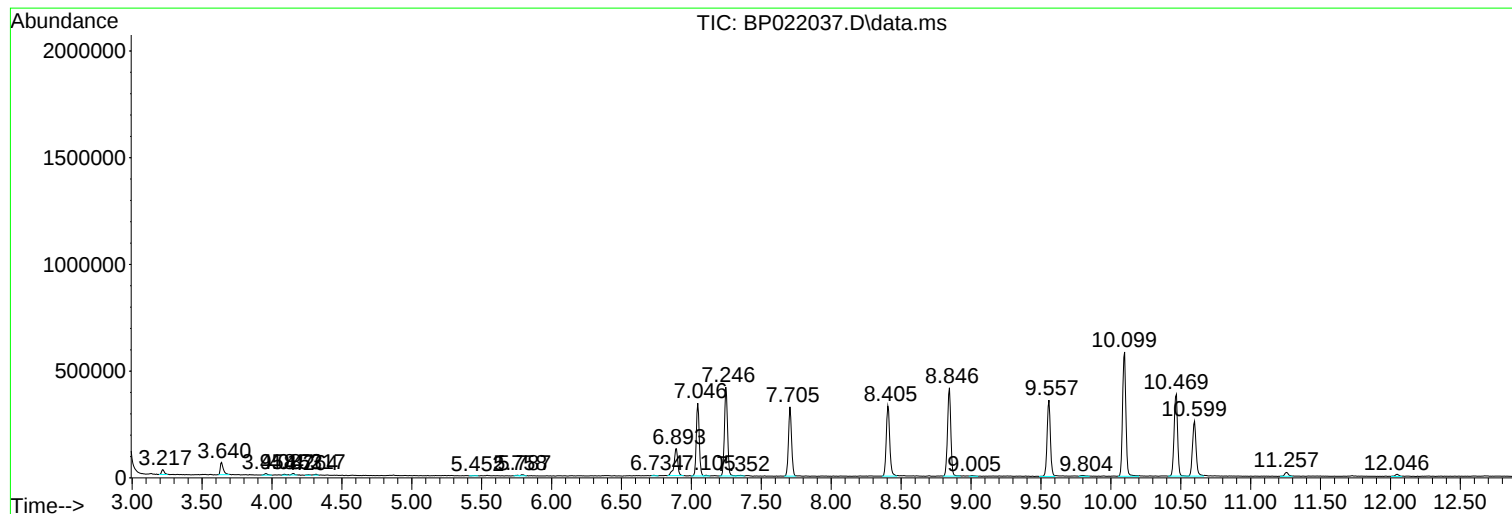

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022037.D
Acq On : 25 Sep 2024 20:51
Operator : RC/JU
Sample : P4013-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022037.D
Acq On : 25 Sep 2024 20:51
Operator : RC/JU
Sample : P4013-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc