

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022038.D
 Acq On : 25 Sep 2024 21:31
 Operator : RC/JU
 Sample : P4013-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	45	rBV	21687	26282	0.77%	0.096%
2	3.640	107	111	120	rBV	87684	139644	4.07%	0.512%
3	3.852	145	147	152	rVB5	3229	4156	0.12%	0.015%
4	3.958	162	165	169	rVB3	5435	7200	0.21%	0.026%
5	4.093	183	188	190	rBV6	4255	6318	0.18%	0.023%
6	4.152	193	198	206	rVB2	7212	10985	0.32%	0.040%
7	5.787	470	476	483	rVB8	4745	7169	0.21%	0.026%
8	6.887	653	663	673	rBV	114019	214888	6.26%	0.788%
9	7.046	682	690	697	rBV	302632	483693	14.08%	1.775%
10	7.099	697	699	704	rVB6	2830	3821	0.11%	0.014%
11	7.246	716	724	734	rBV	377806	614299	17.89%	2.254%
12	7.340	734	740	742	rVV6	2825	5173	0.15%	0.019%
13	7.399	746	750	755	rVB7	3065	5163	0.15%	0.019%
14	7.705	795	802	811	rBV	304696	486388	14.16%	1.784%
15	8.405	912	921	934	rBV	309865	508406	14.80%	1.865%
16	8.846	988	996	1005	rBV	406999	656514	19.12%	2.409%
17	9.005	1019	1023	1032	rVB	5920	10218	0.30%	0.037%
18	9.558	1106	1117	1126	rBV	336268	572749	16.68%	2.101%
19	9.793	1151	1157	1158	rBV6	3450	4197	0.12%	0.015%
20	10.093	1200	1208	1217	rBV	550694	904016	26.32%	3.317%
21	10.463	1263	1271	1281	rBV	374053	632095	18.41%	2.319%
22	10.599	1286	1294	1310	rBV	383234	710911	20.70%	2.608%
23	11.257	1399	1406	1416	rBV3	21090	41378	1.20%	0.152%
24	11.716	1477	1484	1492	rVB9	4480	9232	0.27%	0.034%
25	12.046	1535	1540	1547	rVB4	7675	12478	0.36%	0.046%
26	12.922	1682	1689	1694	rVB9	1968	3773	0.11%	0.014%
27	13.152	1726	1728	1733	rVB5	2392	3716	0.11%	0.014%
28	13.722	1817	1825	1836	rBV	1006089	1461886	42.57%	5.363%
29	14.004	1862	1873	1885	rBV	1079196	1553451	45.23%	5.699%
30	14.310	1918	1925	1932	rBV	675514	973124	28.34%	3.570%
31	14.534	1956	1963	1979	rBV	76592	178856	5.21%	0.656%
32	14.740	1993	1998	2005	rVB	8239	16135	0.47%	0.059%
33	15.140	2061	2066	2071	rBV7	4508	8788	0.26%	0.032%
34	15.322	2090	2097	2109	rBV	1550484	2105708	61.31%	7.725%
35	15.440	2109	2117	2128	rBV	440917	620752	18.08%	2.277%
36	15.569	2135	2139	2145	rVB5	6679	11420	0.33%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022038.D
 Acq On : 25 Sep 2024 21:31
 Operator : RC/JU
 Sample : P4013-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.687	2153	2159	2162	rBV8	3003	5438	0.16%	0.020%
38	15.904	2191	2196	2200	rBV8	2345	3782	0.11%	0.014%
39	16.034	2213	2218	2221	rBV4	4735	6344	0.18%	0.023%
40	16.651	2321	2323	2328	rVB5	3559	4719	0.14%	0.017%
41	16.769	2342	2343	2350	rVB6	3093	4404	0.13%	0.016%
42	16.892	2358	2364	2365	rBV5	2459	3645	0.11%	0.013%
43	17.040	2386	2389	2394	rBV6	3341	5263	0.15%	0.019%
44	17.110	2394	2401	2407	rVV	877101	1311400	38.19%	4.811%
45	17.210	2411	2418	2432	rVV2	1472004	2482747	72.29%	9.109%
46	17.410	2450	2452	2457	rVB4	2841	3538	0.10%	0.013%
47	17.810	2516	2520	2525	rVB7	4254	8357	0.24%	0.031%
48	17.992	2547	2551	2553	rBV5	7228	8238	0.24%	0.030%
49	18.051	2557	2561	2567	rBV3	23196	35555	1.04%	0.130%
50	18.122	2570	2573	2578	rVB	8852	12137	0.35%	0.045%
51	18.357	2611	2613	2618	rBV6	3560	5912	0.17%	0.022%
52	19.145	2742	2747	2751	rBV3	24317	36426	1.06%	0.134%
53	19.210	2754	2758	2763	rBV	24193	37523	1.09%	0.138%
54	19.375	2784	2786	2794	rVB8	15580	17595	0.51%	0.065%
55	19.545	2813	2815	2817	rBV3	6886	5757	0.17%	0.021%
56	19.592	2817	2823	2832	rVV	2283798	3204166	93.30%	11.755%
57	21.539	3148	3154	3164	rVB	1088612	1733592	50.48%	6.360%
58	24.598	3664	3674	3685	rVB	1352277	3434300	100.00%	12.600%
59	24.821	3703	3712	3725	rVB	638013	1871212	54.49%	6.865%




Sum of corrected areas: 27257032

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022038.D
Acq On : 25 Sep 2024 21:31
Operator : RC/JU
Sample : P4013-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

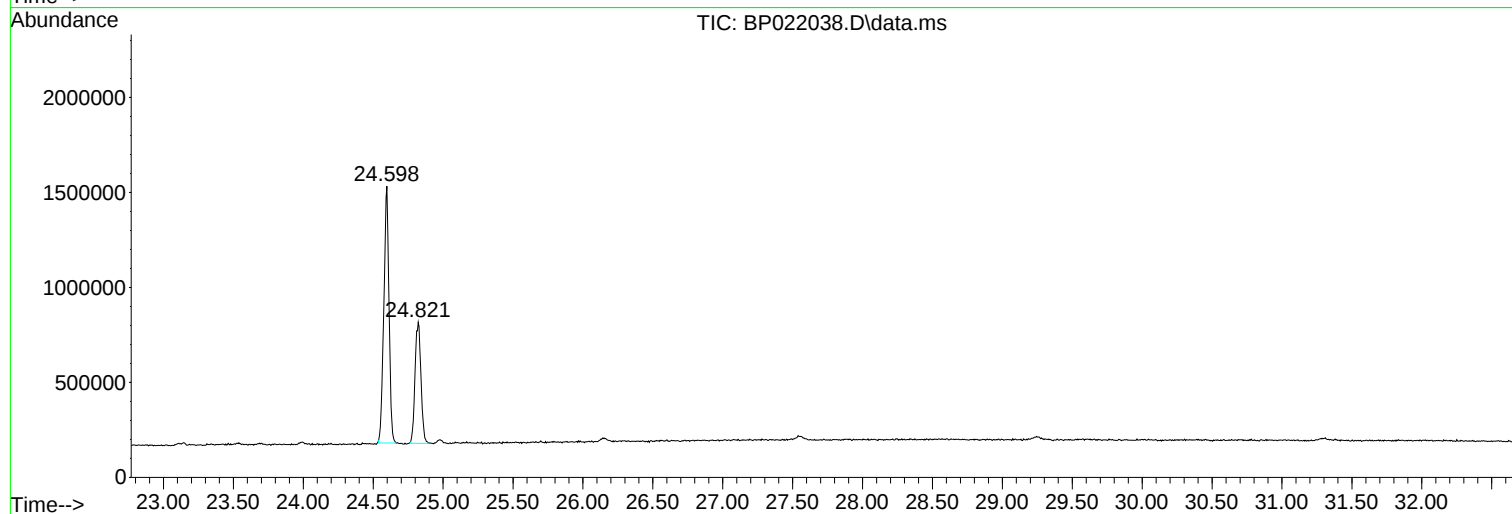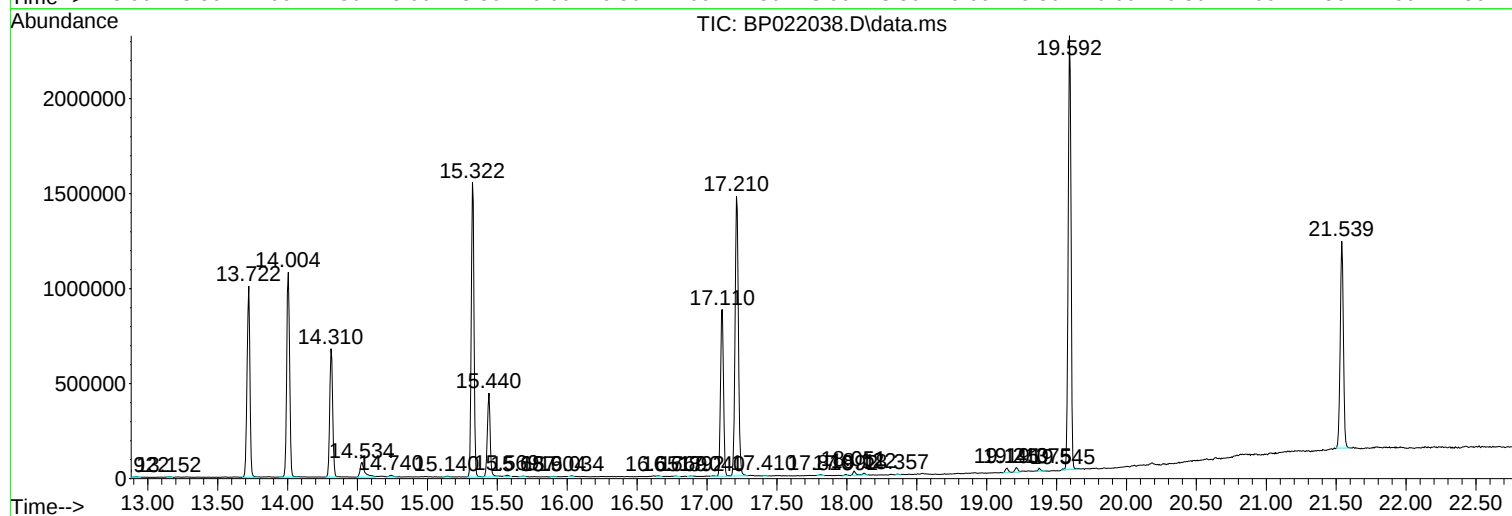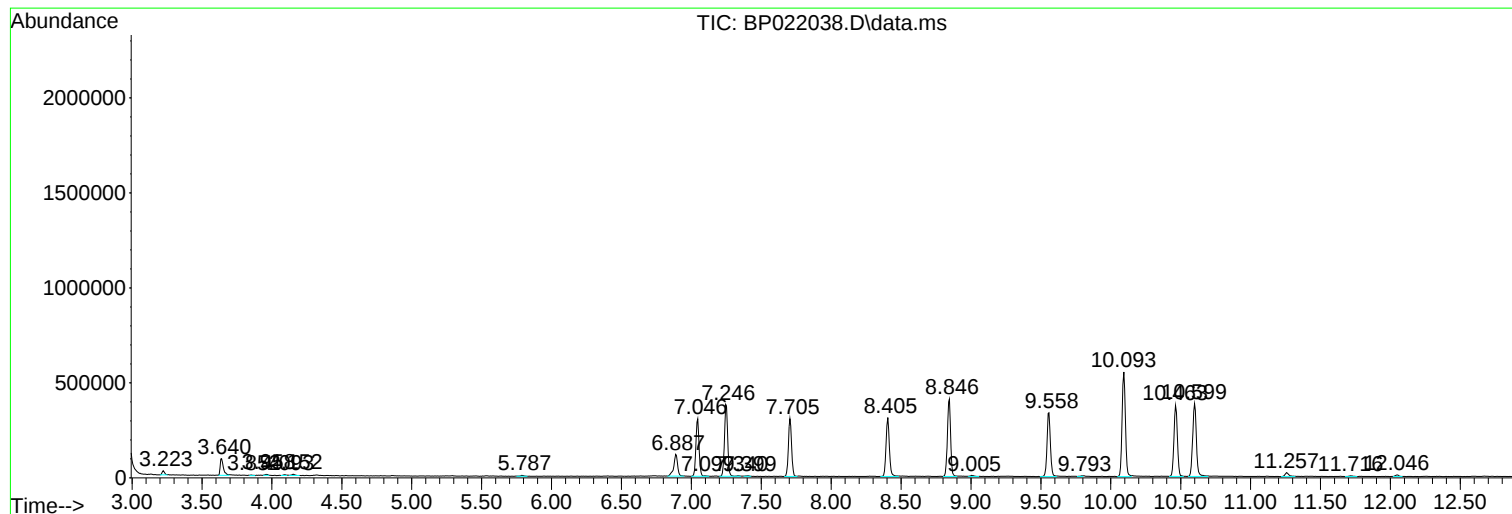

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022038.D
Acq On : 25 Sep 2024 21:31
Operator : RC/JU
Sample : P4013-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022038.D
Acq On : 25 Sep 2024 21:31
Operator : RC/JU
Sample : P4013-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------