

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022042.D
 Acq On : 26 Sep 2024 00:55
 Operator : RC/JU
 Sample : PB163459BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK459

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	35	40	46	rVB	36478	48863	1.17%	0.137%
2	3.634	105	110	125	rBV	418202	623286	14.96%	1.743%
3	3.958	159	165	176	rBV2	12038	20412	0.49%	0.057%
4	6.887	656	663	674	rVB	503292	819418	19.66%	2.291%
5	7.046	683	690	702	rVV	395776	613965	14.73%	1.716%
6	7.246	717	724	735	rBV	507993	832146	19.97%	2.326%
7	7.705	793	802	812	rBV	408321	623623	14.96%	1.743%
8	8.146	873	877	886	rBV	2228	5423	0.13%	0.015%
9	8.405	914	921	934	rBV2	627083	1044933	25.07%	2.921%
10	8.516	936	940	944	rVB7	5142	9536	0.23%	0.027%
11	8.846	987	996	1011	rBV	529397	836001	20.06%	2.337%
12	9.410	1089	1092	1096	rBV3	3517	4578	0.11%	0.013%
13	9.558	1110	1117	1128	rBV	426254	712352	17.09%	1.992%
14	9.881	1166	1172	1180	rVB7	2670	6153	0.15%	0.017%
15	10.093	1198	1208	1218	rBV	672325	1153813	27.69%	3.226%
16	10.163	1218	1220	1225	rVB6	3324	4640	0.11%	0.013%
17	10.463	1264	1271	1279	rBV	498053	832583	19.98%	2.328%
18	10.599	1286	1294	1312	rBV	593050	1061387	25.47%	2.967%
19	10.793	1323	1327	1335	rVB9	4765	9068	0.22%	0.025%
20	12.046	1535	1540	1547	rBV2	10901	18786	0.45%	0.053%
21	12.122	1547	1553	1561	rVB4	4281	8473	0.20%	0.024%
22	12.346	1585	1591	1595	rBV3	5964	10647	0.26%	0.030%
23	12.493	1608	1616	1621	rBV10	4492	10129	0.24%	0.028%
24	12.746	1656	1659	1665	rVB6	3298	4480	0.11%	0.013%
25	13.104	1713	1720	1723	rBV6	5241	8960	0.21%	0.025%
26	13.134	1723	1725	1729	rVV3	5659	8695	0.21%	0.024%
27	13.181	1729	1733	1739	rVB3	4724	9149	0.22%	0.026%
28	13.722	1818	1825	1831	rBV	1238793	1765545	42.36%	4.936%
29	13.887	1847	1853	1857	rVB9	2848	5185	0.12%	0.014%
30	14.004	1865	1873	1883	rBV	1279815	1969640	47.26%	5.506%
31	14.310	1918	1925	1932	rBV	841890	1218116	29.23%	3.405%
32	14.375	1932	1936	1941	rVB4	7666	12687	0.30%	0.035%
33	14.516	1954	1960	1970	rBV	560607	839472	20.14%	2.347%
34	14.628	1977	1979	1984	rVB6	7119	9061	0.22%	0.025%
35	14.728	1993	1996	1997	rBV2	4648	5592	0.13%	0.016%
36	14.951	2029	2034	2040	rBV10	4440	9114	0.22%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022042.D
 Acq On : 26 Sep 2024 00:55
 Operator : RC/JU
 Sample : PB163459BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK459

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.151	2061	2068	2071	rBV	7269	10860	0.26%	0.030%
38	15.322	2090	2097	2103	rBV	1976981	2589525	62.13%	7.239%
39	15.381	2103	2107	2113	rVV3	13239	22780	0.55%	0.064%
40	15.451	2113	2119	2128	rVV	558973	739560	17.75%	2.068%
41	15.569	2135	2139	2142	rBV2	7871	13270	0.32%	0.037%
42	16.128	2227	2234	2239	rBV8	5415	9259	0.22%	0.026%
43	16.281	2255	2260	2265	rBV7	7249	11193	0.27%	0.031%
44	16.398	2276	2280	2288	rVB8	6676	12686	0.30%	0.035%
45	16.569	2305	2309	2314	rBV7	4302	7680	0.18%	0.021%
46	16.757	2335	2341	2344	rBV7	4701	8999	0.22%	0.025%
47	16.892	2359	2364	2366	rBV5	3372	5100	0.12%	0.014%
48	17.110	2395	2401	2407	rBV	1196923	1647558	39.53%	4.606%
49	17.210	2412	2418	2432	rVB2	2035672	3087816	74.09%	8.633%
50	17.539	2471	2474	2479	rVB2	4798	7790	0.19%	0.022%
51	17.816	2516	2521	2525	rBV7	5138	8572	0.21%	0.024%
52	18.122	2571	2573	2578	rVB	7883	7484	0.18%	0.021%
53	19.133	2740	2745	2751	rVB4	23875	43544	1.04%	0.122%
54	19.216	2754	2759	2762	rBV2	21999	36841	0.88%	0.103%
55	19.586	2816	2822	2833	rBV2	2429894	3901419	93.61%	10.907%
56	21.539	3148	3154	3161	rBV	1281931	2117690	50.81%	5.920%
57	24.604	3665	3675	3691	rVB	1458900	4167602	100.00%	11.651%
58	24.827	3705	3713	3727	rVB	850434	2136392	51.26%	5.973%




Sum of corrected areas: 35769531

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022042.D
Acq On : 26 Sep 2024 00:55
Operator : RC/JU
Sample : PB163459BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK459

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

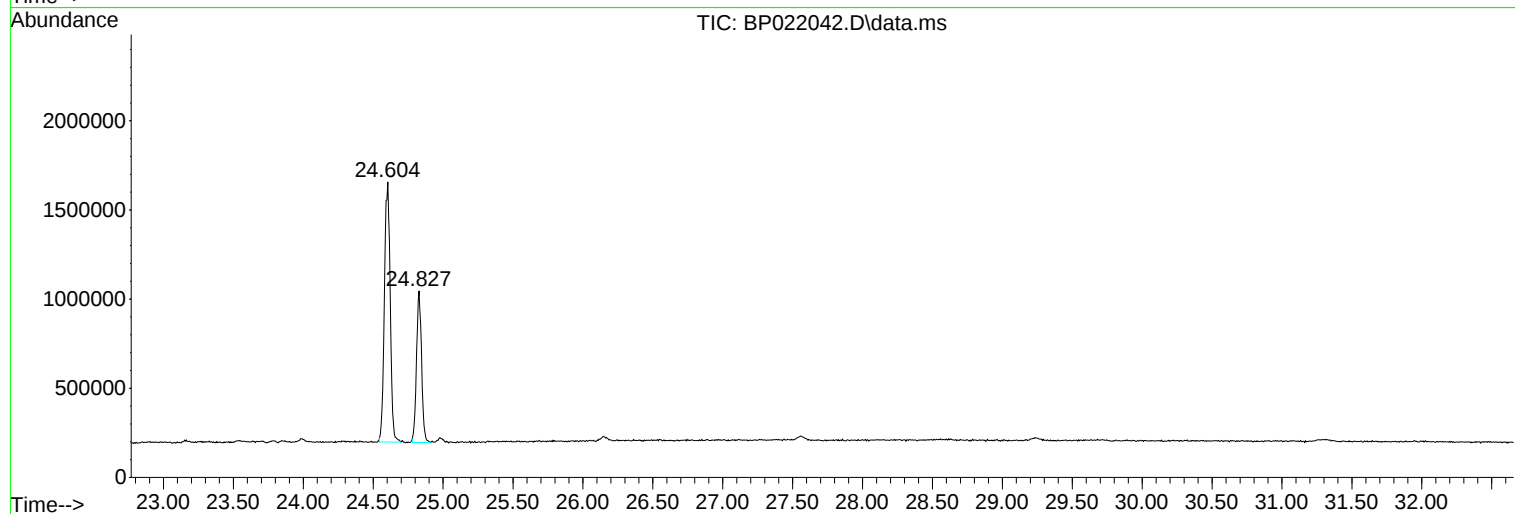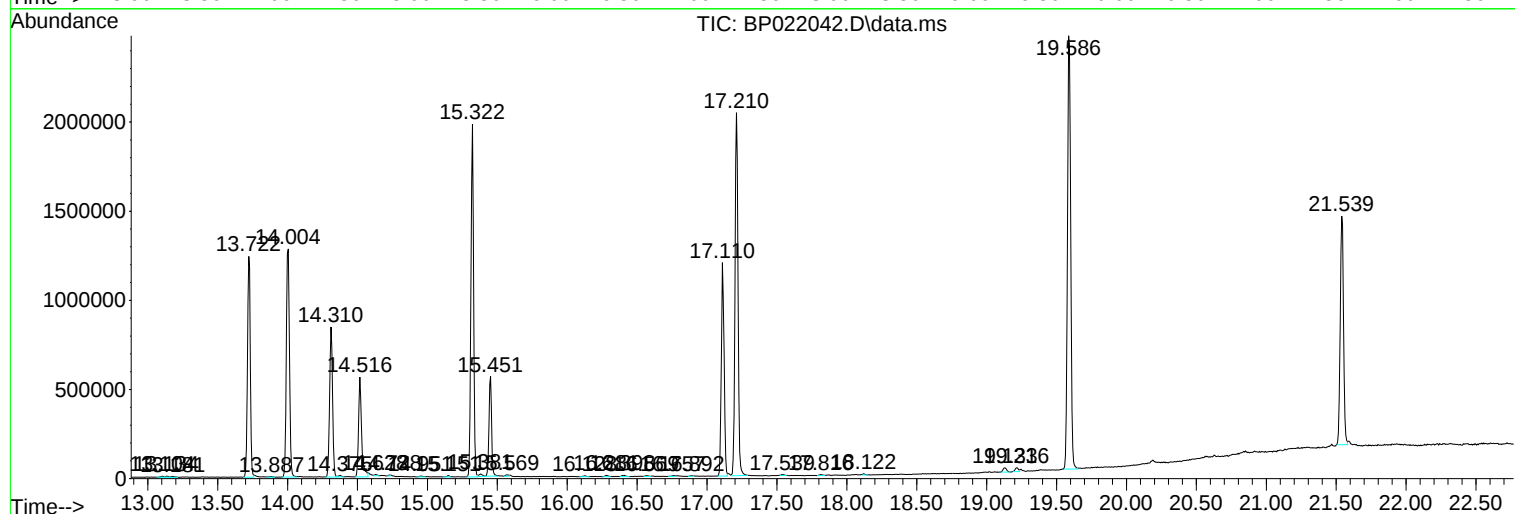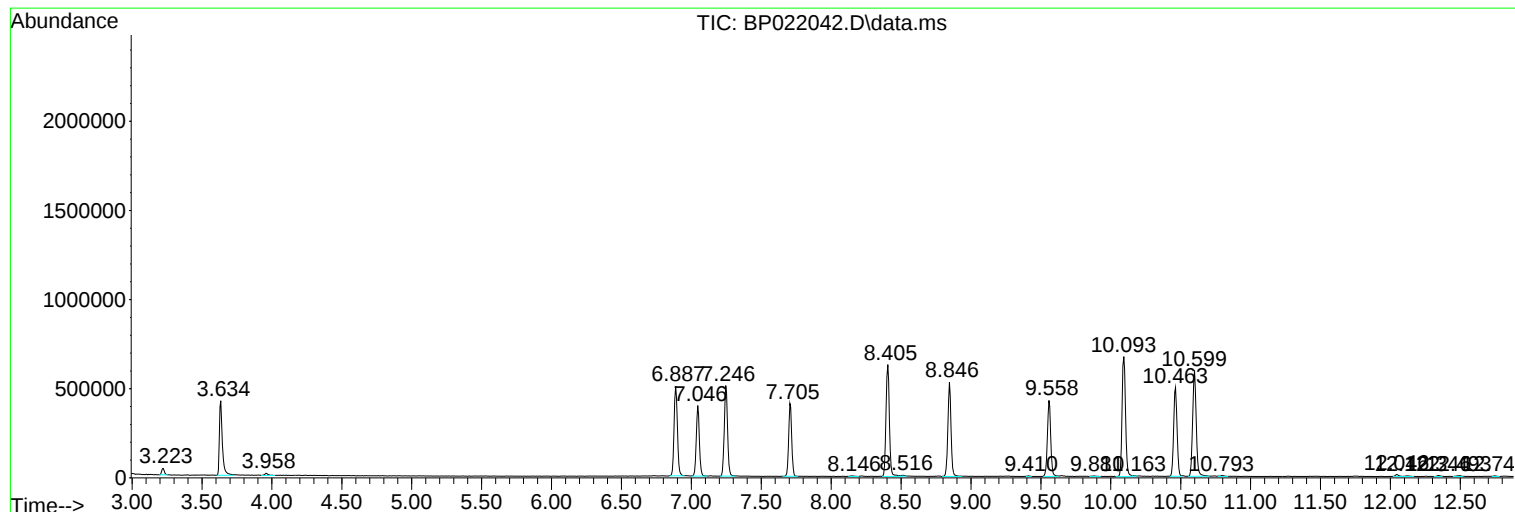

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022042.D
Acq On : 26 Sep 2024 00:55
Operator : RC/JU
Sample : PB163459BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK459

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022042.D
Acq On : 26 Sep 2024 00:55
Operator : RC/JU
Sample : PB163459BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK459

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------