

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022045.D
 Acq On : 26 Sep 2024 02:58
 Operator : RC/JU
 Sample : P4106-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COSX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	45	rBV	19210	24444	0.75%	0.100%
2	3.640	107	111	120	rBV	47210	74704	2.30%	0.304%
3	3.958	160	165	171	rBV5	5022	8612	0.26%	0.035%
4	4.258	212	216	219	rBV6	2806	4878	0.15%	0.020%
5	4.870	313	320	324	rVB7	2769	5930	0.18%	0.024%
6	6.134	531	535	542	rVB7	3755	6511	0.20%	0.027%
7	6.887	654	663	672	rBV	102645	168872	5.19%	0.688%
8	7.046	684	690	698	rBV	290890	424951	13.07%	1.730%
9	7.246	717	724	737	rBV	336344	546307	16.80%	2.225%
10	7.705	794	802	811	rBV	283965	453791	13.96%	1.848%
11	8.052	854	861	866	rBV6	3133	6022	0.19%	0.025%
12	8.305	896	904	912	rBV6	3836	9520	0.29%	0.039%
13	8.399	913	920	932	rBV	284733	478264	14.71%	1.948%
14	8.846	987	996	1013	rVB	354843	607322	18.68%	2.473%
15	9.275	1061	1069	1081	rVB5	5756	13979	0.43%	0.057%
16	9.405	1086	1091	1099	rVB9	3070	6161	0.19%	0.025%
17	9.558	1109	1117	1127	rBV	312165	527998	16.24%	2.150%
18	10.093	1200	1208	1222	rBV	480491	822982	25.31%	3.351%
19	10.328	1242	1248	1253	rBV5	7800	12061	0.37%	0.049%
20	10.463	1263	1271	1285	rBV	337824	590437	18.16%	2.404%
21	10.599	1287	1294	1307	rBV2	57232	111654	3.43%	0.455%
22	10.852	1331	1337	1347	rVB6	4404	10491	0.32%	0.043%
23	11.063	1368	1373	1379	rVB10	2805	5003	0.15%	0.020%
24	11.263	1403	1407	1412	rVB7	2837	5153	0.16%	0.021%
25	11.752	1482	1490	1496	rBV2	23156	36642	1.13%	0.149%
26	12.052	1532	1541	1546	rBV3	6623	12334	0.38%	0.050%
27	12.446	1601	1608	1612	rBV7	3770	8359	0.26%	0.034%
28	12.493	1612	1616	1623	rVB9	3209	5657	0.17%	0.023%
29	12.734	1652	1657	1661	rVB8	2559	3773	0.12%	0.015%
30	12.928	1685	1690	1693	rBV4	3403	4171	0.13%	0.017%
31	13.110	1715	1721	1728	rBV4	16927	32241	0.99%	0.131%
32	13.316	1751	1756	1761	rBV	8163	11710	0.36%	0.048%
33	13.716	1815	1824	1840	rBV	917495	1353110	41.62%	5.510%
34	13.999	1864	1872	1881	rBV	922457	1377930	42.38%	5.611%
35	14.310	1918	1925	1933	rBV	560764	887627	27.30%	3.614%
36	14.528	1956	1962	1978	rBV	70069	161974	4.98%	0.660%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022045.D
 Acq On : 26 Sep 2024 02:58
 Operator : RC/JU
 Sample : P4106-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COSX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	14.728	1990	1996	2006	rVB	3848	13113	0.40%	0.053%
38	15.316	2088	2096	2109	rBV	1294744	1947109	59.89%	7.929%
39	15.440	2109	2117	2131	rVV	374178	630024	19.38%	2.565%
40	15.563	2135	2138	2148	rVB5	6493	13254	0.41%	0.054%
41	15.687	2153	2159	2167	rVB	19723	32729	1.01%	0.133%
42	16.275	2255	2259	2263	rBV7	2459	4401	0.14%	0.018%
43	16.604	2311	2315	2320	rVB7	2951	4392	0.14%	0.018%
44	16.757	2338	2341	2350	rVB7	3285	7486	0.23%	0.030%
45	17.104	2392	2400	2410	rBV	897104	1206184	37.10%	4.912%
46	17.210	2410	2418	2431	rVV	1498665	2305055	70.90%	9.386%
47	18.045	2555	2560	2567	rBV5	21616	33092	1.02%	0.135%
48	18.528	2636	2642	2648	rBV4	62249	84453	2.60%	0.344%
49	19.134	2741	2745	2751	rVB2	19109	28917	0.89%	0.118%
50	19.210	2754	2758	2762	rBV2	19856	28984	0.89%	0.118%
51	19.375	2784	2786	2792	rVB7	8908	11481	0.35%	0.047%
52	19.586	2816	2822	2831	rBV	2338716	2921185	89.85%	11.895%
53	21.533	3146	3153	3161	rVB2	842998	1538074	47.31%	6.263%
54	24.604	3665	3675	3689	rVB	1325430	3251040	100.00%	13.238%
55	24.816	3703	3711	3724	rVB	604697	1675175	51.53%	6.821%




Sum of corrected areas: 24557723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022045.D
Acq On : 26 Sep 2024 02:58
Operator : RC/JU
Sample : P4106-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

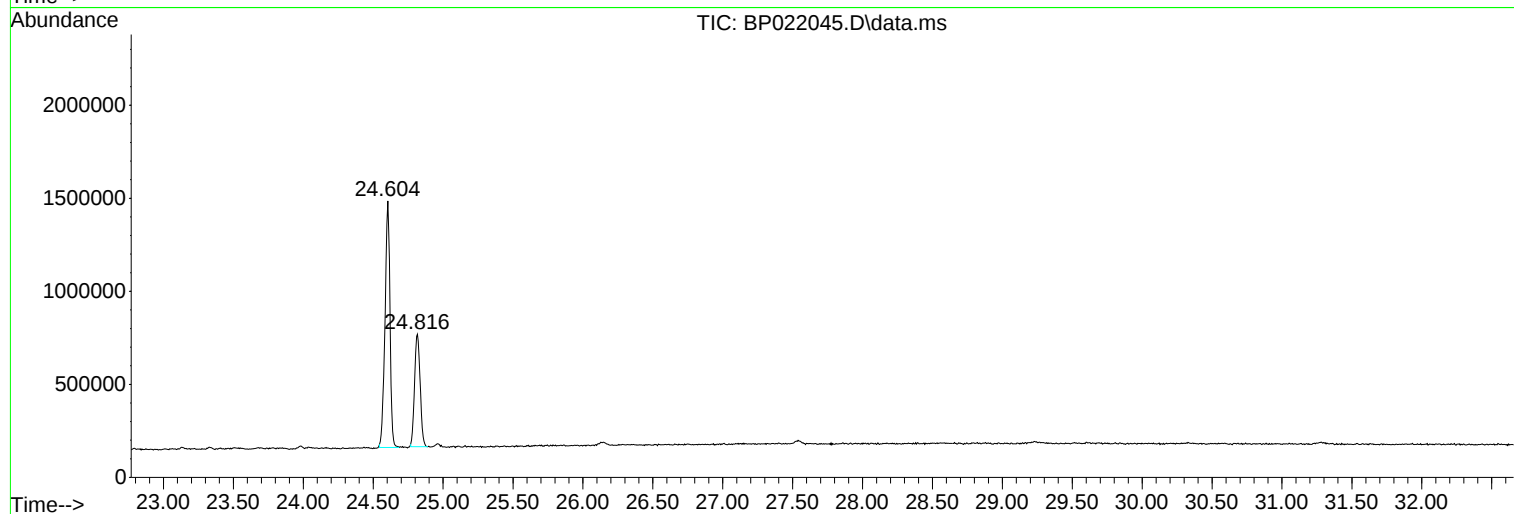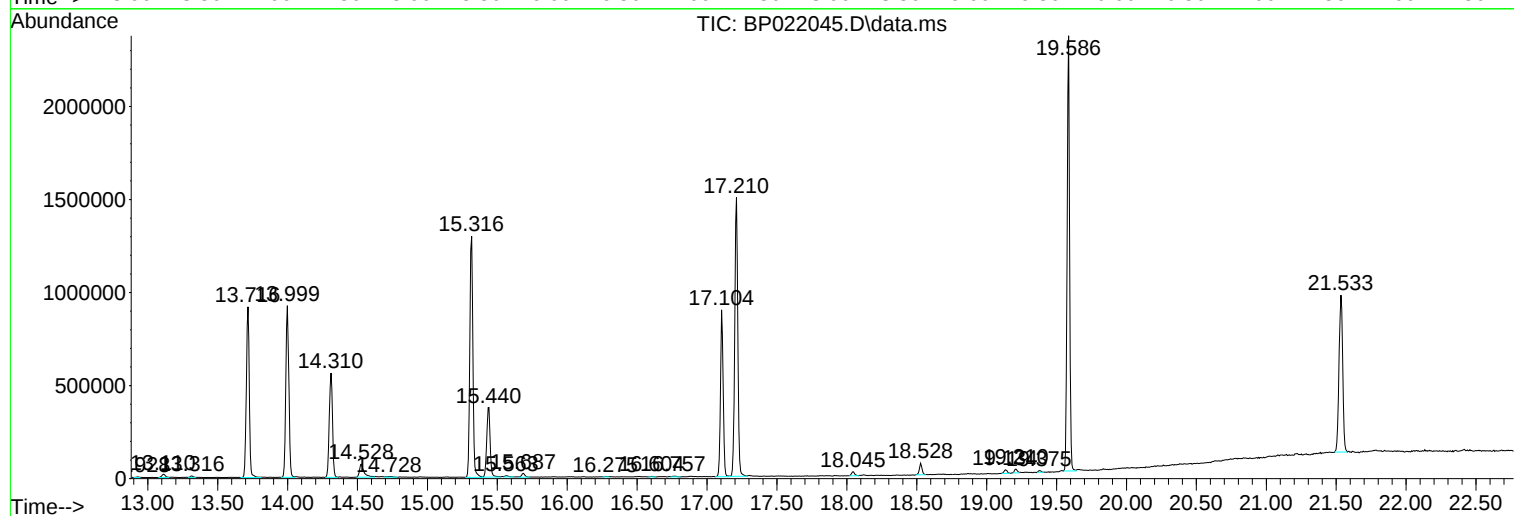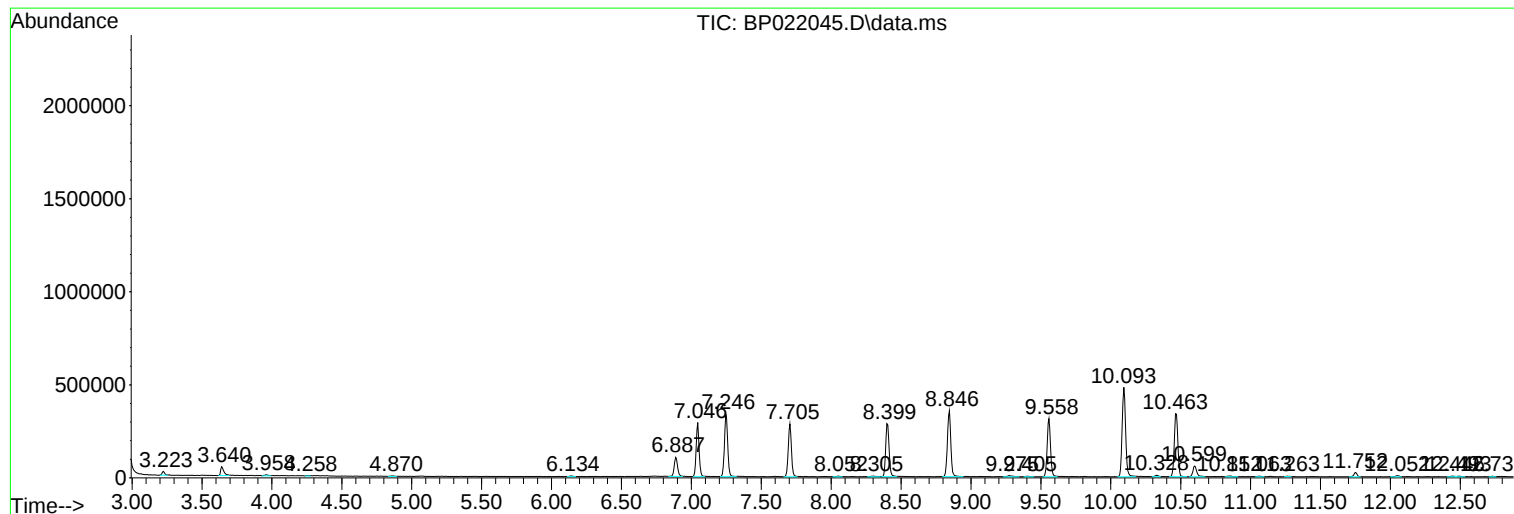

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022045.D
Acq On : 26 Sep 2024 02:58
Operator : RC/JU
Sample : P4106-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022045.D
Acq On : 26 Sep 2024 02:58
Operator : RC/JU
Sample : P4106-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0SX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc