

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022052.D
 Acq On : 26 Sep 2024 07:43
 Operator : RC/JU
 Sample : P4107-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	38	rBV	38138	49709	1.95%	0.218%
2	3.222	38	40	44	rVV	22413	26428	1.04%	0.116%
3	3.258	44	46	49	rVB2	6688	5889	0.23%	0.026%
4	3.364	62	64	69	rVB6	2542	3273	0.13%	0.014%
5	3.499	84	87	91	rBV6	2119	3420	0.13%	0.015%
6	3.640	107	111	123	rBV	101237	156068	6.12%	0.685%
7	3.964	162	166	171	rVB	5945	8741	0.34%	0.038%
8	4.481	249	254	264	rVB	51908	73153	2.87%	0.321%
9	4.869	315	320	325	rBV6	2509	3865	0.15%	0.017%
10	5.069	348	354	358	rBV3	9433	15705	0.62%	0.069%
11	6.887	657	663	677	rVB	96800	162268	6.36%	0.712%
12	7.046	681	690	700	rBV	224464	355102	13.92%	1.559%
13	7.246	716	724	737	rBV	292937	483687	18.97%	2.123%
14	7.705	795	802	815	rBV	297477	483089	18.94%	2.120%
15	8.052	853	861	867	rBV4	8846	16531	0.65%	0.073%
16	8.405	914	921	934	rBV	293922	464427	18.21%	2.038%
17	8.840	988	995	1003	rBV	292536	478920	18.78%	2.102%
18	9.557	1110	1117	1125	rBV	250589	416862	16.35%	1.830%
19	9.646	1130	1132	1138	rVV6	1506	2702	0.11%	0.012%
20	9.722	1142	1145	1152	rVB9	1664	2858	0.11%	0.013%
21	10.093	1201	1208	1223	rBV	376226	687121	26.94%	3.016%
22	10.328	1242	1248	1255	rVB9	3920	7208	0.28%	0.032%
23	10.469	1264	1272	1280	rBV	355703	641805	25.17%	2.817%
24	10.599	1286	1294	1306	rBV	513793	799891	31.37%	3.511%
25	11.269	1403	1408	1411	rBV7	1510	2837	0.11%	0.012%
26	11.746	1487	1489	1494	rVB6	1991	2790	0.11%	0.012%
27	12.051	1534	1541	1551	rVB3	6144	12383	0.49%	0.054%
28	12.922	1684	1689	1698	rVB4	4688	8370	0.33%	0.037%
29	13.710	1816	1823	1831	rBV	825718	1119666	43.90%	4.914%
30	13.998	1866	1872	1885	rBV2	724874	1159949	45.48%	5.091%
31	14.322	1919	1927	1934	rBV	620738	1006495	39.47%	4.418%
32	14.539	1955	1964	1977	rBV3	58329	145090	5.69%	0.637%
33	14.622	1977	1978	1986	rVV8	6118	12246	0.48%	0.054%
34	14.687	1986	1989	1992	rVV5	3727	5930	0.23%	0.026%
35	14.739	1995	1998	2002	rVB5	4764	7421	0.29%	0.033%
36	15.157	2062	2069	2073	rVB9	1682	4062	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022052.D
 Acq On : 26 Sep 2024 07:43
 Operator : RC/JU
 Sample : P4107-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.322	2086	2097	2105	rBV	998660	1595905	62.58%	7.005%
38	15.434	2110	2116	2131	rVV	343735	468667	18.38%	2.057%
39	15.557	2135	2137	2144	rVB7	3795	5896	0.23%	0.026%
40	16.775	2337	2344	2348	rVB10	3258	6232	0.24%	0.027%
41	16.886	2357	2363	2366	rBV7	2413	4802	0.19%	0.021%
42	16.992	2377	2381	2385	rBV7	2170	2907	0.11%	0.013%
43	17.104	2394	2400	2411	rBV	1047221	1386077	54.35%	6.084%
44	17.210	2411	2418	2430	rVB2	1134032	1829127	71.72%	8.028%
45	17.710	2500	2503	2506	rBV4	2811	4338	0.17%	0.019%
46	18.051	2556	2561	2566	rBV6	14560	21682	0.85%	0.095%
47	18.122	2570	2573	2575	rBV4	3606	4744	0.19%	0.021%
48	19.139	2742	2746	2750	rVB3	17707	25754	1.01%	0.113%
49	19.210	2754	2758	2764	rVV	19597	30261	1.19%	0.133%
50	19.375	2784	2786	2791	rBV5	8156	10431	0.41%	0.046%
51	19.586	2816	2822	2832	rBV	1862549	2379523	93.31%	10.444%
52	21.533	3147	3153	3164	rVB	1097786	1735400	68.05%	7.617%
53	24.592	3664	3673	3687	rVB	1001167	2550220	100.00%	11.193%
54	24.810	3702	3710	3722	rVB	729327	1885160	73.92%	8.274%




Sum of corrected areas: 22783087

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022052.D
Acq On : 26 Sep 2024 07:43
Operator : RC/JU
Sample : P4107-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

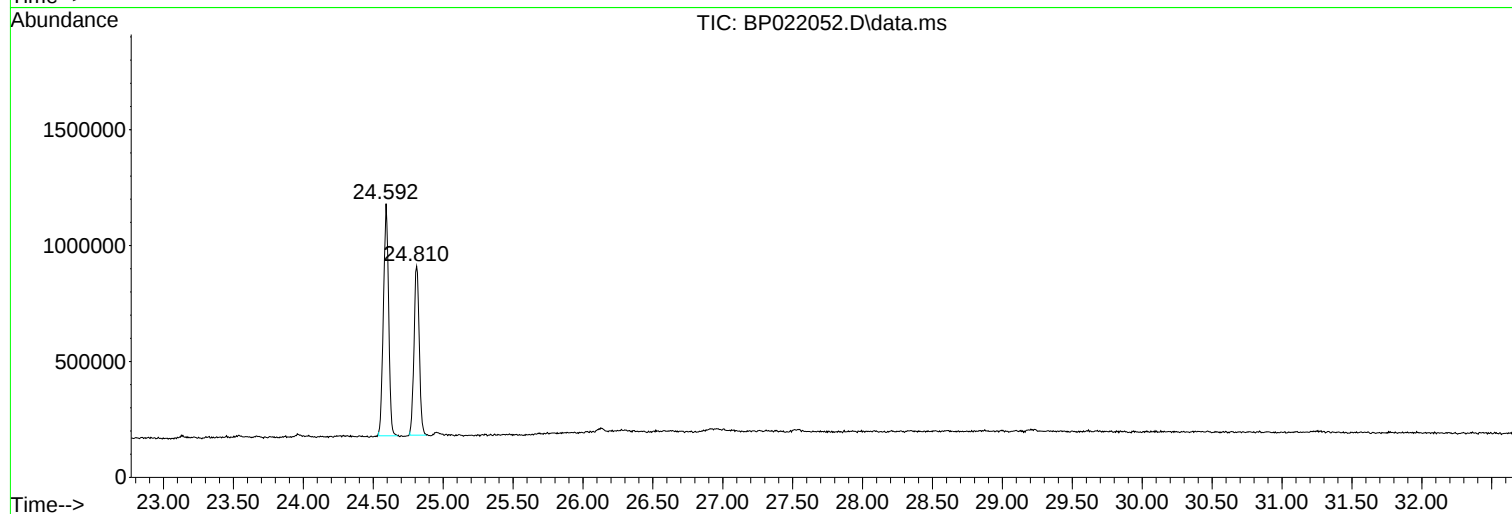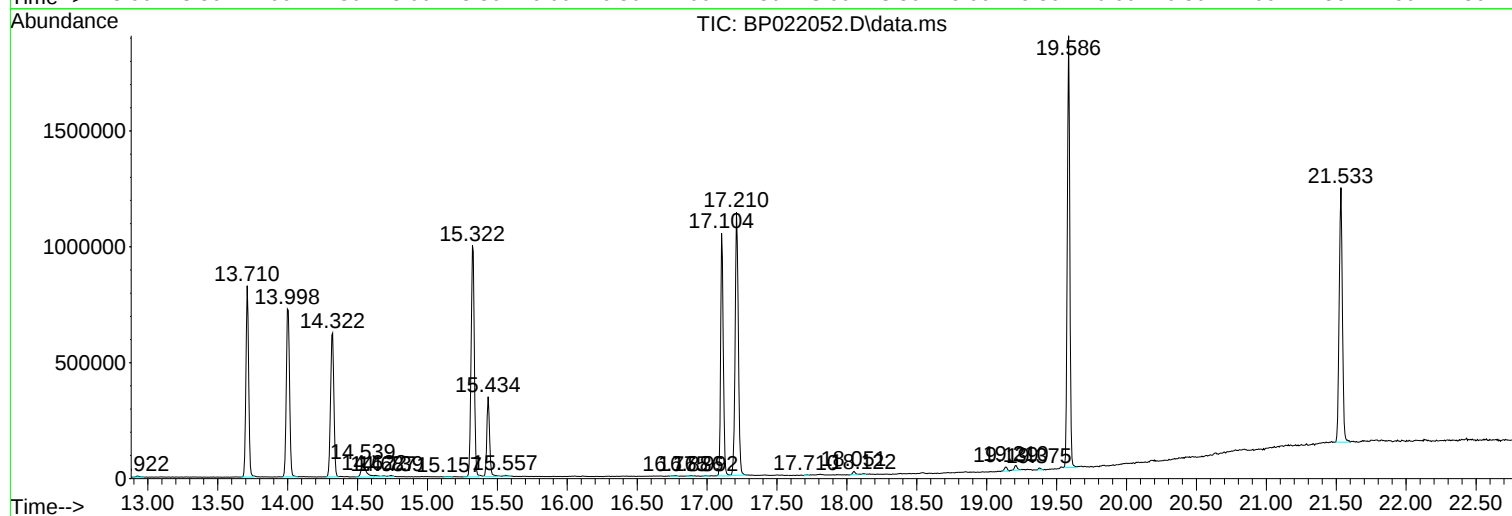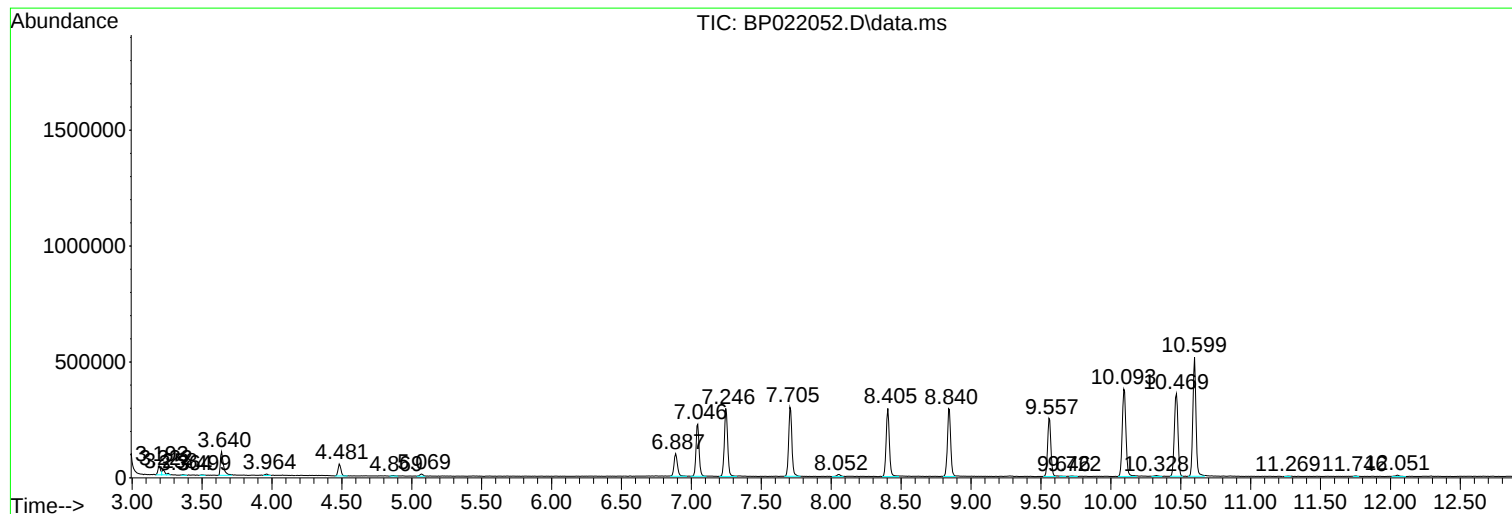

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022052.D
Acq On : 26 Sep 2024 07:43
Operator : RC/JU
Sample : P4107-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022052.D
Acq On : 26 Sep 2024 07:43
Operator : RC/JU
Sample : P4107-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------