

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022056.D
 Acq On : 26 Sep 2024 10:26
 Operator : RC/JU
 Sample : PB163505BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK505

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	46	rVB	35484	46768	1.08%	0.116%
2	3.634	106	110	126	rBV	426091	617503	14.30%	1.534%
3	3.958	161	165	173	rVB3	12857	19519	0.45%	0.048%
4	6.887	655	663	679	rBV	562161	895457	20.74%	2.225%
5	7.040	683	689	700	rVB	405749	659729	15.28%	1.639%
6	7.246	716	724	733	rBV	540904	884379	20.48%	2.197%
7	7.704	795	802	810	rBV	491168	797828	18.48%	1.982%
8	8.404	913	921	930	rBV	656504	1104542	25.58%	2.744%
9	8.516	938	940	945	rVB6	4639	5144	0.12%	0.013%
10	8.840	988	995	1009	rBV	534439	875361	20.27%	2.175%
11	9.410	1086	1092	1098	rVB4	2906	5904	0.14%	0.015%
12	9.551	1109	1116	1128	rBV	469130	767455	17.77%	1.907%
13	9.651	1128	1133	1140	rVB9	4088	8452	0.20%	0.021%
14	10.087	1199	1207	1227	rBV	773082	1232511	28.54%	3.062%
15	10.457	1262	1270	1278	rBV	617401	1071266	24.81%	2.661%
16	10.593	1285	1293	1304	rBV	626726	1121751	25.98%	2.787%
17	10.793	1322	1327	1332	rVB9	4617	8938	0.21%	0.022%
18	12.045	1531	1540	1548	rBV3	11840	22447	0.52%	0.056%
19	12.122	1548	1553	1558	rVB4	4166	7750	0.18%	0.019%
20	12.340	1584	1590	1594	rBV7	4429	8969	0.21%	0.022%
21	12.492	1609	1616	1623	rVB8	4959	10086	0.23%	0.025%
22	13.104	1716	1720	1722	rBV3	4215	5406	0.13%	0.013%
23	13.139	1723	1726	1728	rVV3	4276	5476	0.13%	0.014%
24	13.181	1728	1733	1738	rVV6	4058	7264	0.17%	0.018%
25	13.716	1817	1824	1837	rBV	1411356	1945099	45.04%	4.832%
26	13.887	1848	1853	1858	rVB9	2579	4966	0.11%	0.012%
27	13.998	1864	1872	1885	rBV	1424071	2115957	49.00%	5.257%
28	14.304	1918	1924	1932	rVV	1112155	1602738	37.11%	3.982%
29	14.375	1932	1936	1940	rVB2	5620	8000	0.19%	0.020%
30	14.522	1953	1961	1972	rBV	565841	951642	22.04%	2.364%
31	14.675	1985	1987	1991	rVB5	4114	5080	0.12%	0.013%
32	14.728	1992	1996	2006	rVB3	8851	18711	0.43%	0.046%
33	14.951	2029	2034	2038	rBV8	3867	7805	0.18%	0.019%
34	15.145	2060	2067	2075	rBV2	7027	13217	0.31%	0.033%
35	15.316	2088	2096	2103	rBV	2086886	2823399	65.38%	7.014%
36	15.369	2103	2105	2111	rVV2	13220	17744	0.41%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022056.D
 Acq On : 26 Sep 2024 10:26
 Operator : RC/JU
 Sample : PB163505BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK505

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.439	2111	2117	2127	rVV	547738	810580	18.77%	2.014%
38	15.563	2134	2138	2147	rVB7	10891	27206	0.63%	0.068%
39	16.116	2226	2232	2237	rBV9	5091	9511	0.22%	0.024%
40	16.275	2254	2259	2265	rVB8	5803	9911	0.23%	0.025%
41	16.398	2276	2280	2286	rBV7	6807	10325	0.24%	0.026%
42	16.763	2335	2342	2344	rBV7	5371	8901	0.21%	0.022%
43	17.110	2391	2401	2407	rBV	1470619	2186203	50.63%	5.431%
44	17.210	2412	2418	2438	rVB	2483221	3338579	77.31%	8.294%
45	17.533	2470	2473	2479	rVB3	5006	7242	0.17%	0.018%
46	17.816	2518	2521	2525	rVB5	6121	5837	0.14%	0.015%
47	18.057	2558	2562	2567	rVB7	5686	7943	0.18%	0.020%
48	18.122	2570	2573	2576	rVB2	5584	7292	0.17%	0.018%
49	19.133	2740	2745	2750	rBV4	33138	44886	1.04%	0.112%
50	19.210	2754	2758	2761	rBV	23775	36223	0.84%	0.090%
51	19.586	2816	2822	2833	rBV	3242972	4171392	96.60%	10.363%
52	21.533	3146	3153	3166	rVB	1655234	2771654	64.18%	6.886%
53	24.592	3663	3673	3688	rVB	1742349	4318367	100.00%	10.729%
54	24.815	3702	3711	3726	rVB	1060872	2774675	64.25%	6.893%




Sum of corrected areas: 40250990

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022056.D
Acq On : 26 Sep 2024 10:26
Operator : RC/JU
Sample : PB163505BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

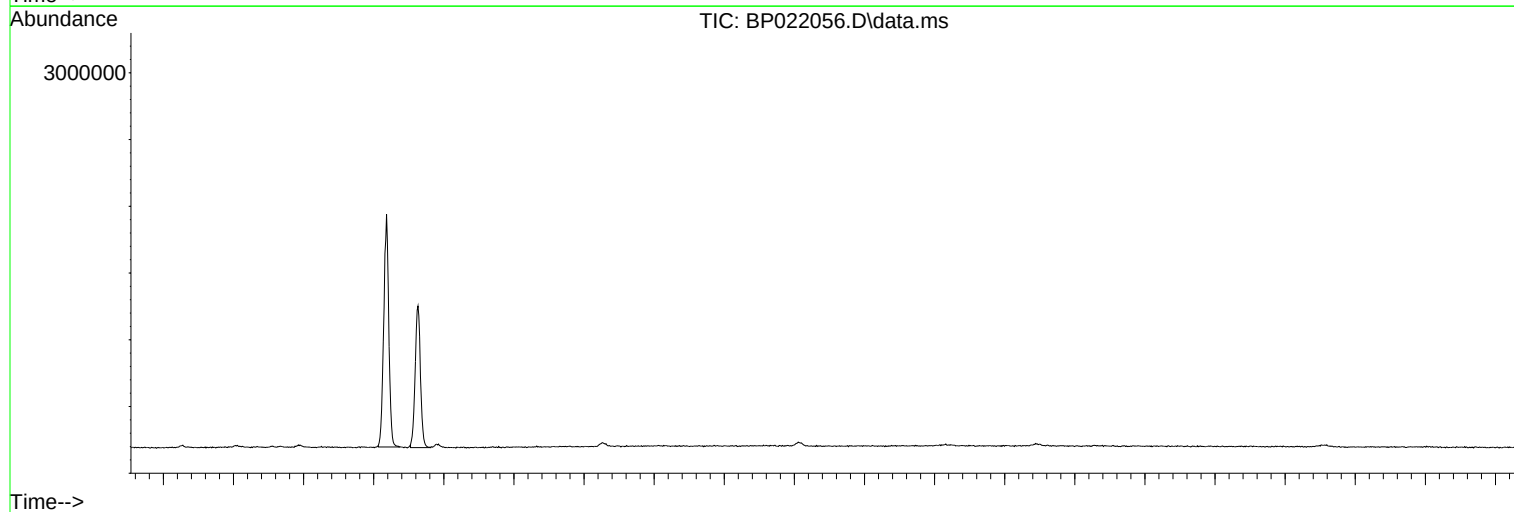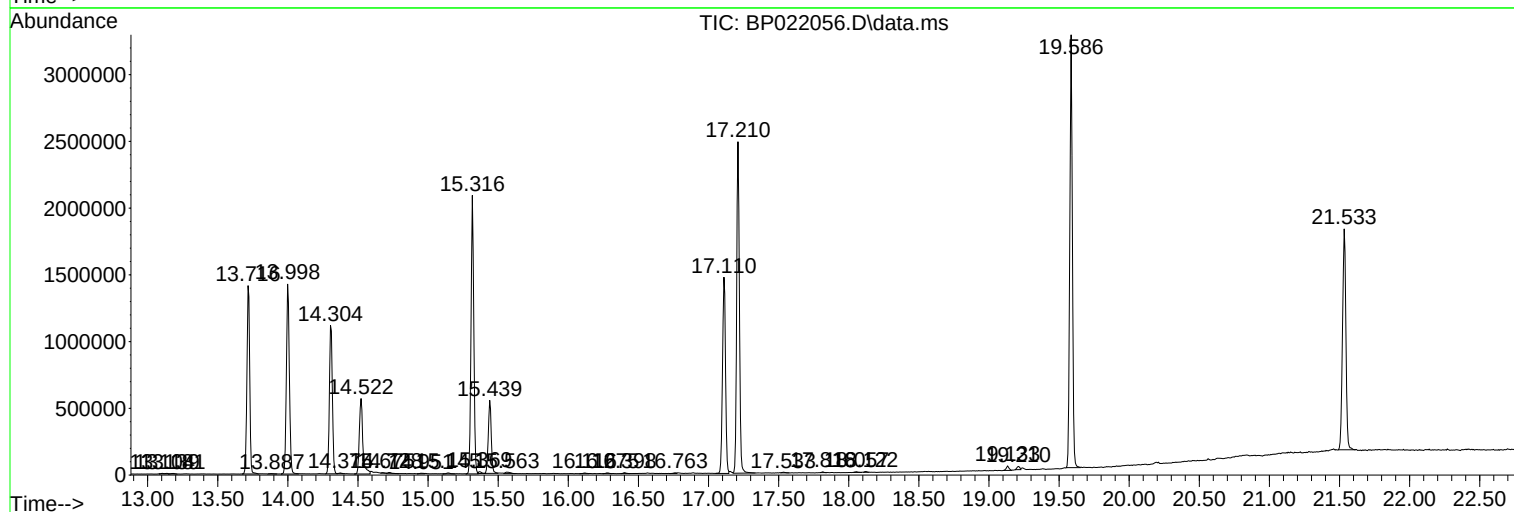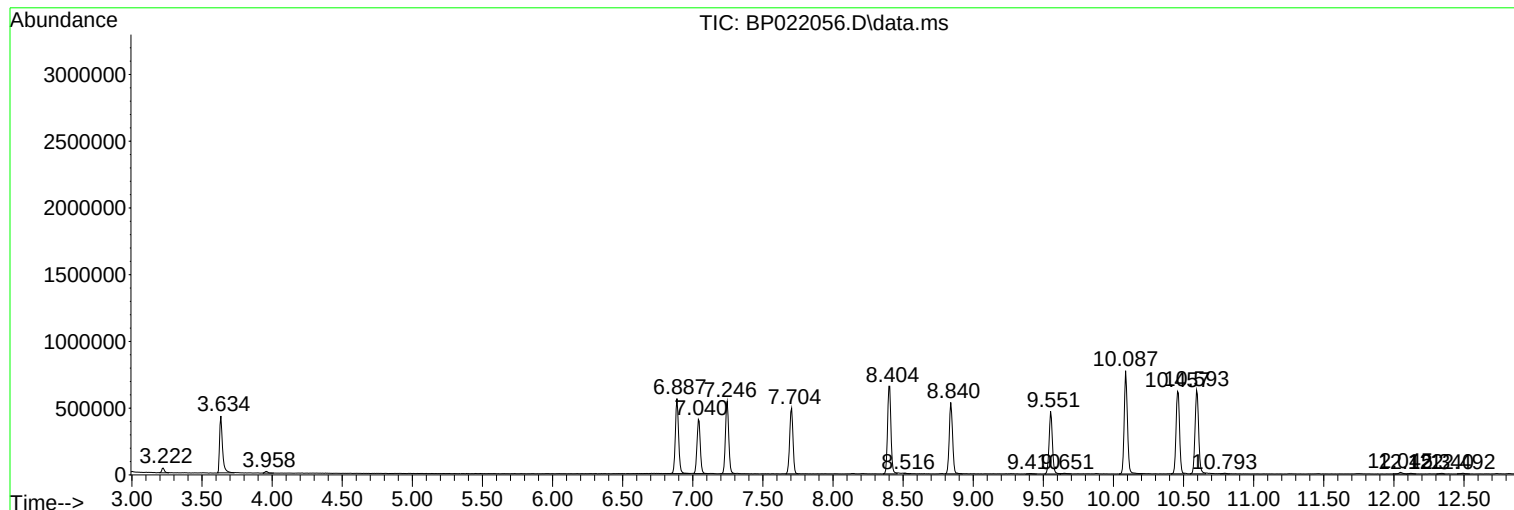

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022056.D
Acq On : 26 Sep 2024 10:26
Operator : RC/JU
Sample : PB163505BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022056.D
Acq On : 26 Sep 2024 10:26
Operator : RC/JU
Sample : PB163505BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------