

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022057.D
 Acq On : 26 Sep 2024 11:06
 Operator : RC/JU
 Sample : PB163541BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	45	rVB	32693	37491	0.95%	0.108%
2	3.634	106	110	126	rBV	370914	555959	14.04%	1.595%
3	3.958	160	165	172	rVB2	12874	19598	0.49%	0.056%
4	6.887	656	663	680	rBV	468148	757997	19.14%	2.175%
5	7.046	683	690	701	rVB	358208	539272	13.62%	1.547%
6	7.246	717	724	736	rBV	476850	770818	19.46%	2.212%
7	7.704	793	802	812	rBV	424680	674905	17.04%	1.937%
8	8.399	908	920	934	rBV	554918	953999	24.09%	2.737%
9	8.846	988	996	1006	rBV	480606	772402	19.50%	2.216%
10	9.557	1110	1117	1128	rBV	425870	684573	17.29%	1.964%
11	10.093	1199	1208	1222	rBV	597470	1095963	27.67%	3.145%
12	10.463	1264	1271	1280	rBV	536245	911898	23.03%	2.617%
13	10.598	1286	1294	1307	rBV	591113	995490	25.14%	2.856%
14	11.269	1403	1408	1414	rBV10	3402	5595	0.14%	0.016%
15	12.045	1535	1540	1547	rBV4	7088	14903	0.38%	0.043%
16	13.098	1711	1719	1723	rBV10	2084	4516	0.11%	0.013%
17	13.716	1816	1824	1839	rBV	1107278	1689664	42.66%	4.848%
18	13.998	1864	1872	1884	rBV	1257072	1824089	46.06%	5.234%
19	14.310	1916	1925	1939	rBV	900800	1371620	34.63%	3.936%
20	14.522	1953	1961	1984	rBV	501651	886162	22.38%	2.543%
21	14.675	1984	1987	1991	rVB5	3637	4291	0.11%	0.012%
22	15.151	2060	2068	2072	rBV7	3086	6351	0.16%	0.018%
23	15.310	2088	2095	2103	rBV	1673110	2419567	61.10%	6.943%
24	15.363	2103	2104	2109	rVB5	5702	5704	0.14%	0.016%
25	15.433	2109	2116	2126	rBV	478269	726922	18.36%	2.086%
26	15.557	2134	2137	2148	rVB8	8283	17835	0.45%	0.051%
27	16.116	2228	2232	2238	rVB9	4352	8008	0.20%	0.023%
28	16.392	2272	2279	2284	rBV10	3149	7636	0.19%	0.022%
29	16.751	2332	2340	2341	rBV7	3861	5641	0.14%	0.016%
30	16.769	2341	2343	2348	rVB6	3210	5115	0.13%	0.015%
31	17.104	2393	2400	2411	rBV	1306687	1807158	45.63%	5.185%
32	17.216	2411	2419	2430	rBV	1848037	2811207	70.98%	8.066%
33	17.504	2462	2468	2469	rBV6	3711	6896	0.17%	0.020%
34	17.816	2518	2521	2526	rVB7	4221	5572	0.14%	0.016%
35	18.051	2557	2561	2567	rBV9	4532	7501	0.19%	0.022%
36	18.251	2590	2595	2598	rBV6	2657	5988	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022057.D
Acq On : 26 Sep 2024 11:06
Operator : RC/JU
Sample : PB163541BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	19.133	2739	2745	2749	rBV2	24492	42304	1.07%	0.121%
38	19.210	2754	2758	2768	rVV2	20011	39897	1.01%	0.114%
39	19.386	2786	2788	2790	rBV2	5839	5337	0.13%	0.015%
40	19.592	2816	2823	2834	rBV	2392714	3540075	89.39%	10.158%
41	21.539	3148	3154	3166	rBV2	1456394	2350554	59.35%	6.745%
42	24.609	3665	3676	3688	rVB	1532429	3960310	100.00%	11.364%
43	24.833	3705	3714	3726	rVB	989400	2493935	62.97%	7.156%

Sum of corrected areas: 34850718




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022057.D
Acq On : 26 Sep 2024 11:06
Operator : RC/JU
Sample : PB163541BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

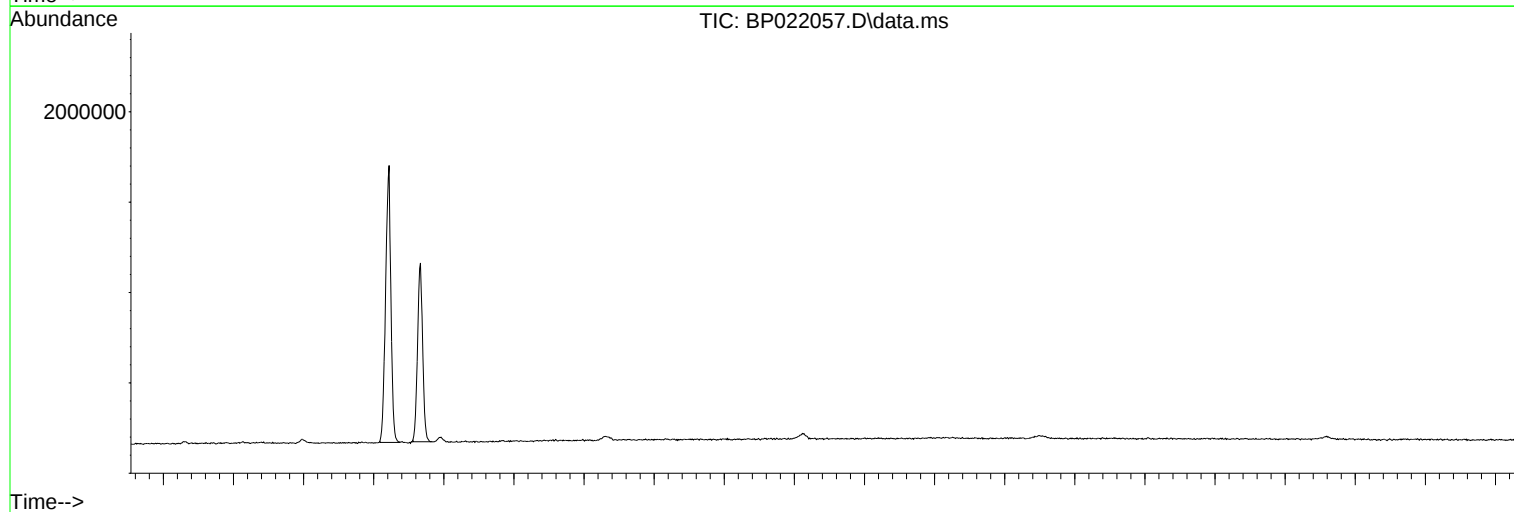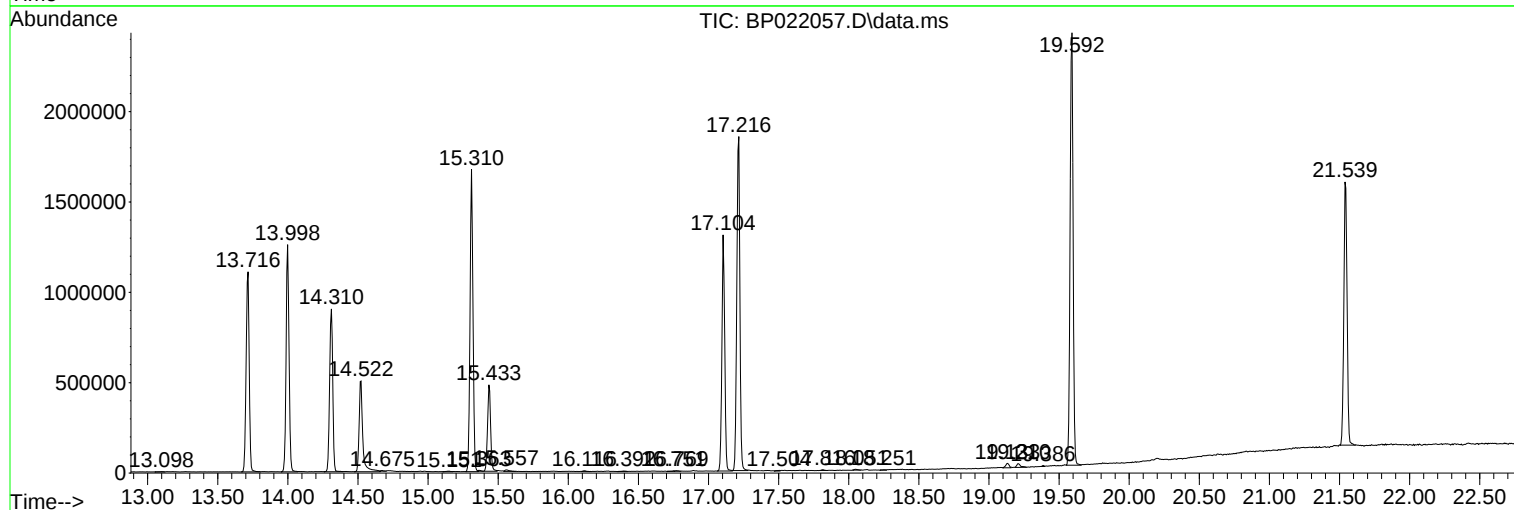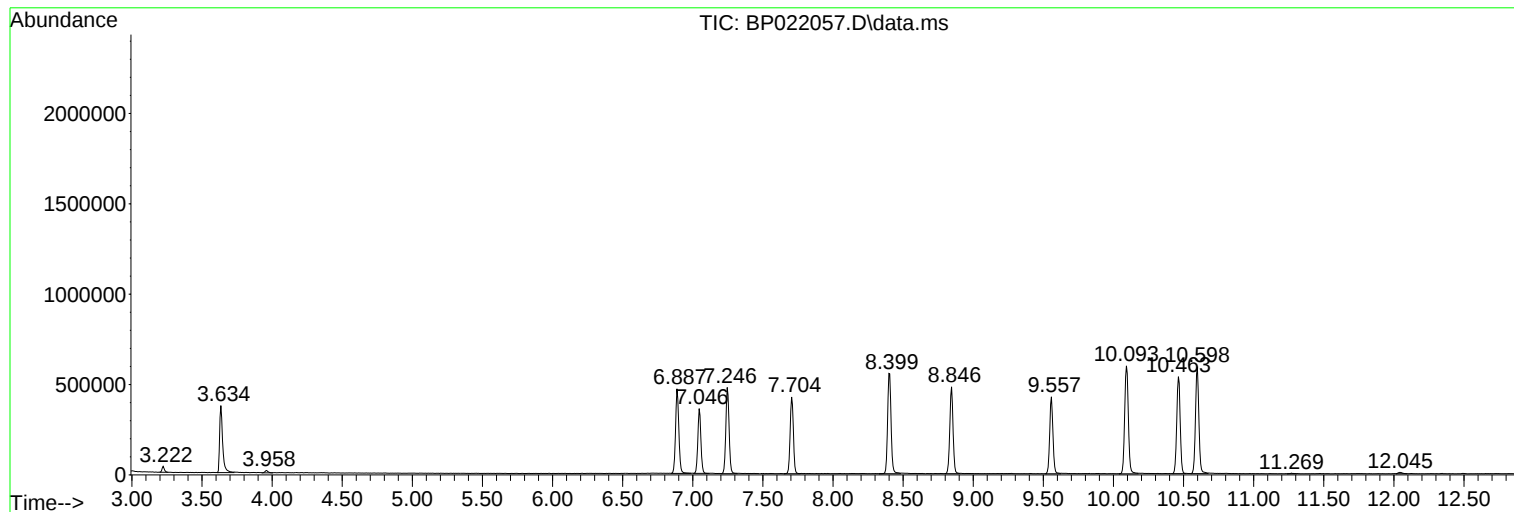

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022057.D
Acq On : 26 Sep 2024 11:06
Operator : RC/JU
Sample : PB163541BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022057.D
Acq On : 26 Sep 2024 11:06
Operator : RC/JU
Sample : PB163541BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc