

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022058.D
 Acq On : 26 Sep 2024 11:47
 Operator : RC/JU
 Sample : P4084-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	46	rVB	24764	33891	0.80%	0.112%
2	3.640	107	111	126	rBV	64563	108359	2.56%	0.358%
3	3.958	161	165	173	rVB3	5946	11007	0.26%	0.036%
4	4.864	314	319	326	rVB4	3644	4612	0.11%	0.015%
5	6.381	573	577	583	rBV5	4914	7880	0.19%	0.026%
6	6.887	653	663	673	rBV	145338	239554	5.67%	0.791%
7	7.046	683	690	699	rBV	342967	508432	12.03%	1.679%
8	7.246	716	724	736	rBV	435769	672710	15.91%	2.221%
9	7.705	794	802	809	rBV	325334	527338	12.48%	1.741%
10	7.769	809	813	819	rVB4	7232	12218	0.29%	0.040%
11	8.405	913	921	933	rBV	336269	607185	14.36%	2.005%
12	8.511	936	939	946	rVB3	3837	6724	0.16%	0.022%
13	8.787	981	986	989	rBV6	5317	8734	0.21%	0.029%
14	8.840	989	995	1005	rVB	423257	708470	16.76%	2.339%
15	8.969	1013	1017	1021	rVB7	3133	4775	0.11%	0.016%
16	9.269	1060	1068	1074	rVB6	4869	8295	0.20%	0.027%
17	9.552	1109	1116	1131	rBV	386430	637366	15.08%	2.104%
18	10.093	1197	1208	1225	rBV	660855	1015239	24.02%	3.352%
19	10.463	1263	1271	1278	rVV	419485	709402	16.78%	2.342%
20	10.522	1278	1281	1286	rVB7	4278	6248	0.15%	0.021%
21	10.599	1286	1294	1311	rBV	256068	485836	11.49%	1.604%
22	11.110	1377	1381	1387	rVB4	5181	9244	0.22%	0.031%
23	11.752	1483	1490	1498	rBV3	11914	22869	0.54%	0.076%
24	12.052	1534	1541	1547	rBV4	6379	13483	0.32%	0.045%
25	12.293	1578	1582	1587	rVV3	3705	5810	0.14%	0.019%
26	12.675	1642	1647	1651	rBV7	3735	6321	0.15%	0.021%
27	12.922	1684	1689	1696	rVB5	7356	11838	0.28%	0.039%
28	13.228	1736	1741	1746	rBV8	4316	8115	0.19%	0.027%
29	13.628	1804	1809	1814	rVB9	4023	5543	0.13%	0.018%
30	13.722	1817	1825	1837	rVV	1190568	1605985	37.99%	5.303%
31	14.004	1865	1873	1884	rBV	1156774	1626080	38.47%	5.369%
32	14.304	1918	1924	1936	rBV	733266	1046445	24.76%	3.455%
33	14.387	1936	1938	1947	rVB10	2895	6028	0.14%	0.020%
34	14.516	1954	1960	1980	rBV	115655	244204	5.78%	0.806%
35	14.734	1993	1997	2003	rVB7	5977	10239	0.24%	0.034%
36	14.993	2036	2041	2046	rVB7	2914	5884	0.14%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022058.D
 Acq On : 26 Sep 2024 11:47
 Operator : RC/JU
 Sample : P4084-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	15.140	2060	2066	2071	rBV3	5241	9529	0.23%	0.031%
38	15.316	2089	2096	2104	rBV	1721354	2291415	54.21%	7.566%
39	15.428	2110	2115	2127	rBV	506743	721523	17.07%	2.382%
40	15.557	2133	2137	2144	rVB4	9412	14693	0.35%	0.049%
41	15.687	2155	2159	2163	rVB3	5912	7554	0.18%	0.025%
42	17.098	2392	2399	2408	rBV	897260	1393690	32.97%	4.602%
43	17.198	2408	2416	2434	rBV	1825189	2745300	64.94%	9.064%
44	17.798	2512	2518	2525	rVB2	52447	81715	1.93%	0.270%
45	18.034	2554	2558	2567	rBV7	13754	22936	0.54%	0.076%
46	19.122	2740	2743	2749	rVB2	25360	35398	0.84%	0.117%
47	19.198	2752	2756	2762	rVV2	24844	38078	0.90%	0.126%
48	19.369	2782	2785	2789	rBV5	9726	12113	0.29%	0.040%
49	19.528	2808	2812	2814	rBV5	11154	15442	0.37%	0.051%
50	19.575	2814	2820	2830	rVV	2688878	3668482	86.78%	12.113%
51	21.528	3146	3152	3163	rVB	1229486	1936145	45.80%	6.393%
52	24.586	3661	3672	3685	rVB	1724226	4227158	100.00%	13.957%
53	24.804	3701	3709	3722	rVB	771886	2113177	49.99%	6.977%




Sum of corrected areas: 30286711

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022058.D
Acq On : 26 Sep 2024 11:47
Operator : RC/JU
Sample : P4084-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

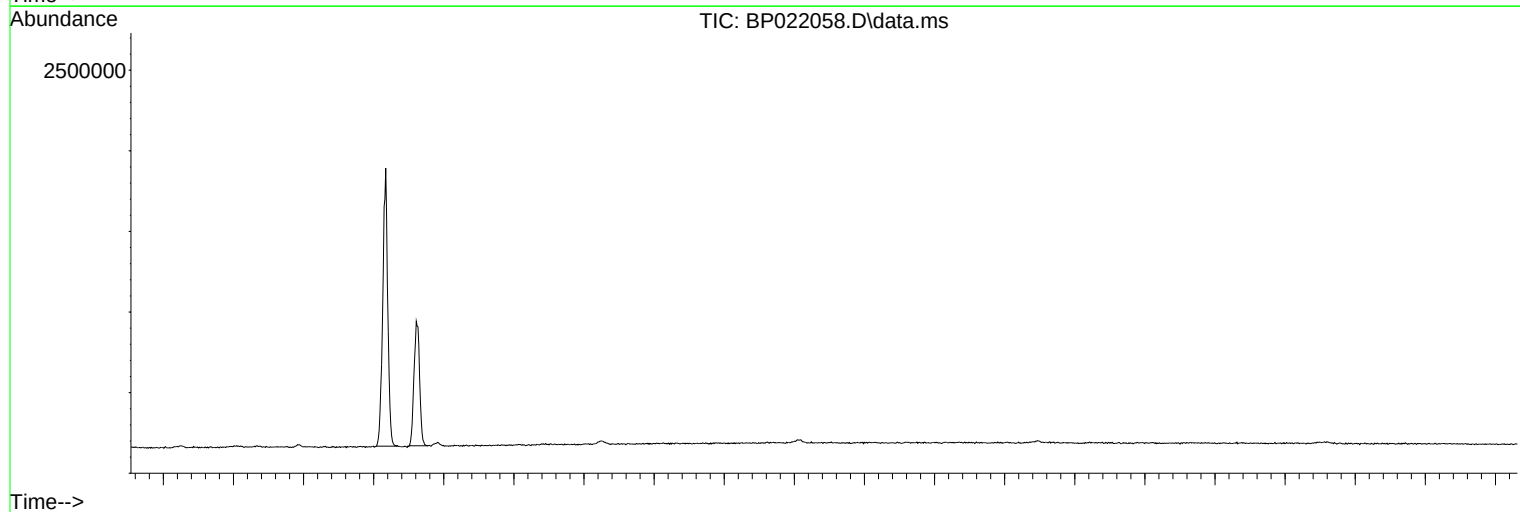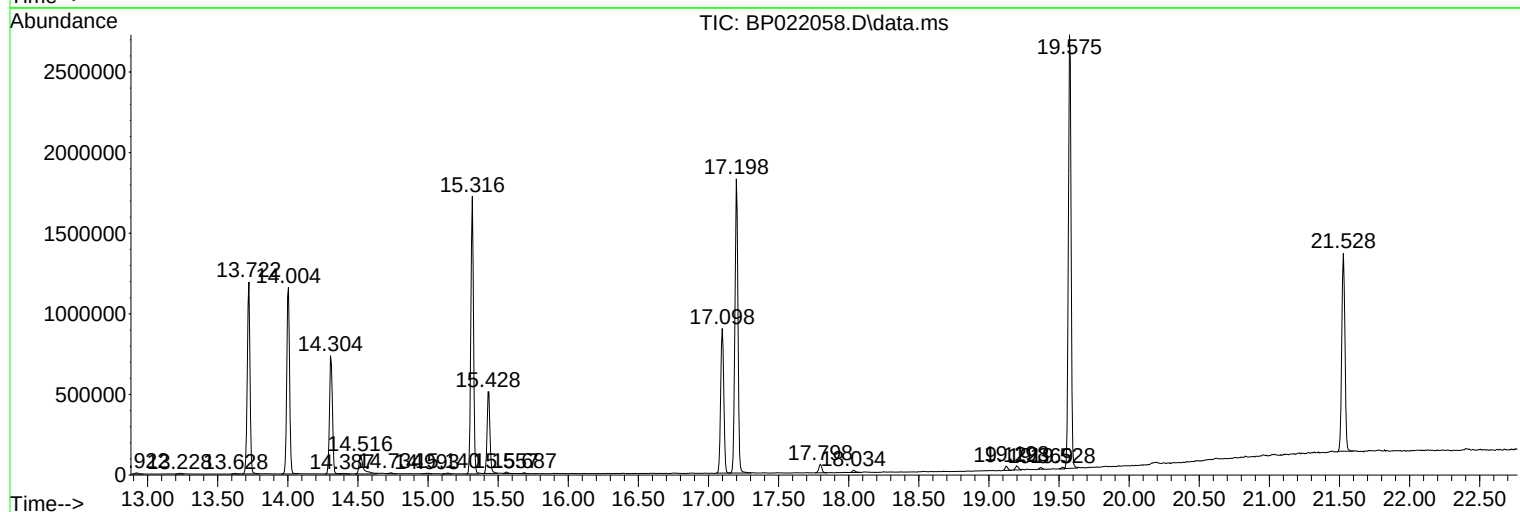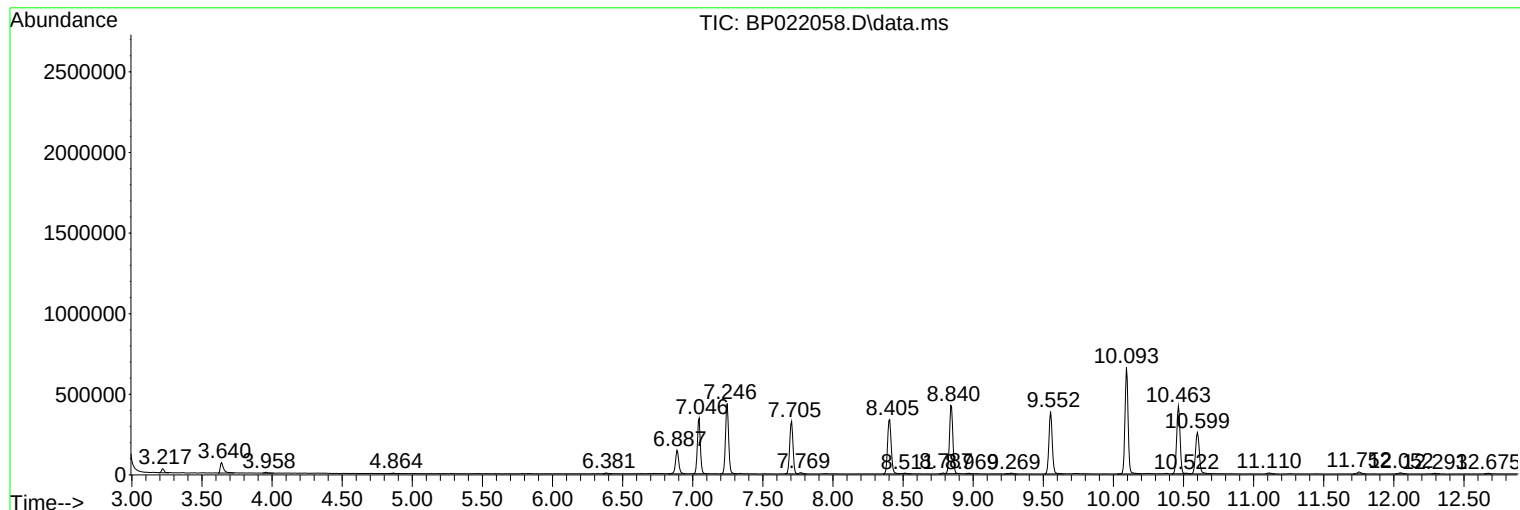

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022058.D
Acq On : 26 Sep 2024 11:47
Operator : RC/JU
Sample : P4084-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022058.D
Acq On : 26 Sep 2024 11:47
Operator : RC/JU
Sample : P4084-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------