

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022062.D
 Acq On : 26 Sep 2024 14:30
 Operator : RC/JU
 Sample : P4080-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	35	40	49	rVB	28441	38387	0.74%	0.097%
2	3.634	106	110	124	rBV	109338	174848	3.37%	0.441%
3	3.958	161	165	171	rVB	13454	19518	0.38%	0.049%
4	6.887	654	663	677	rVB	172538	286315	5.52%	0.722%
5	7.040	682	689	702	rVB	411064	651673	12.55%	1.643%
6	7.246	717	724	733	rBV	492765	820015	15.80%	2.067%
7	7.705	791	802	809	rBV	465349	707493	13.63%	1.783%
8	7.769	809	813	820	rVB2	16086	26474	0.51%	0.067%
9	8.405	913	921	931	rBV	453792	764859	14.74%	1.928%
10	8.511	935	939	945	rVB	10968	17584	0.34%	0.044%
11	8.840	988	995	1011	rBV	542934	909230	17.52%	2.292%
12	9.558	1109	1117	1124	rBV	482597	796703	15.35%	2.008%
13	9.669	1131	1136	1143	rVB9	2790	5767	0.11%	0.015%
14	10.093	1200	1208	1219	rBV	765206	1250251	24.09%	3.152%
15	10.463	1263	1271	1280	rBV	563813	946099	18.23%	2.385%
16	10.599	1286	1294	1309	rBV	531626	954034	18.38%	2.405%
17	10.999	1354	1362	1368	rBV	9115	17684	0.34%	0.045%
18	11.063	1368	1373	1376	rVV2	9889	16636	0.32%	0.042%
19	11.104	1376	1380	1391	rVB	15135	28610	0.55%	0.072%
20	11.204	1391	1397	1402	rBV3	7631	15871	0.31%	0.040%
21	11.563	1450	1458	1469	rBV4	13696	32382	0.62%	0.082%
22	11.957	1520	1525	1530	rBV4	5211	8818	0.17%	0.022%
23	12.040	1533	1539	1545	rBV3	12066	21334	0.41%	0.054%
24	13.304	1751	1754	1759	rVB7	3242	5714	0.11%	0.014%
25	13.716	1817	1824	1832	rBV	1553519	2012178	38.77%	5.072%
26	14.004	1864	1873	1881	rBV	1615618	2202582	42.43%	5.552%
27	14.316	1917	1926	1933	rBV	986491	1461594	28.16%	3.684%
28	14.445	1943	1948	1954	rVB9	2985	6595	0.13%	0.017%
29	14.528	1954	1962	1980	rBV	121821	293507	5.65%	0.740%
30	14.734	1993	1997	2003	rVB8	6631	13260	0.26%	0.033%
31	15.328	2090	2098	2106	rBV	1877935	2981009	57.43%	7.515%
32	15.440	2111	2117	2127	rBV	724941	905624	17.45%	2.283%
33	15.557	2135	2137	2146	rVB2	10029	18405	0.35%	0.046%
34	16.028	2209	2217	2223	rBV4	11757	25497	0.49%	0.064%
35	16.175	2237	2242	2249	rBV2	11918	21116	0.41%	0.053%
36	16.251	2249	2255	2261	rVV4	13590	28433	0.55%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022062.D
 Acq On : 26 Sep 2024 14:30
 Operator : RC/JU
 Sample : P4080-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	16.316	2261	2266	2270	rBV3	13698	22293	0.43%	0.056%
38	16.357	2270	2273	2277	rVB4	6981	9303	0.18%	0.023%
39	16.398	2277	2280	2282	rBV4	5080	5544	0.11%	0.014%
40	16.498	2292	2297	2303	rVB4	7444	16915	0.33%	0.043%
41	16.581	2306	2311	2314	rBV	10946	18659	0.36%	0.047%
42	16.669	2322	2326	2331	rVB4	6757	11208	0.22%	0.028%
43	17.116	2395	2402	2411	rBV	1494193	1959636	37.75%	4.940%
44	17.216	2411	2419	2432	rVB2	2347815	3718134	71.63%	9.373%
45	17.945	2540	2543	2548	rVB3	8079	10794	0.21%	0.027%
46	18.057	2557	2562	2569	rBV3	35471	51963	1.00%	0.131%
47	18.128	2570	2574	2578	rVB6	3358	6621	0.13%	0.017%
48	19.139	2742	2746	2751	rBV	29953	44376	0.85%	0.112%
49	19.210	2754	2758	2764	rBV	35759	58160	1.12%	0.147%
50	19.386	2784	2788	2794	rVB5	24766	32038	0.62%	0.081%
51	19.592	2817	2823	2831	rBV	3753199	4816083	92.79%	12.140%
52	21.545	3148	3155	3166	rVB	1612232	2532347	48.79%	6.384%
53	24.598	3664	3674	3686	rVB	1953339	5190558	100.00%	13.084%
54	24.816	3704	3711	3725	rVB	1008761	2679305	51.62%	6.754%




Sum of corrected areas: 39670036

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022062.D
Acq On : 26 Sep 2024 14:30
Operator : RC/JU
Sample : P4080-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

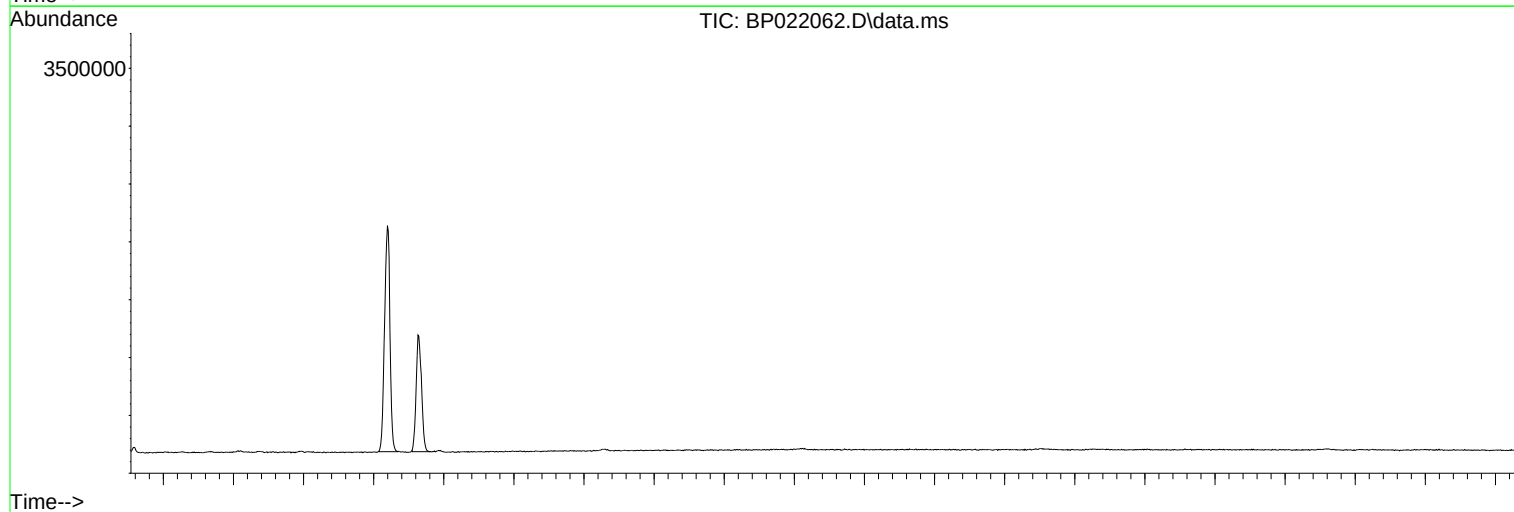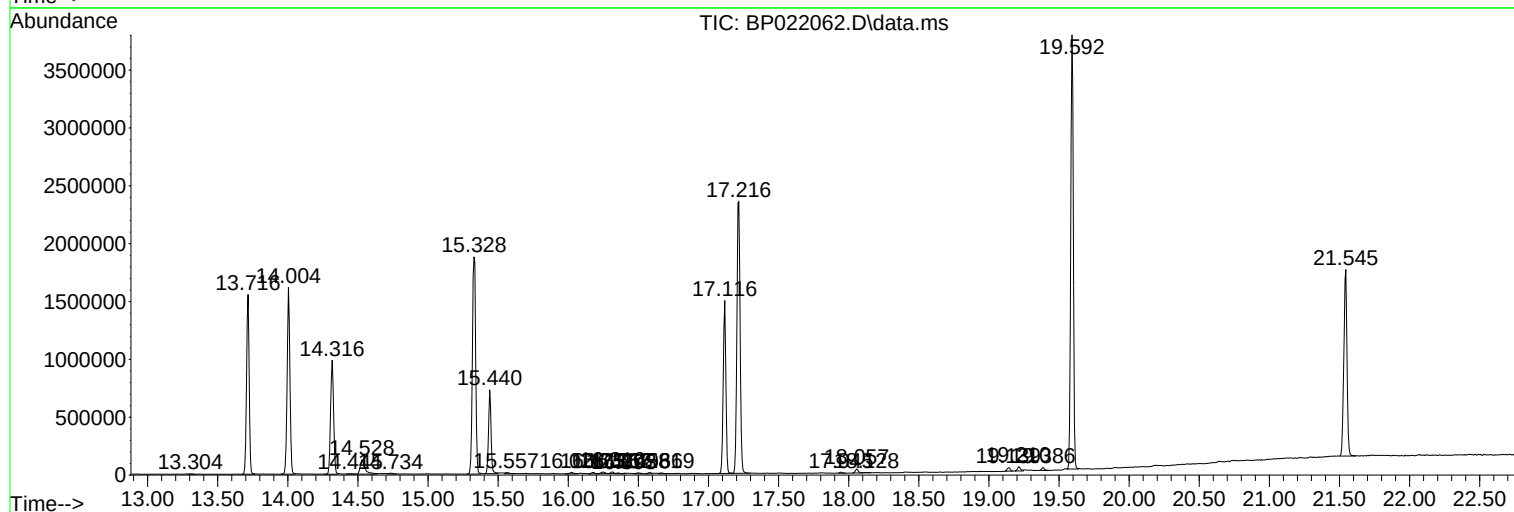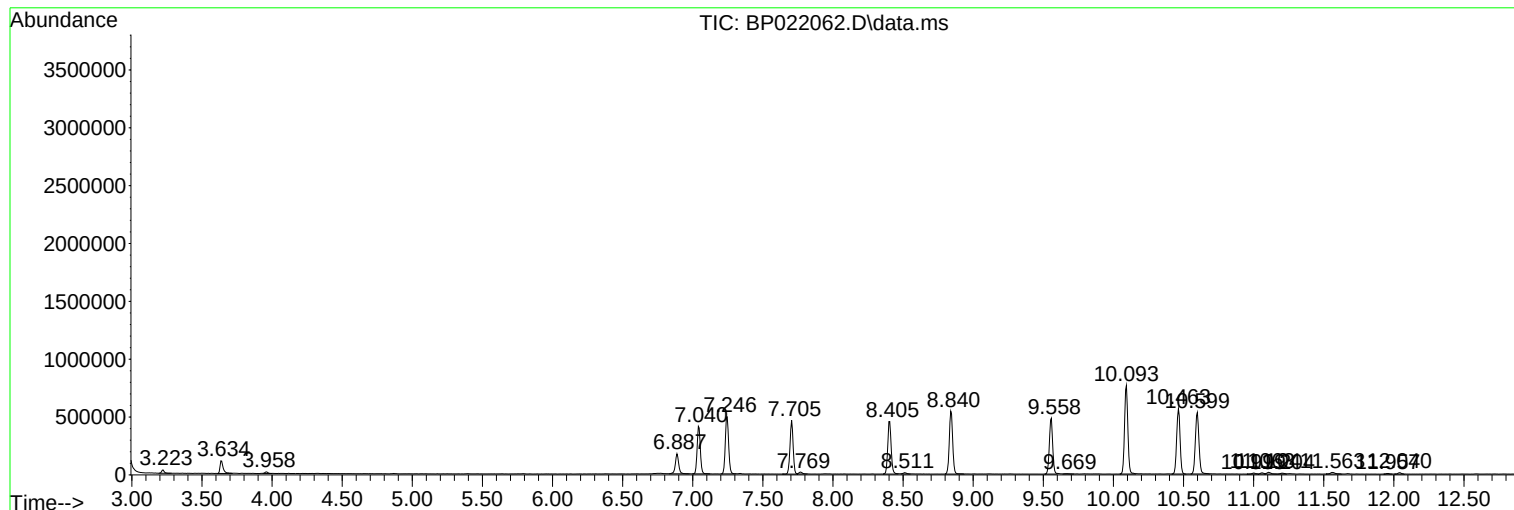

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022062.D
Acq On : 26 Sep 2024 14:30
Operator : RC/JU
Sample : P4080-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022062.D
Acq On : 26 Sep 2024 14:30
Operator : RC/JU
Sample : P4080-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
