

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022063.D
Acq On : 26 Sep 2024 15:10
Operator : RC/JU
Sample : P4080-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BP022063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	36	39	47	rVB	23248	30804	0.76%	0.102%
2	3.634	107	110	122	rBV	99188	148320	3.68%	0.492%
3	3.957	160	165	172	rVB	21184	31063	0.77%	0.103%
4	4.863	316	319	326	rVB8	2171	4479	0.11%	0.015%
5	6.746	630	639	649	rBV9	7116	25205	0.63%	0.084%
6	6.893	653	664	676	rVB	128734	225254	5.59%	0.747%
7	7.046	683	690	698	rBV	351615	538272	13.36%	1.785%
8	7.246	716	724	734	rBV	447506	690354	17.14%	2.289%
9	7.340	736	740	746	rVB9	3313	6899	0.17%	0.023%
10	7.704	795	802	809	rBV	347065	564495	14.02%	1.872%
11	7.769	809	813	824	rVB4	12241	21665	0.54%	0.072%
12	8.404	913	921	933	rBV	346983	603161	14.98%	2.000%
13	8.516	935	940	944	rVB3	8296	13897	0.35%	0.046%
14	8.840	988	995	1008	rBV	428087	734310	18.23%	2.435%
15	9.557	1110	1117	1131	rBV	387313	653826	16.23%	2.168%
16	10.098	1201	1209	1223	rBV	586383	1025446	25.46%	3.400%
17	10.463	1263	1271	1279	rBV	424320	735271	18.26%	2.438%
18	10.598	1286	1294	1305	rBV	409176	741438	18.41%	2.459%
19	10.675	1305	1307	1315	rVB8	3036	5510	0.14%	0.018%
20	11.010	1357	1364	1368	rBV3	6588	13291	0.33%	0.044%
21	11.063	1368	1373	1376	rVV2	6847	11836	0.29%	0.039%
22	11.110	1376	1381	1389	rVB2	11405	22202	0.55%	0.074%
23	11.204	1393	1397	1403	rBV3	5624	10656	0.26%	0.035%
24	11.557	1446	1457	1468	rBV9	9261	29110	0.72%	0.097%
25	11.675	1473	1477	1481	rVV4	3491	4663	0.12%	0.015%
26	11.957	1521	1525	1528	rBV4	3106	5401	0.13%	0.018%
27	12.051	1535	1541	1545	rBV2	8805	13818	0.34%	0.046%
28	13.716	1817	1824	1834	rBV	1085491	1537655	38.18%	5.099%
29	14.004	1865	1873	1882	rBV	1073670	1658077	41.17%	5.498%
30	14.316	1915	1926	1938	rBV	769763	1074810	26.69%	3.564%
31	14.533	1955	1963	1976	rBV2	81166	191575	4.76%	0.635%
32	14.733	1994	1997	2007	rVB2	4782	10823	0.27%	0.036%
33	15.327	2089	2098	2107	rBV	1504328	2278040	56.56%	7.554%
34	15.439	2111	2117	2131	rBV	419051	595968	14.80%	1.976%
35	15.563	2136	2138	2149	rVB10	7519	17252	0.43%	0.057%
36	16.027	2210	2217	2224	rBV8	7743	17372	0.43%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022063.D
 Acq On : 26 Sep 2024 15:10
 Operator : RC/JU
 Sample : P4080-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	16.180	2238	2243	2249	rBV	8988	16742	0.42%	0.056%
38	16.251	2249	2255	2262	rVV4	10602	23841	0.59%	0.079%
39	16.316	2262	2266	2270	rVV2	12364	19230	0.48%	0.064%
40	16.357	2270	2273	2277	rVB5	5294	6841	0.17%	0.023%
41	16.504	2294	2298	2306	rVB6	5106	12340	0.31%	0.041%
42	16.580	2306	2311	2316	rBV	7496	16053	0.40%	0.053%
43	16.663	2322	2325	2330	rVB4	5125	7159	0.18%	0.024%
44	16.763	2337	2342	2344	rBV5	4201	7704	0.19%	0.026%
45	17.116	2396	2402	2408	rBV	1053160	1413403	35.09%	4.687%
46	17.210	2411	2418	2432	rVB	1852778	2732625	67.85%	9.061%
47	17.416	2450	2453	2458	rVB7	3028	4509	0.11%	0.015%
48	17.810	2518	2520	2523	rVB4	3327	4166	0.10%	0.014%
49	17.945	2537	2543	2547	rVB5	6839	10516	0.26%	0.035%
50	18.057	2556	2562	2571	rBV9	19678	34963	0.87%	0.116%
51	19.139	2742	2746	2751	rBV	24304	37792	0.94%	0.125%
52	19.221	2755	2760	2764	rBV	25956	37649	0.93%	0.125%
53	19.386	2785	2788	2794	rVB5	17372	20432	0.51%	0.068%
54	19.539	2812	2814	2817	rBV4	7801	8518	0.21%	0.028%
55	19.598	2817	2824	2832	rBV	2871486	3556669	88.31%	11.794%
56	21.539	3148	3154	3163	rBV	1069555	1839047	45.66%	6.098%
57	24.603	3665	3675	3690	rVB	1483803	4027630	100.00%	13.355%
58	24.821	3704	3712	3724	rVB	680500	2027277	50.33%	6.722%

Sum of corrected areas: 30157324




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022063.D
Acq On : 26 Sep 2024 15:10
Operator : RC/JU
Sample : P4080-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

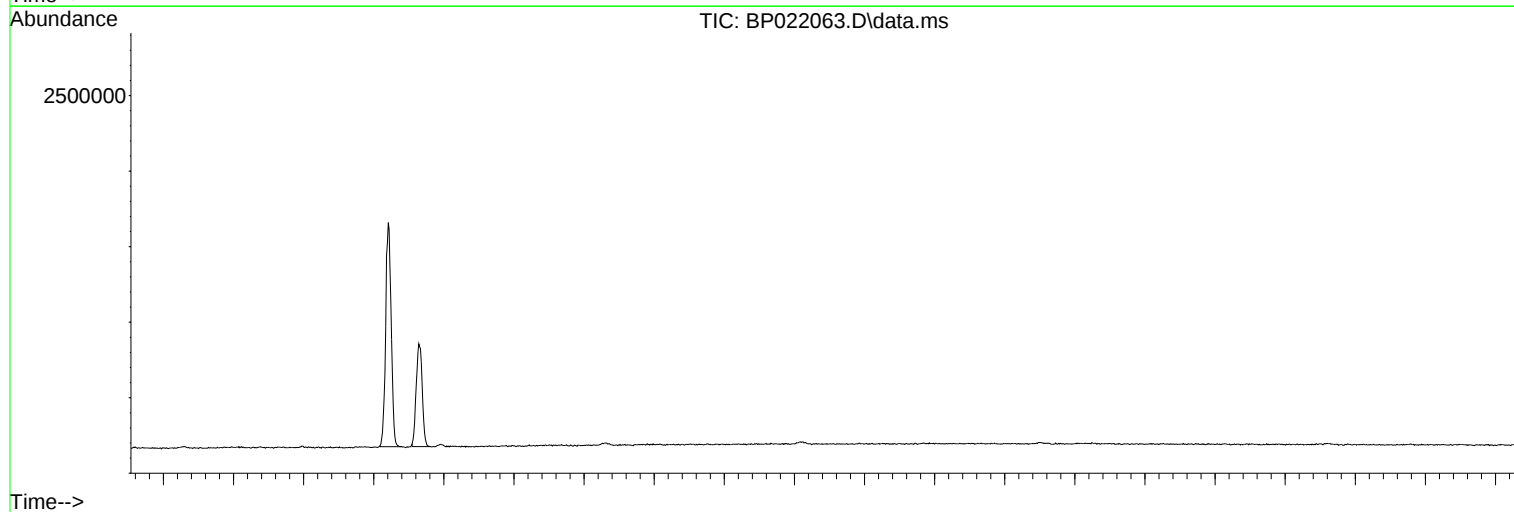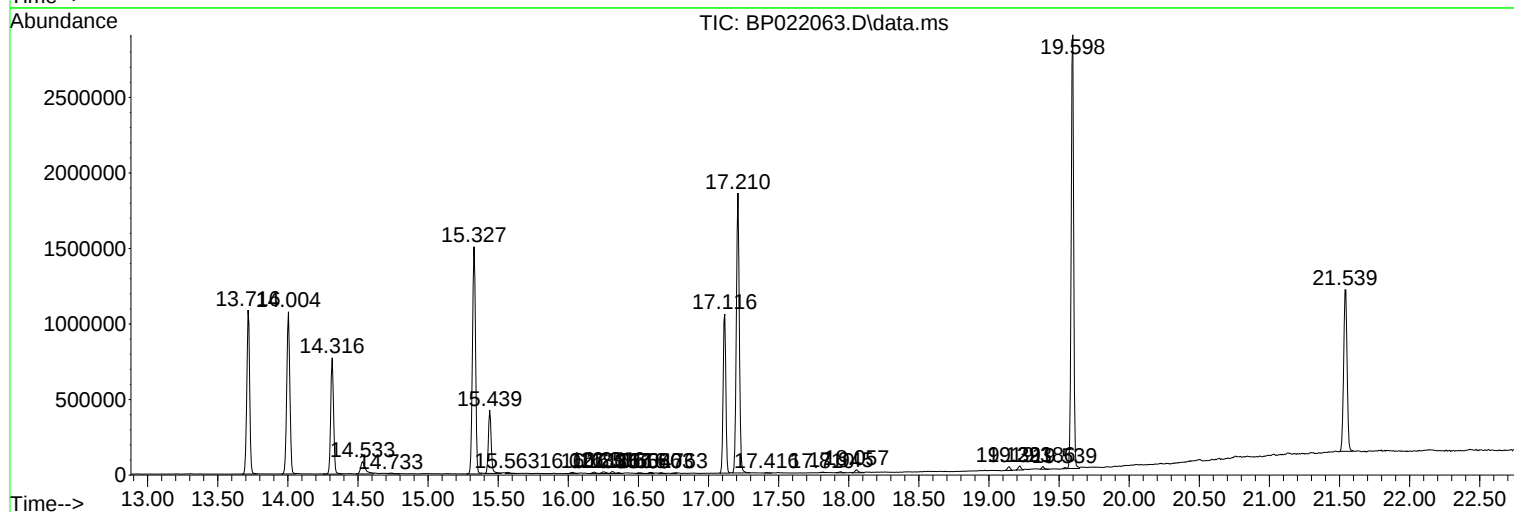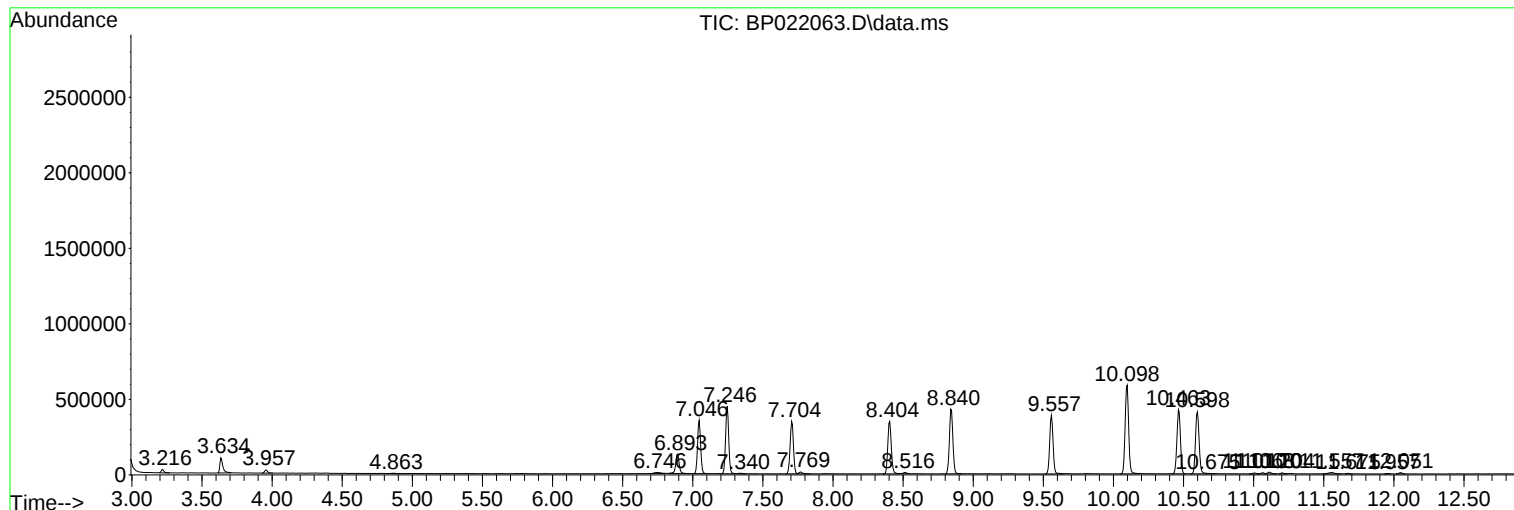

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022063.D
Acq On : 26 Sep 2024 15:10
Operator : RC/JU
Sample : P4080-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022063.D
Acq On : 26 Sep 2024 15:10
Operator : RC/JU
Sample : P4080-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
