

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022065.D
 Acq On : 26 Sep 2024 16:32
 Operator : RC/JU
 Sample : PB163588BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	35	38	49	rVB	35135	48881	1.05%	0.126%
2	3.628	104	109	126	rBV	423706	628095	13.55%	1.618%
3	3.952	160	164	169	rVB3	9501	14732	0.32%	0.038%
4	6.887	654	663	677	rBV	559860	871913	18.80%	2.246%
5	7.046	684	690	697	rVV	410291	625603	13.49%	1.612%
6	7.128	700	704	711	rVB7	3342	6396	0.14%	0.016%
7	7.246	717	724	735	rBV	576101	873343	18.83%	2.250%
8	7.705	793	802	809	rBV	413150	667764	14.40%	1.720%
9	8.146	873	877	883	rVB7	3728	6086	0.13%	0.016%
10	8.216	886	889	894	rVB7	3057	5963	0.13%	0.015%
11	8.399	913	920	930	rBV	647739	1078483	23.26%	2.778%
12	8.505	935	938	945	rVB4	6033	12366	0.27%	0.032%
13	8.763	978	982	988	rVB9	4106	5819	0.13%	0.015%
14	8.840	988	995	1008	rBV	532345	873467	18.84%	2.250%
15	9.405	1084	1091	1100	rVB5	4813	9946	0.21%	0.026%
16	9.557	1108	1117	1129	rBV	449542	767011	16.54%	1.976%
17	9.652	1129	1133	1137	rVB5	4907	8512	0.18%	0.022%
18	9.875	1166	1171	1175	rBV3	3560	5539	0.12%	0.014%
19	10.093	1201	1208	1224	rBV	710891	1222745	26.37%	3.150%
20	10.463	1264	1271	1278	rBV	566315	887912	19.15%	2.287%
21	10.599	1285	1294	1305	rBV	624724	1130858	24.39%	2.913%
22	10.804	1324	1329	1334	rBV7	6404	10599	0.23%	0.027%
23	11.457	1436	1440	1449	rVB7	2424	6191	0.13%	0.016%
24	11.757	1486	1491	1495	rBV6	4426	7308	0.16%	0.019%
25	12.051	1535	1541	1547	rBV3	11846	20305	0.44%	0.052%
26	12.122	1548	1553	1559	rVB5	6552	10830	0.23%	0.028%
27	12.346	1587	1591	1596	rVB3	7497	11659	0.25%	0.030%
28	12.493	1609	1616	1625	rVB8	7441	17629	0.38%	0.045%
29	12.740	1653	1658	1664	rBV7	4520	7922	0.17%	0.020%
30	12.822	1666	1672	1677	rVB9	3781	7326	0.16%	0.019%
31	13.104	1715	1720	1723	rBV2	8492	13205	0.28%	0.034%
32	13.140	1723	1726	1730	rVV2	8582	13657	0.29%	0.035%
33	13.187	1730	1734	1738	rVB3	6671	10859	0.23%	0.028%
34	13.728	1818	1826	1832	rBV	1360895	1918531	41.37%	4.943%
35	13.769	1832	1833	1842	rVB	13684	15657	0.34%	0.040%
36	13.881	1849	1852	1859	rVB8	4168	7278	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022065.D
 Acq On : 26 Sep 2024 16:32
 Operator : RC/JU
 Sample : PB163588BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	14.010	1865	1874	1888	rBV2	1170088	2101425	45.32%	5.414%
38	14.322	1919	1927	1934	rBV	868777	1328931	28.66%	3.424%
39	14.381	1934	1937	1942	rVB2	10602	14850	0.32%	0.038%
40	14.528	1954	1962	1976	rBV	580008	978312	21.10%	2.520%
41	14.640	1978	1981	1986	rVV3	16958	32430	0.70%	0.084%
42	14.692	1986	1990	1993	rVV6	10391	20742	0.45%	0.053%
43	14.728	1993	1996	2005	rVB	11517	25767	0.56%	0.066%
44	14.963	2031	2036	2039	rBV5	4469	7942	0.17%	0.020%
45	15.157	2062	2069	2074	rVB	13611	18461	0.40%	0.048%
46	15.334	2090	2099	2105	rBV	1620919	2767381	59.68%	7.129%
47	15.387	2105	2108	2114	rVV2	24469	41355	0.89%	0.107%
48	15.457	2114	2120	2130	rVV	506178	713334	15.38%	1.838%
49	15.587	2134	2142	2148	rVB4	14545	34183	0.74%	0.088%
50	16.134	2232	2235	2239	rBV5	5428	7770	0.17%	0.020%
51	16.292	2257	2262	2267	rBV6	9366	15292	0.33%	0.039%
52	16.416	2276	2283	2290	rBV6	10498	22236	0.48%	0.057%
53	16.569	2305	2309	2313	rBV6	7091	10860	0.23%	0.028%
54	16.781	2340	2345	2347	rBV6	5218	9372	0.20%	0.024%
55	17.128	2396	2404	2410	rBV	1148895	1818962	39.23%	4.686%
56	17.222	2414	2420	2439	rVB	2330922	3289928	70.95%	8.475%
57	17.551	2472	2476	2480	rVB2	10016	14501	0.31%	0.037%
58	17.828	2520	2523	2527	rVB6	4877	5162	0.11%	0.013%
59	18.063	2560	2563	2568	rBV7	4619	7801	0.17%	0.020%
60	18.139	2571	2576	2581	rVB	12243	16863	0.36%	0.043%
61	19.145	2742	2747	2752	rBV3	28076	43268	0.93%	0.111%
62	19.222	2756	2760	2763	rBV	28735	41448	0.89%	0.107%
63	19.257	2763	2766	2770	rVB2	16801	24520	0.53%	0.063%
64	19.604	2818	2825	2835	rBV	2748247	4218429	90.97%	10.867%
65	21.551	3150	3156	3169	rVB	1516340	2365482	51.01%	6.094%
66	24.610	3666	3676	3693	rVB2	1825790	4637009	100.00%	11.946%
67	24.845	3706	3716	3731	rVB	914951	2352553	50.73%	6.061%




Sum of corrected areas: 38816959

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022065.D
Acq On : 26 Sep 2024 16:32
Operator : RC/JU
Sample : PB163588BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

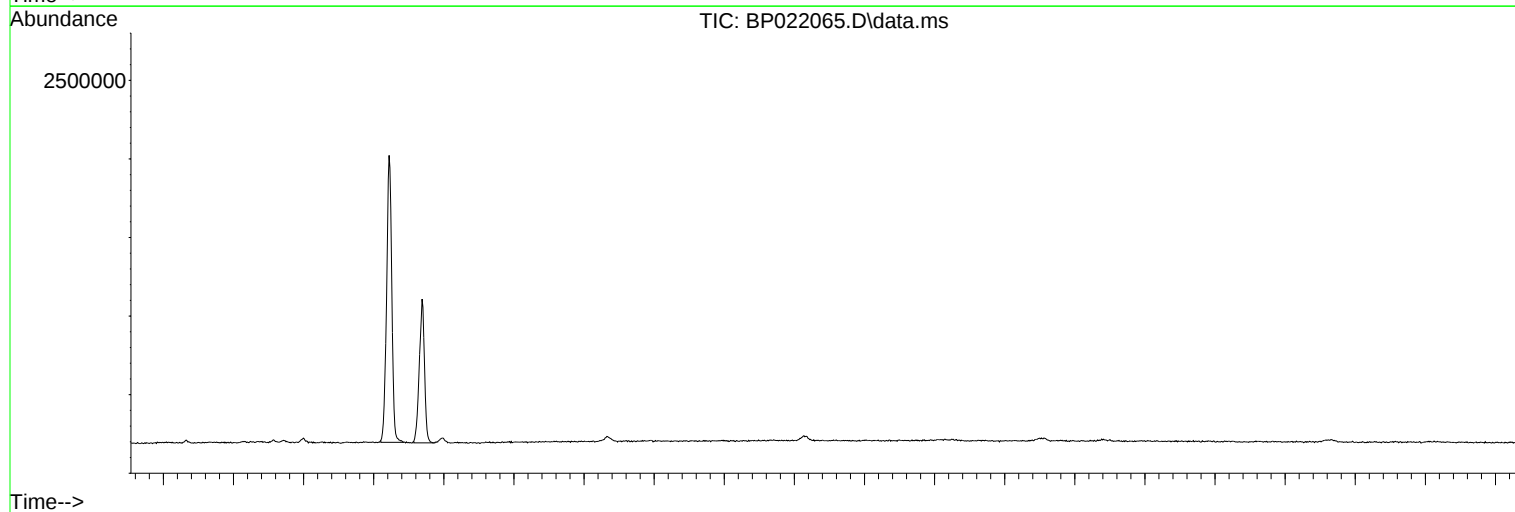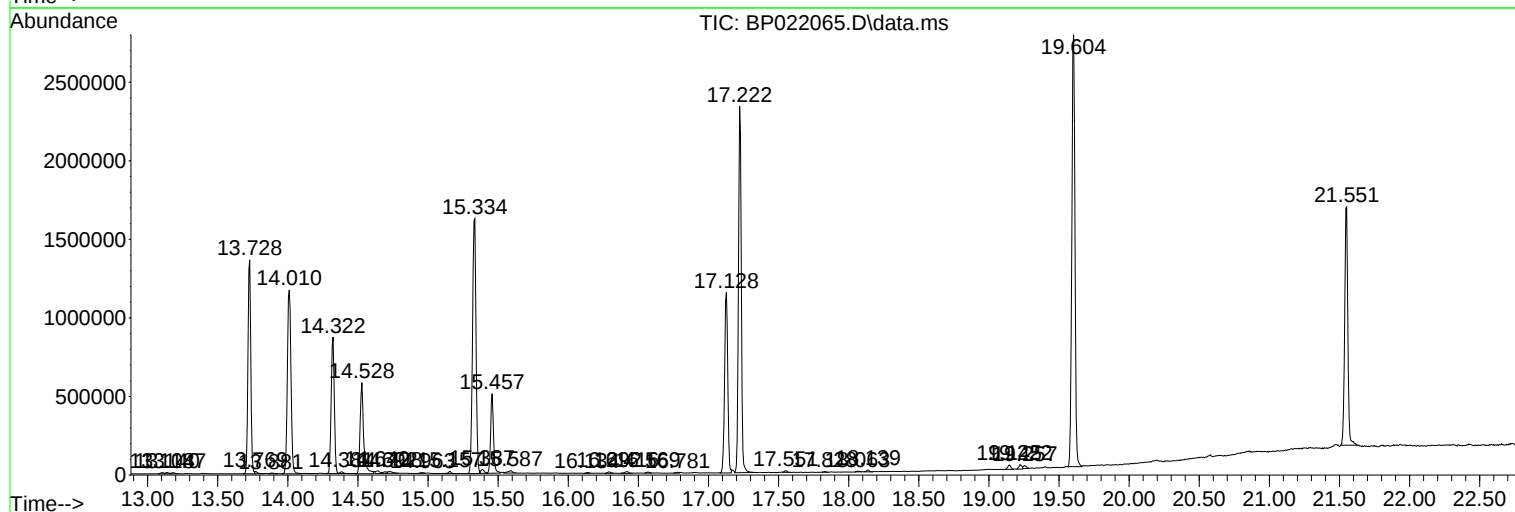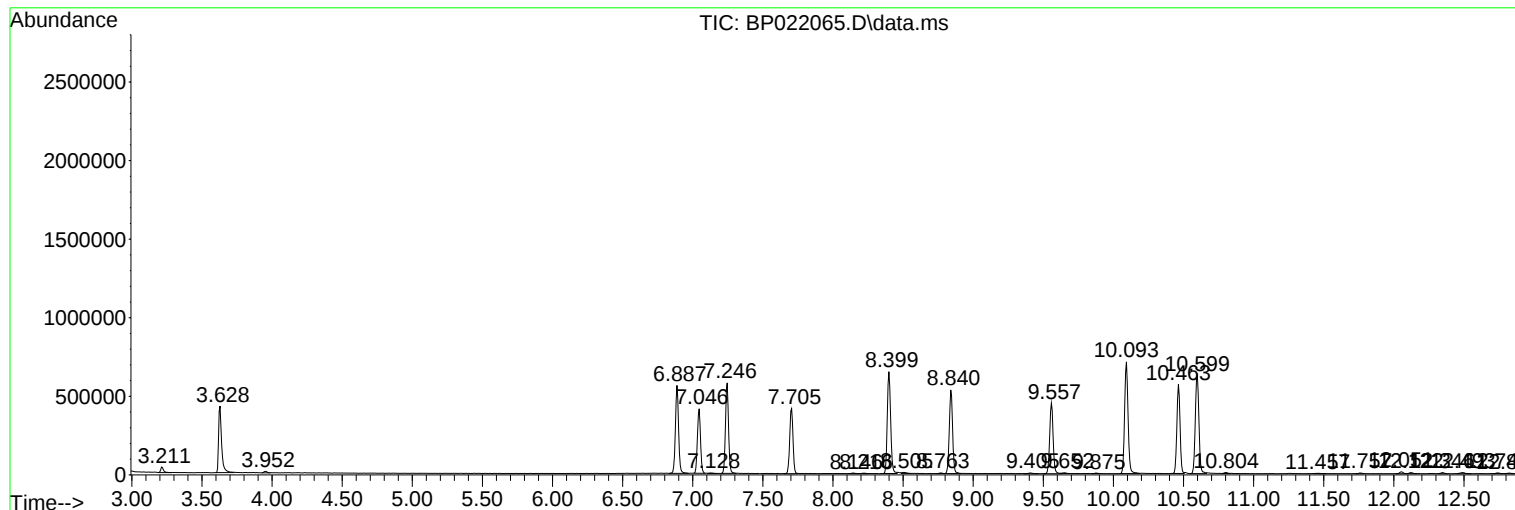

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022065.D
Acq On : 26 Sep 2024 16:32
Operator : RC/JU
Sample : PB163588BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022065.D
Acq On : 26 Sep 2024 16:32
Operator : RC/JU
Sample : PB163588BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------