

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022068.D
 Acq On : 26 Sep 2024 18:35
 Operator : RC/JU
 Sample : P4013-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	35	40	53	rVB	37869	58592	0.99%	0.120%
2	3.634	106	110	122	rBV	98342	161250	2.74%	0.331%
3	3.958	161	165	170	rBV3	8037	11798	0.20%	0.024%
4	4.399	236	240	244	rVB4	4691	8182	0.14%	0.017%
5	6.728	630	636	639	rBV7	3577	7350	0.12%	0.015%
6	6.887	652	663	676	rBV	215048	365832	6.21%	0.751%
7	7.040	683	689	699	rVB	527449	834595	14.16%	1.713%
8	7.246	715	724	734	rBV	695532	1074802	18.23%	2.206%
9	7.705	792	802	812	rBV	609157	976809	16.57%	2.005%
10	8.140	870	876	882	rBV9	4444	8439	0.14%	0.017%
11	8.399	911	920	929	rBV	588071	943404	16.00%	1.936%
12	8.510	935	939	945	rVB5	7460	13985	0.24%	0.029%
13	8.763	975	982	988	rBV5	4848	9110	0.15%	0.019%
14	8.840	988	995	1010	rVV	722808	1152088	19.54%	2.365%
15	9.410	1085	1092	1099	rBV2	5152	10340	0.18%	0.021%
16	9.557	1110	1117	1128	rBV	611045	1018976	17.29%	2.091%
17	9.646	1128	1132	1139	rVB7	5845	10152	0.17%	0.021%
18	10.093	1197	1208	1224	rBV	962079	1614421	27.39%	3.313%
19	10.463	1261	1271	1278	rBV	796203	1331134	22.58%	2.732%
20	10.604	1288	1295	1308	rVB	52954	114665	1.95%	0.235%
21	10.799	1321	1328	1334	rVB9	7300	13139	0.22%	0.027%
22	11.257	1400	1406	1413	rBV8	7339	13839	0.23%	0.028%
23	11.410	1425	1432	1436	rBV8	4047	6914	0.12%	0.014%
24	11.751	1486	1490	1496	rVB8	4142	8391	0.14%	0.017%
25	12.046	1534	1540	1546	rBV2	14069	24662	0.42%	0.051%
26	12.122	1548	1553	1561	rBV2	8776	15210	0.26%	0.031%
27	12.340	1585	1590	1596	rVB2	9086	15346	0.26%	0.031%
28	12.493	1610	1616	1622	rVB6	8703	17019	0.29%	0.035%
29	12.734	1652	1657	1665	rVB10	5701	9974	0.17%	0.020%
30	12.816	1667	1671	1677	rVV7	5100	8585	0.15%	0.018%
31	13.098	1712	1719	1722	rBV4	9291	15487	0.26%	0.032%
32	13.140	1722	1726	1729	rVV2	11045	18278	0.31%	0.038%
33	13.181	1729	1733	1739	rVB3	8995	15057	0.26%	0.031%
34	13.387	1761	1768	1777	rBV3	3194	6653	0.11%	0.014%
35	13.716	1817	1824	1829	rBV	1899684	2557090	43.38%	5.248%
36	13.751	1829	1830	1837	rVB2	13925	17764	0.30%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
 Data File : BP022068.D
 Acq On : 26 Sep 2024 18:35
 Operator : RC/JU
 Sample : P4013-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	13.887	1849	1853	1859	rVB9	4240	6832	0.12%	0.014%
38	14.004	1864	1873	1883	rBV2	1507316	2399896	40.71%	4.925%
39	14.316	1919	1926	1933	rVV	1420840	2065998	35.05%	4.240%
40	14.375	1933	1936	1945	rVB2	12872	21912	0.37%	0.045%
41	14.534	1956	1963	1977	rBV	179279	379329	6.43%	0.779%
42	14.640	1979	1981	1985	rVV5	16102	25963	0.44%	0.053%
43	14.687	1985	1989	1991	rVV4	10707	17423	0.30%	0.036%
44	14.740	1991	1998	2010	rVB2	34626	73938	1.25%	0.152%
45	14.957	2029	2035	2039	rBV6	7164	12340	0.21%	0.025%
46	15.145	2059	2067	2072	rBV3	13405	26749	0.45%	0.055%
47	15.322	2090	2097	2103	rBV	2457833	3697892	62.73%	7.589%
48	15.375	2103	2106	2111	rVV2	33009	42954	0.73%	0.088%
49	15.439	2111	2117	2128	rVV	790341	1100721	18.67%	2.259%
50	15.563	2134	2138	2141	rBV4	11381	18243	0.31%	0.037%
51	15.598	2141	2144	2149	rVB	15382	19689	0.33%	0.040%
52	16.034	2213	2218	2225	rBV	20798	34662	0.59%	0.071%
53	16.287	2257	2261	2265	rVB4	9807	14033	0.24%	0.029%
54	16.398	2276	2280	2288	rVB2	15463	20827	0.35%	0.043%
55	16.569	2305	2309	2314	rVB4	9156	11076	0.19%	0.023%
56	16.769	2336	2343	2350	rBV4	8157	21806	0.37%	0.045%
57	16.892	2359	2364	2367	rVB3	4334	7303	0.12%	0.015%
58	17.110	2394	2401	2411	rBV	1957493	2793221	47.38%	5.733%
59	17.216	2411	2419	2432	rVB	2668080	4308821	73.09%	8.843%
60	17.410	2450	2452	2459	rVB4	4810	7241	0.12%	0.015%
61	17.522	2467	2471	2478	rVB2	13018	18821	0.32%	0.039%
62	17.804	2516	2519	2526	rVB8	12731	20988	0.36%	0.043%
63	18.045	2556	2560	2567	rBV3	32679	47323	0.80%	0.097%
64	18.122	2569	2573	2577	rVV	26005	33880	0.57%	0.070%
65	18.539	2642	2644	2649	rVB6	8222	10908	0.19%	0.022%
66	19.145	2742	2747	2751	rBV2	35734	55656	0.94%	0.114%
67	19.216	2754	2759	2762	rBV	46631	67868	1.15%	0.139%
68	19.245	2762	2764	2769	rVB2	23863	29386	0.50%	0.060%
69	19.380	2783	2787	2794	rBV7	23025	30298	0.51%	0.062%
70	19.592	2817	2823	2834	rBV	4051574	5555650	94.24%	11.402%
71	21.545	3149	3155	3162	rBV	2380086	3563692	60.45%	7.314%
72	24.610	3666	3676	3694	rVB	2248734	5894936	100.00%	12.099%
73	24.833	3704	3714	3726	rVB	1422965	3776771	64.07%	7.751%

Sum of corrected areas: 48724378




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022068.D
Acq On : 26 Sep 2024 18:35
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

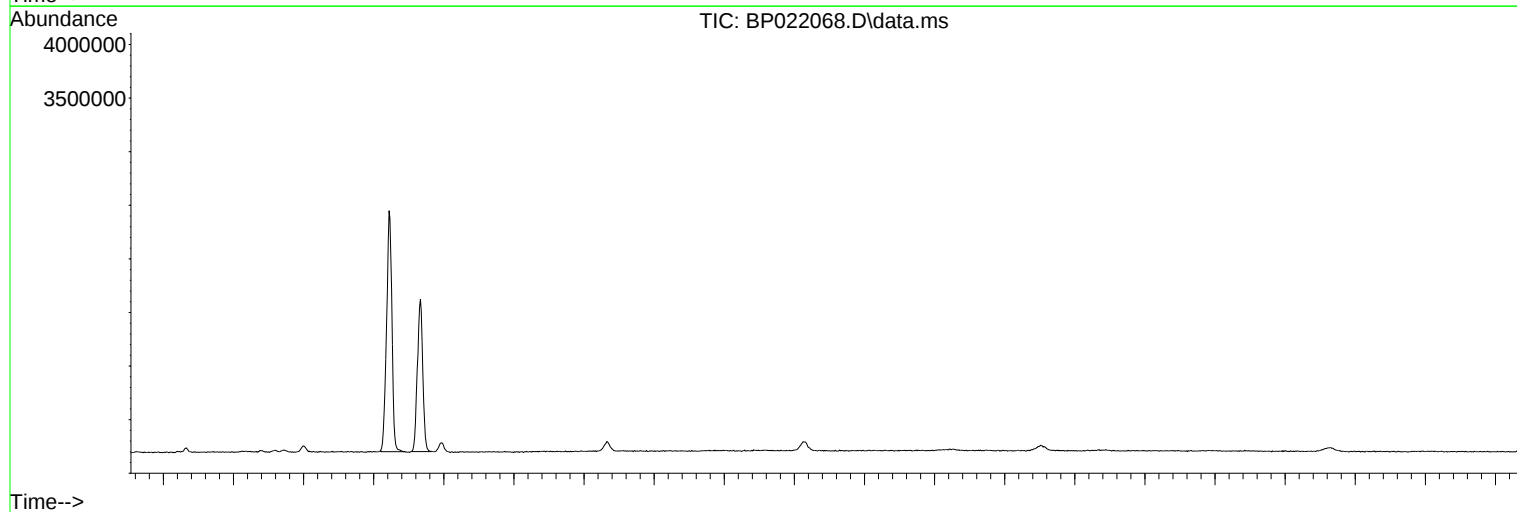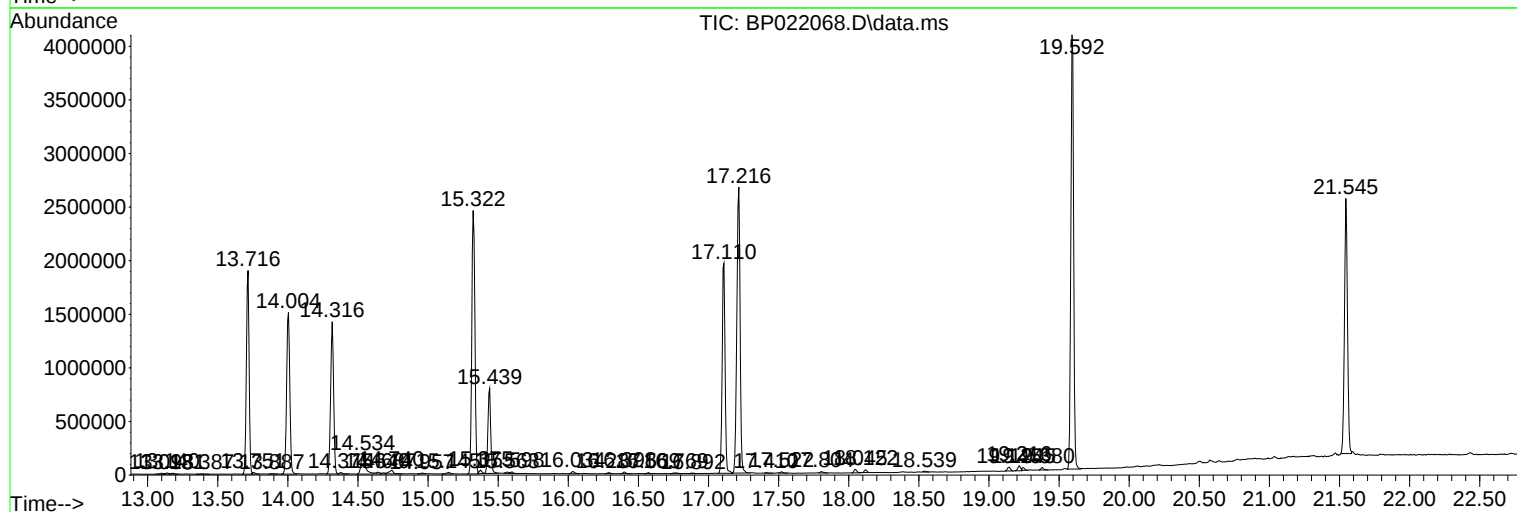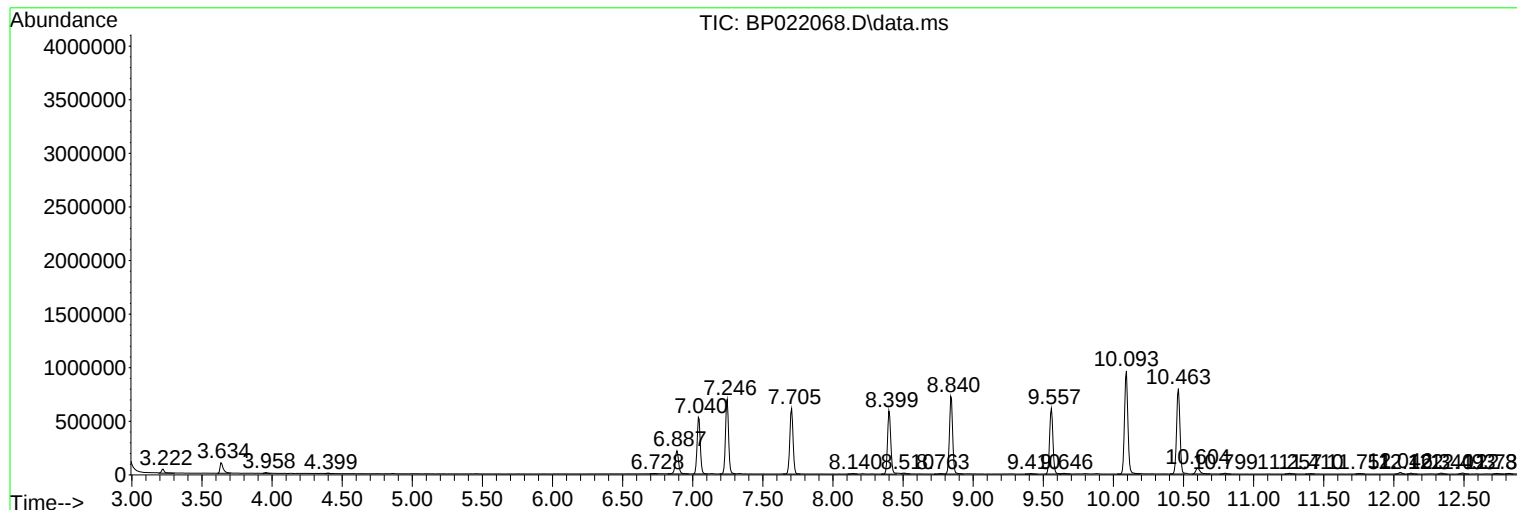

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022068.D
Acq On : 26 Sep 2024 18:35
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092424\
Data File : BP022068.D
Acq On : 26 Sep 2024 18:35
Operator : RC/JU
Sample : P4013-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
